

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028059.D
 Acq On : 22 Sep 2022 12:42
 Operator : SY/MD
 Sample : N4674-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV028059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	227050	233358	15.00%	2.010%
2	1.561	155	162	174	rBV	182602	206013	13.24%	1.774%
3	2.098	320	329	356	rVB	402005	593692	38.16%	5.113%
4	2.497	448	453	466	rVB4	4570	7846	0.50%	0.068%
5	2.635	494	496	499	rVB	682	408	0.03%	0.004%
6	2.670	499	507	509	rBV3	393	427	0.03%	0.004%
7	2.764	532	536	542	rVV3	610	496	0.03%	0.004%
8	2.847	560	562	567	rVB3	434	304	0.02%	0.003%
9	2.947	591	593	597	rVB3	504	325	0.02%	0.003%
10	2.976	597	602	603	rBV	406	347	0.02%	0.003%
11	3.027	616	618	621	rBV2	439	309	0.02%	0.003%
12	3.082	633	635	637	rVV3	565	301	0.02%	0.003%
13	3.162	657	660	663	rBV3	487	355	0.02%	0.003%
14	3.198	669	671	673	rVB	851	330	0.02%	0.003%
15	3.236	680	683	686	rVB3	416	286	0.02%	0.002%
16	3.256	686	689	691	rBV2	580	388	0.02%	0.003%
17	3.297	700	702	705	rVB2	634	344	0.02%	0.003%
18	3.320	705	709	711	rBV	766	504	0.03%	0.004%
19	3.342	711	716	718	rBV	918	609	0.04%	0.005%
20	3.397	728	733	734	rBV2	507	355	0.02%	0.003%
21	3.448	745	749	751	rBV2	678	639	0.04%	0.006%
22	3.584	789	791	795	rBV2	767	506	0.03%	0.004%
23	3.674	813	819	825	rBV3	765	879	0.06%	0.008%
24	3.825	862	866	871	rBV2	473	535	0.03%	0.005%
25	3.879	873	883	917	rBV	126786	378422	24.32%	3.259%
26	4.339	1011	1026	1048	rBV	253150	613449	39.43%	5.283%
27	4.603	1104	1108	1110	rVB2	815	478	0.03%	0.004%
28	4.651	1119	1123	1131	rVV8	869	899	0.06%	0.008%
29	4.805	1168	1171	1173	rBV2	540	368	0.02%	0.003%
30	4.841	1179	1182	1187	rBV3	863	941	0.06%	0.008%
31	4.940	1212	1213	1218	rBV4	358	293	0.02%	0.003%
32	5.037	1226	1243	1270	rBV2	611770	1555858	100.00%	13.400%
33	5.336	1333	1336	1338	rBV2	712	432	0.03%	0.004%
34	5.394	1351	1354	1356	rBV3	924	669	0.04%	0.006%
35	5.529	1394	1396	1399	rBV3	1387	854	0.05%	0.007%
36	5.609	1408	1421	1444	rBV	416697	858467	55.18%	7.394%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028059.D
 Acq On : 22 Sep 2022 12:42
 Operator : SY/MD
 Sample : N4674-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.902	1503	1512	1529	rVB6	6973	16662	1.07%	0.144%
38	6.063	1547	1562	1587	rBV	346267	715010	45.96%	6.158%
39	6.255	1620	1622	1623	rBV	1087	426	0.03%	0.004%
40	6.323	1641	1643	1651	rVB4	704	610	0.04%	0.005%
41	6.378	1658	1660	1663	rBV3	743	399	0.03%	0.003%
42	6.416	1668	1672	1673	rBV3	716	422	0.03%	0.004%
43	6.526	1703	1706	1708	rBV3	803	525	0.03%	0.005%
44	6.635	1737	1740	1741	rBV2	632	329	0.02%	0.003%
45	6.699	1756	1760	1763	rVB4	562	410	0.03%	0.004%
46	6.760	1776	1779	1780	rBV	797	344	0.02%	0.003%
47	6.812	1790	1795	1799	rBV5	747	638	0.04%	0.005%
48	6.828	1799	1800	1804	rBV3	723	412	0.03%	0.004%
49	6.882	1814	1817	1819	rBV2	731	306	0.02%	0.003%
50	6.979	1837	1847	1872	rVV	180619	333036	21.41%	2.868%
51	7.236	1925	1927	1935	rVB5	688	451	0.03%	0.004%
52	7.310	1938	1950	1973	rBV	681538	1193137	76.69%	10.276%
53	7.615	2036	2045	2071	rBV	129378	231530	14.88%	1.994%
54	7.969	2153	2155	2161	rVB3	1044	667	0.04%	0.006%
55	8.085	2181	2191	2226	rBV	439221	836747	53.78%	7.207%
56	8.480	2311	2314	2315	rBV3	977	444	0.03%	0.004%
57	8.583	2343	2346	2347	rBV2	689	330	0.02%	0.003%
58	8.715	2382	2387	2389	rBV3	668	433	0.03%	0.004%
59	8.789	2408	2410	2412	rBV2	802	378	0.02%	0.003%
60	8.847	2417	2428	2451	rBV	662839	1062859	68.31%	9.154%
61	9.136	2516	2518	2521	rBV2	1031	697	0.04%	0.006%
62	9.191	2533	2535	2538	rBV2	703	341	0.02%	0.003%
63	9.342	2579	2582	2585	rBV2	814	615	0.04%	0.005%
64	9.371	2588	2591	2594	rVV3	570	442	0.03%	0.004%
65	9.406	2598	2602	2603	rBV3	579	375	0.02%	0.003%
66	9.484	2623	2626	2631	rVB5	783	627	0.04%	0.005%
67	9.522	2636	2638	2642	rBV2	624	423	0.03%	0.004%
68	9.638	2672	2674	2679	rVV2	559	373	0.02%	0.003%
69	9.696	2690	2692	2695	rBV2	499	411	0.03%	0.004%
70	9.767	2711	2714	2718	rVB2	500	359	0.02%	0.003%
71	9.940	2763	2768	2770	rVB3	752	545	0.04%	0.005%
72	10.014	2787	2791	2793	rBV	570	299	0.02%	0.003%
73	10.123	2817	2825	2834	rVB7	2938	4809	0.31%	0.041%
74	10.210	2840	2852	2871	rBV	479766	746172	47.96%	6.427%
75	10.358	2895	2898	2901	rBV2	832	649	0.04%	0.006%
76	10.416	2913	2916	2918	rBV3	470	339	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
 Data File : VV028059.D
 Acq On : 22 Sep 2022 12:42
 Operator : SY/MD
 Sample : N4674-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.545	2953	2956	2960	rBV4	850	731	0.05%	0.006%
78	10.644	2984	2987	2990	rBV2	1129	850	0.05%	0.007%
79	10.850	3048	3051	3053	rBV3	1191	758	0.05%	0.007%
80	10.911	3063	3070	3076	rBV6	2745	3891	0.25%	0.034%
81	11.027	3099	3106	3108	rBV4	1033	1152	0.07%	0.010%
82	11.078	3117	3122	3125	rBV3	537	519	0.03%	0.004%
83	11.139	3139	3141	3148	rVB3	1874	1498	0.10%	0.013%
84	11.246	3163	3174	3193	rBV	610025	939359	60.38%	8.090%
85	11.506	3253	3255	3258	rVB3	923	382	0.02%	0.003%
86	11.619	3279	3290	3310	rBV	658364	1040142	66.85%	8.958%
87	12.377	3524	3526	3530	rVB3	791	444	0.03%	0.004%
88	13.049	3733	3735	3739	rVB3	946	347	0.02%	0.003%
89	13.085	3743	3746	3753	rVB4	975	1027	0.07%	0.009%
90	13.117	3753	3756	3759	rBV3	656	542	0.03%	0.005%
91	13.242	3792	3795	3797	rBV4	671	442	0.03%	0.004%
92	13.255	3797	3799	3802	rVV3	511	311	0.02%	0.003%
93	13.628	3913	3915	3917	rBV	1025	490	0.03%	0.004%
94	13.747	3948	3952	3954	rBV2	1154	898	0.06%	0.008%
95	13.792	3964	3966	3967	rBV	706	305	0.02%	0.003%
96	13.860	3983	3987	3992	rBV4	646	702	0.05%	0.006%
97	13.882	3992	3994	3997	rBV2	645	350	0.02%	0.003%
98	13.934	4008	4010	4011	rBV	715	281	0.02%	0.002%
99	13.982	4023	4025	4026	rBV2	969	349	0.02%	0.003%
100	14.631	4225	4227	4230	rBV2	609	412	0.03%	0.004%




Sum of corrected areas: 11610849

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028059.D
Acq On : 22 Sep 2022 12:42
Operator : SY/MD
Sample : N4674-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

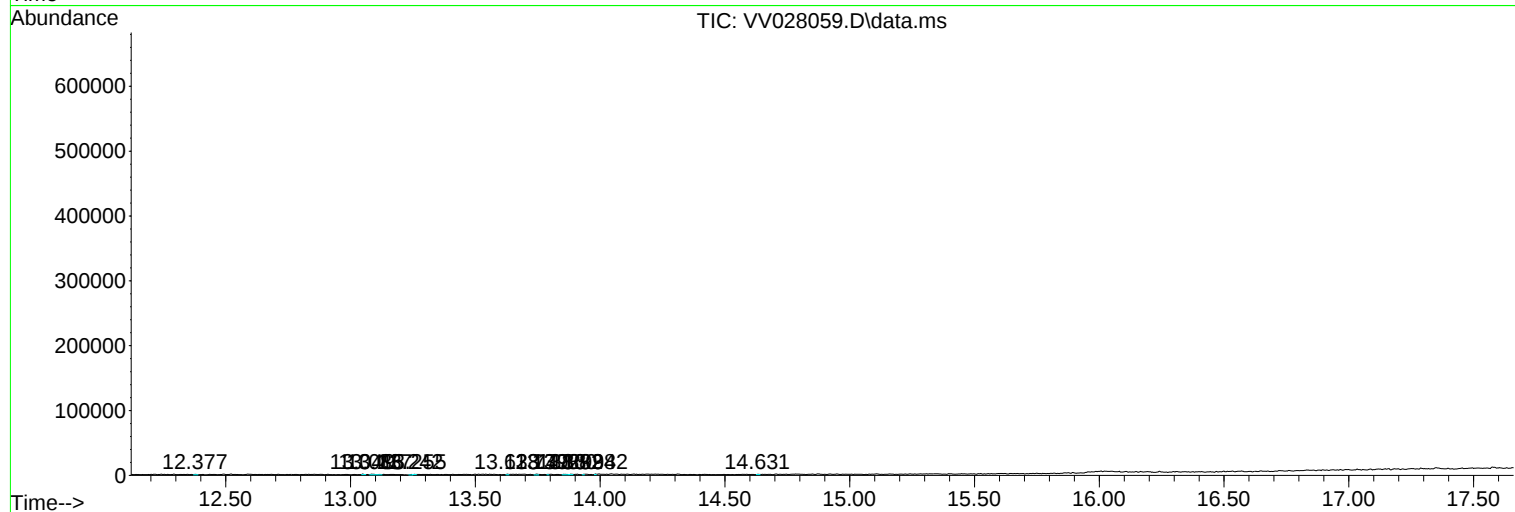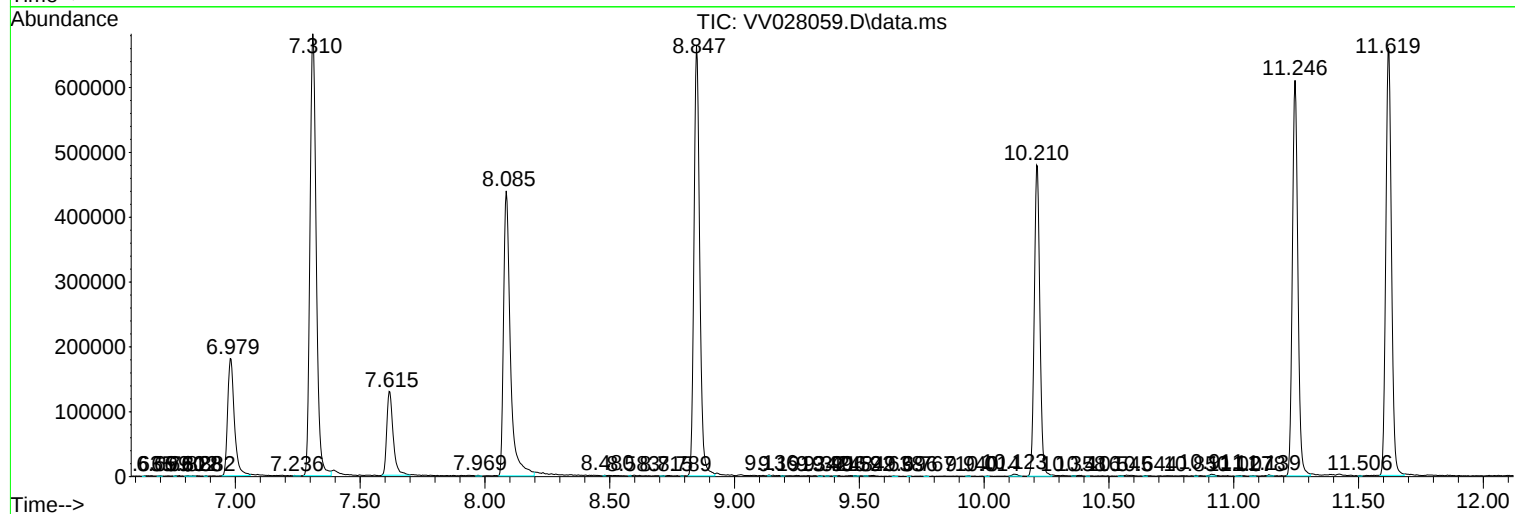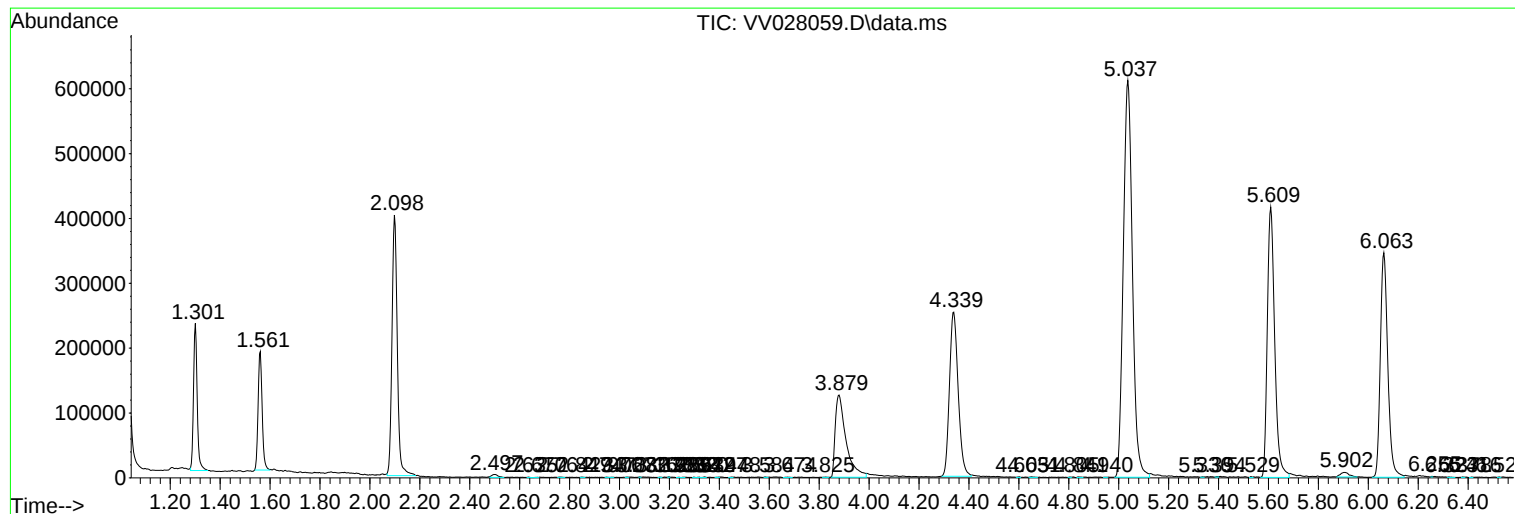

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028059.D
Acq On : 22 Sep 2022 12:42
Operator : SY/MD
Sample : N4674-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028059.D
Acq On : 22 Sep 2022 12:42
Operator : SY/MD
Sample : N4674-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 55 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------