
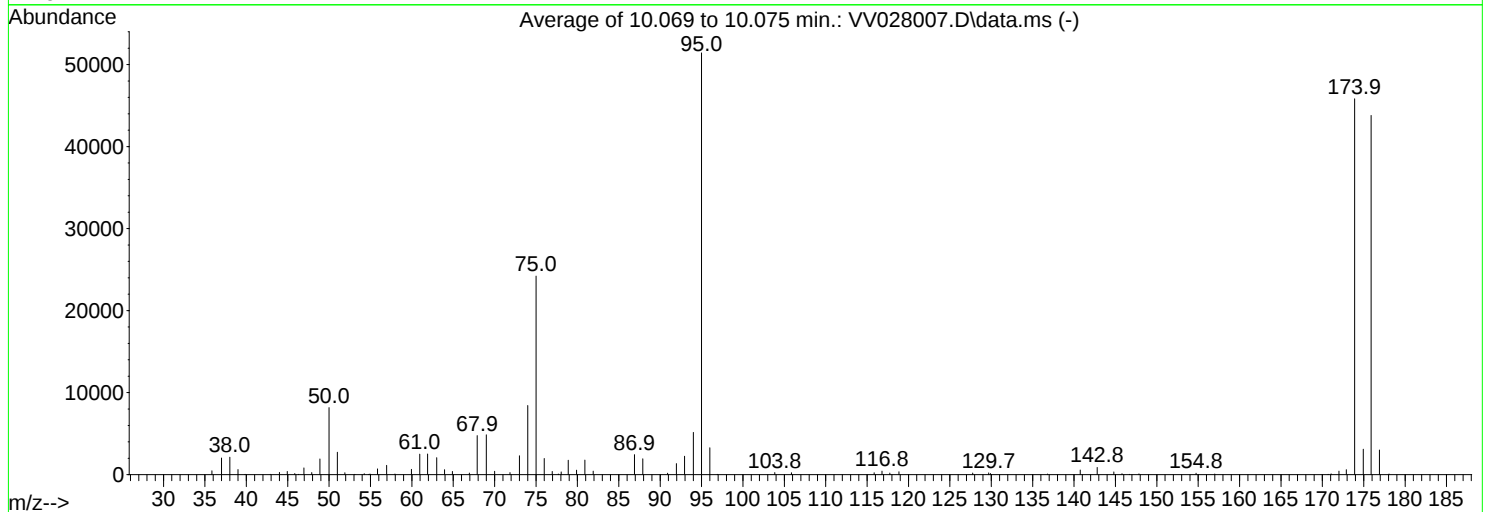


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092122\
Data File : VV028007.D
Acq On : 21 Sep 2022 10:08
Operator : SY/MD
Sample : BFB321
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB321

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Title : VOC Analysis
Last Update : Thu Sep 22 05:25:17 2022

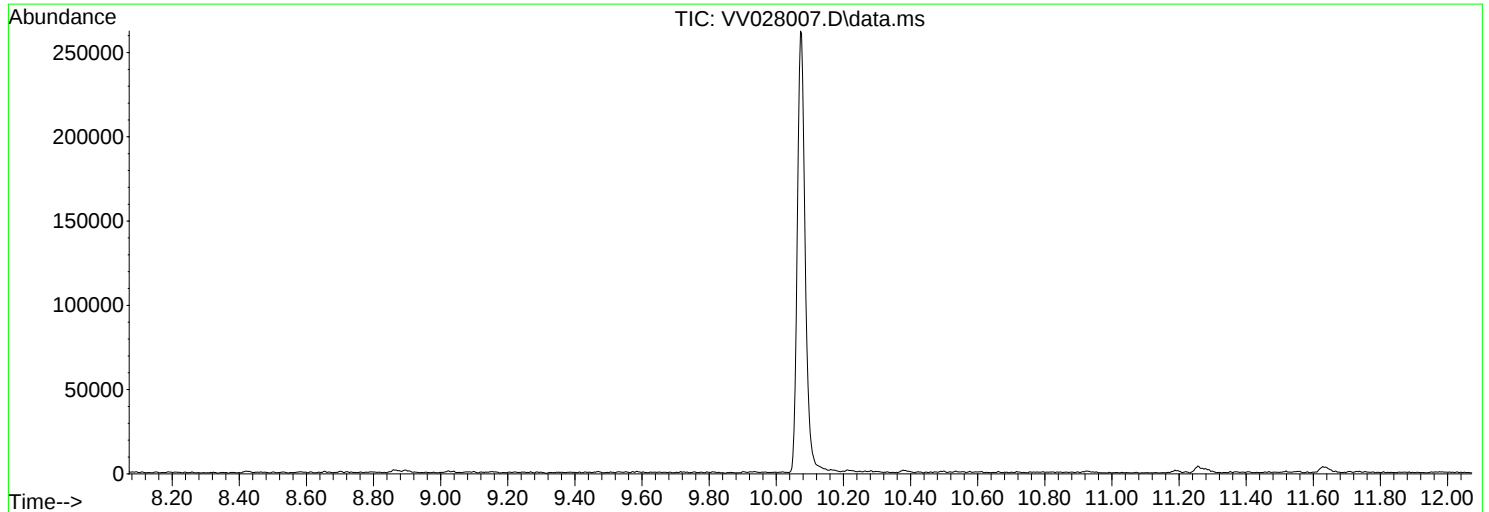

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.9	8182	PASS
75	95	30	80	47.1	24221	PASS
95	95	100	100	100.0	51435	PASS
96	95	5	9	6.4	3274	PASS
173	174	0.00	2	1.3	608	PASS
174	95	50	120	89.1	45840	PASS
175	174	5	9	6.8	3106	PASS
176	174	95	105	95.6	43808	PASS
177	176	5	10	6.9	3004	PASS

m/z	Abundance
39.00	104.0
39.90	288.0
44.00	380.0

Instrument :
MSVOA_V
ClientSampleId :
BFB321

m/z	Abundance
35.90	438.0
37.00	1934.0
38.00	1965.0
39.00	678.0
39.90	307.0
44.00	624.0
45.00	387.0
45.80	150.0
46.90	792.0
47.90	190.0
48.90	1825.0
50.00	7974.0
51.00	2478.0
51.90	188.0
54.20	135.0
54.80	136.0
55.80	660.0
57.00	1043.0
59.90	606.0
61.00	2434.0
61.90	2519.0
63.00	2043.0
63.90	535.0
64.90	317.0
66.90	177.0
67.90	4689.0
69.00	4652.0
70.00	387.0
71.80	215.0
73.00	2208.0
74.00	8087.0
75.00	22960.0
76.00	1906.0
77.00	467.0
77.70	231.0
78.10	312.0
78.90	1596.0
79.90	557.0
80.90	1773.0
81.90	400.0
86.90	2490.0
87.90	1906.0
90.90	155.0
92.00	1180.0
92.90	2089.0
94.00	4833.0
95.00	48480.0
96.00	3206.0
96.90	115.0
103.90	247.0
105.80	212.0
115.90	198.0
116.80	414.0
117.70	146.0
118.80	328.0
127.80	236.0
129.70	225.0
140.80	518.0
142.80	768.0
144.80	307.0
145.80	117.0
146.70	105.0
147.80	166.0
154.70	176.0
171.10	161.0
172.10	414.0
172.90	628.0
173.90	41632.0
174.90	3012.0
175.90	40464.0
176.90	2905.0
178.10	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB321

m/z	Abundance
35.80	494.0
37.00	2114.0
38.00	2193.0
39.00	743.0
39.90	340.0
44.00	664.0
45.00	361.0
45.80	138.0
46.90	889.0
47.90	250.0
48.90	1966.0
50.00	8408.0
51.00	2869.0
51.90	241.0
54.20	120.0
55.00	123.0
55.90	722.0
56.90	1171.0
57.90	107.0
60.00	685.0
60.90	2577.0
61.90	2631.0
63.00	2174.0
63.90	610.0
64.90	387.0
67.00	200.0
67.90	4851.0
69.00	4984.0
70.00	403.0
71.90	255.0
73.00	2368.0
74.00	8791.0
75.00	25000.0
76.00	1998.0
77.00	395.0
78.10	342.0
78.90	1799.0
79.90	557.0
80.90	1861.0
81.90	426.0
86.90	2516.0
87.90	1944.0
90.90	182.0
91.90	1381.0
92.90	2324.0
94.00	5181.0
95.00	53344.0
96.00	3343.0
103.80	264.0
105.90	259.0
115.80	236.0
116.80	445.0
117.80	209.0
118.90	352.0
127.80	193.0
129.70	223.0
129.90	208.0
136.80	113.0
140.80	590.0
142.80	899.0
144.80	362.0
145.80	107.0
147.90	137.0
154.70	171.0
157.00	124.0
171.00	127.0
172.00	443.0
172.90	617.0
173.90	47504.0
174.90	3190.0
175.90	45376.0
176.90	3078.0
178.00	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB321

m/z	Abundance
35.80	493.0
37.00	2040.0
38.00	2199.0
39.00	768.0
39.80	349.0
42.90	123.0
44.00	654.0
44.90	408.0
45.90	127.0
46.30	111.0
47.00	773.0
47.90	313.0
48.90	1949.0
50.00	8163.0
51.00	2850.0
51.90	258.0
53.10	116.0
54.30	119.0
54.90	121.0
55.90	723.0
56.90	1207.0
58.00	125.0
60.00	637.0
60.90	2497.0
61.90	2423.0
63.00	2007.0
64.00	667.0
64.90	451.0
67.00	209.0
67.90	4774.0
69.00	4916.0
70.00	422.0
71.90	310.0
73.00	2356.0
74.00	8428.0
75.00	24704.0
76.00	2007.0
76.80	327.0
78.00	326.0
78.90	1853.0
79.90	500.0
80.90	1680.0
81.90	457.0
86.90	2314.0
87.90	1941.0
90.90	175.0
91.90	1511.0
93.00	2329.0
94.00	5440.0
95.00	52480.0
96.00	3273.0
103.80	231.0
105.90	245.0
115.80	244.0
116.80	424.0
117.80	236.0
118.90	387.0
127.70	161.0
129.70	190.0
129.90	189.0
136.80	138.0
140.70	598.0
142.80	986.0
144.80	314.0
145.80	103.0
154.80	168.0
157.00	124.0
170.70	134.0
171.90	436.0
172.90	580.0
173.90	48384.0
175.00	3117.0
175.90	45584.0
176.90	3030.0

Instrument :
MSVOA_V
ClientSampleId :
BFB321