

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037471.D
 Acq On : 23 Sep 2024 11:16
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 24 03:57:41 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	626269	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	605886	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	281666	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	252134	44.011	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.020%
7) Chloroethane-d5	1.532	69	209225	47.255	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.500%
11) 1,1-Dichloroethene-d2	2.060	65	109712	45.564	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	91.120%
21) 2-Butanone-d5	3.793	46	183187	82.573	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	82.570%
24) Chloroform-d	4.243	84	459955	51.299	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.600%
26) 1,2-Dichloroethane-d4	4.937	65	278641	49.348	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.700%
32) Benzene-d6	4.953	84	927706	50.694	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.380%
36) 1,2-Dichloropropane-d6	5.982	67	291025	50.773	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.540%
41) Toluene-d8	7.236	98	808014	48.923	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.840%
43) trans-1,3-Dichloroprop...	7.551	79	119256	44.972	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.940%
47) 2-Hexanone-d5	8.024	63	110168	70.425	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	70.430%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	325204	46.781	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	93.560%
66) 1,2-Dichlorobenzene-d4	11.554	152	299736	53.133	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.260%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3282	0.757	ug/L	Qvalue # 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
Data File : VV037471.D
Acq On : 23 Sep 2024 11:16
Operator : SY/MD
Sample : VIBLK
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 24 03:57:41 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:56:17 2024
Response via : Initial Calibration

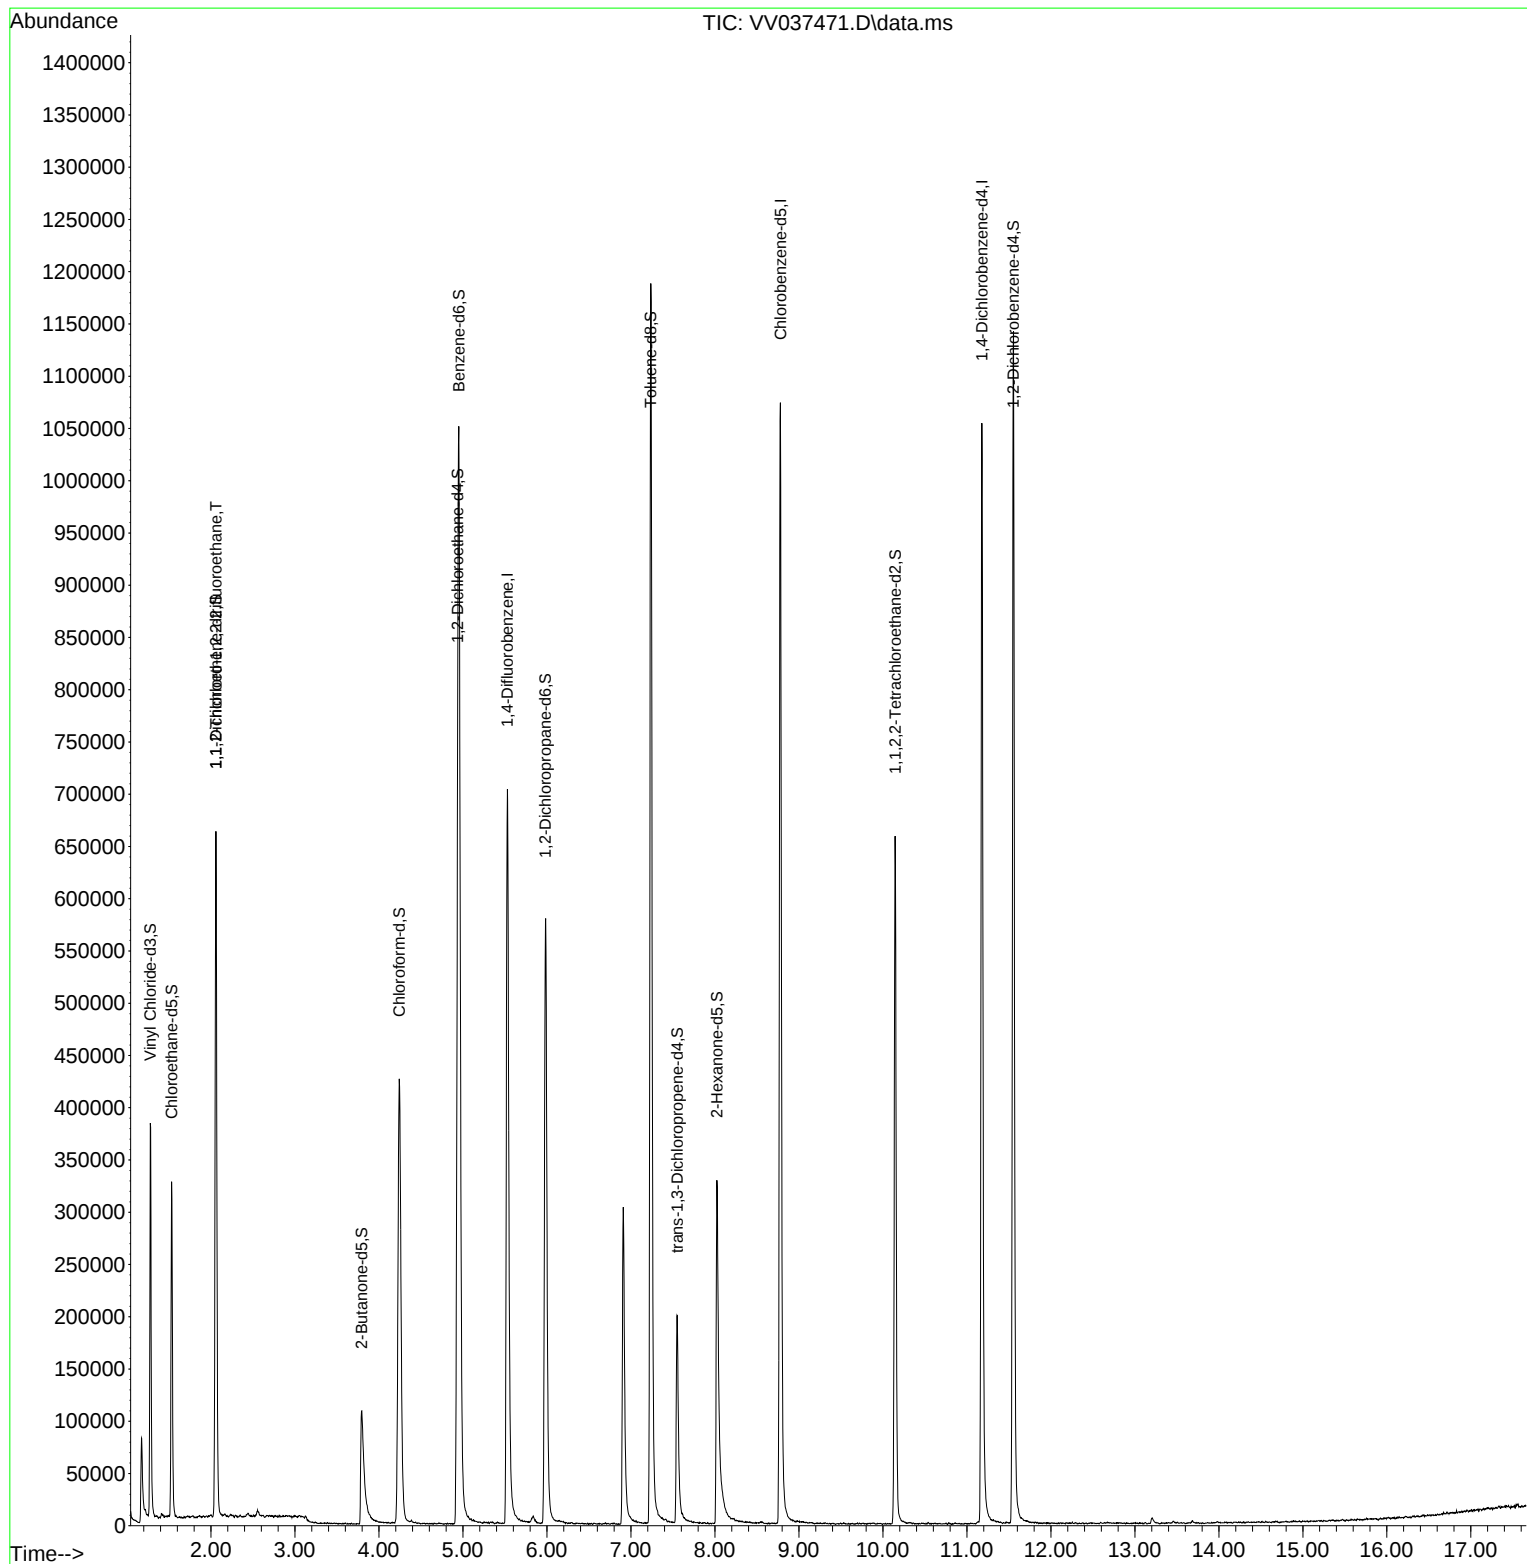

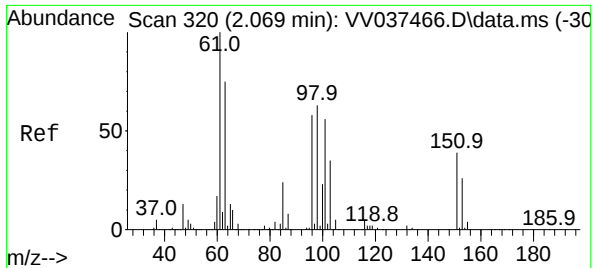

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.757 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV037471.D
 Acq: 23 Sep 2024 11:16

Instrument :
 MSVOA_V
 ClientSampleId :

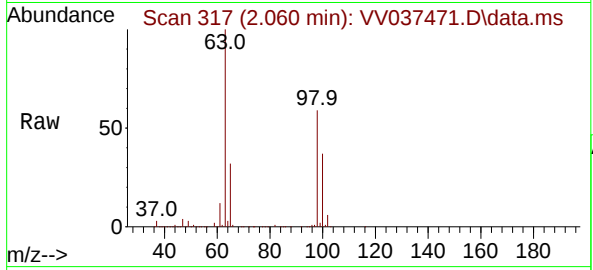

Tgt Ion:	101	Resp:	3282
Ion	Ratio	Lower	Upper
101	100		
85	1.6	35.6	53.4#
151	0.0	55.0	82.4#

