

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037485.D
 Acq On : 23 Sep 2024 16:16
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 24 04:00:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	860878	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	807079	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	416352	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	296550	37.657	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.320%		
7) Chloroethane-d5	1.532	69	242062	39.772	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	79.540%		
11) 1,1-Dichloroethene-d2	2.059	65	130453	39.413	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	78.820%		
21) 2-Butanone-d5	3.793	46	268997	88.208	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.210%		
24) Chloroform-d	4.243	84	572816	46.476	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.960%		
26) 1,2-Dichloroethane-d4	4.937	65	352979	45.477	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.960%		
32) Benzene-d6	4.953	84	1158155	47.510	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.020%		
36) 1,2-Dichloropropane-d6	5.982	67	366696	48.027	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.060%		
41) Toluene-d8	7.236	98	1040634	47.301	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.600%		
43) trans-1,3-Dichloroprop...	7.548	79	166938	47.260	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.520%		
47) 2-Hexanone-d5	8.024	63	202276	97.072	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	97.070%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	419335	45.284	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.560%		
66) 1,2-Dichlorobenzene-d4	11.554	152	400830	48.069	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.140%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.059	101	4195	0.704	ug/L	# 27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
Data File : VV037485.D
Acq On : 23 Sep 2024 16:16
Operator : SY/MD
Sample : VIBLK
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 24 04:00:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:56:17 2024
Response via : Initial Calibration

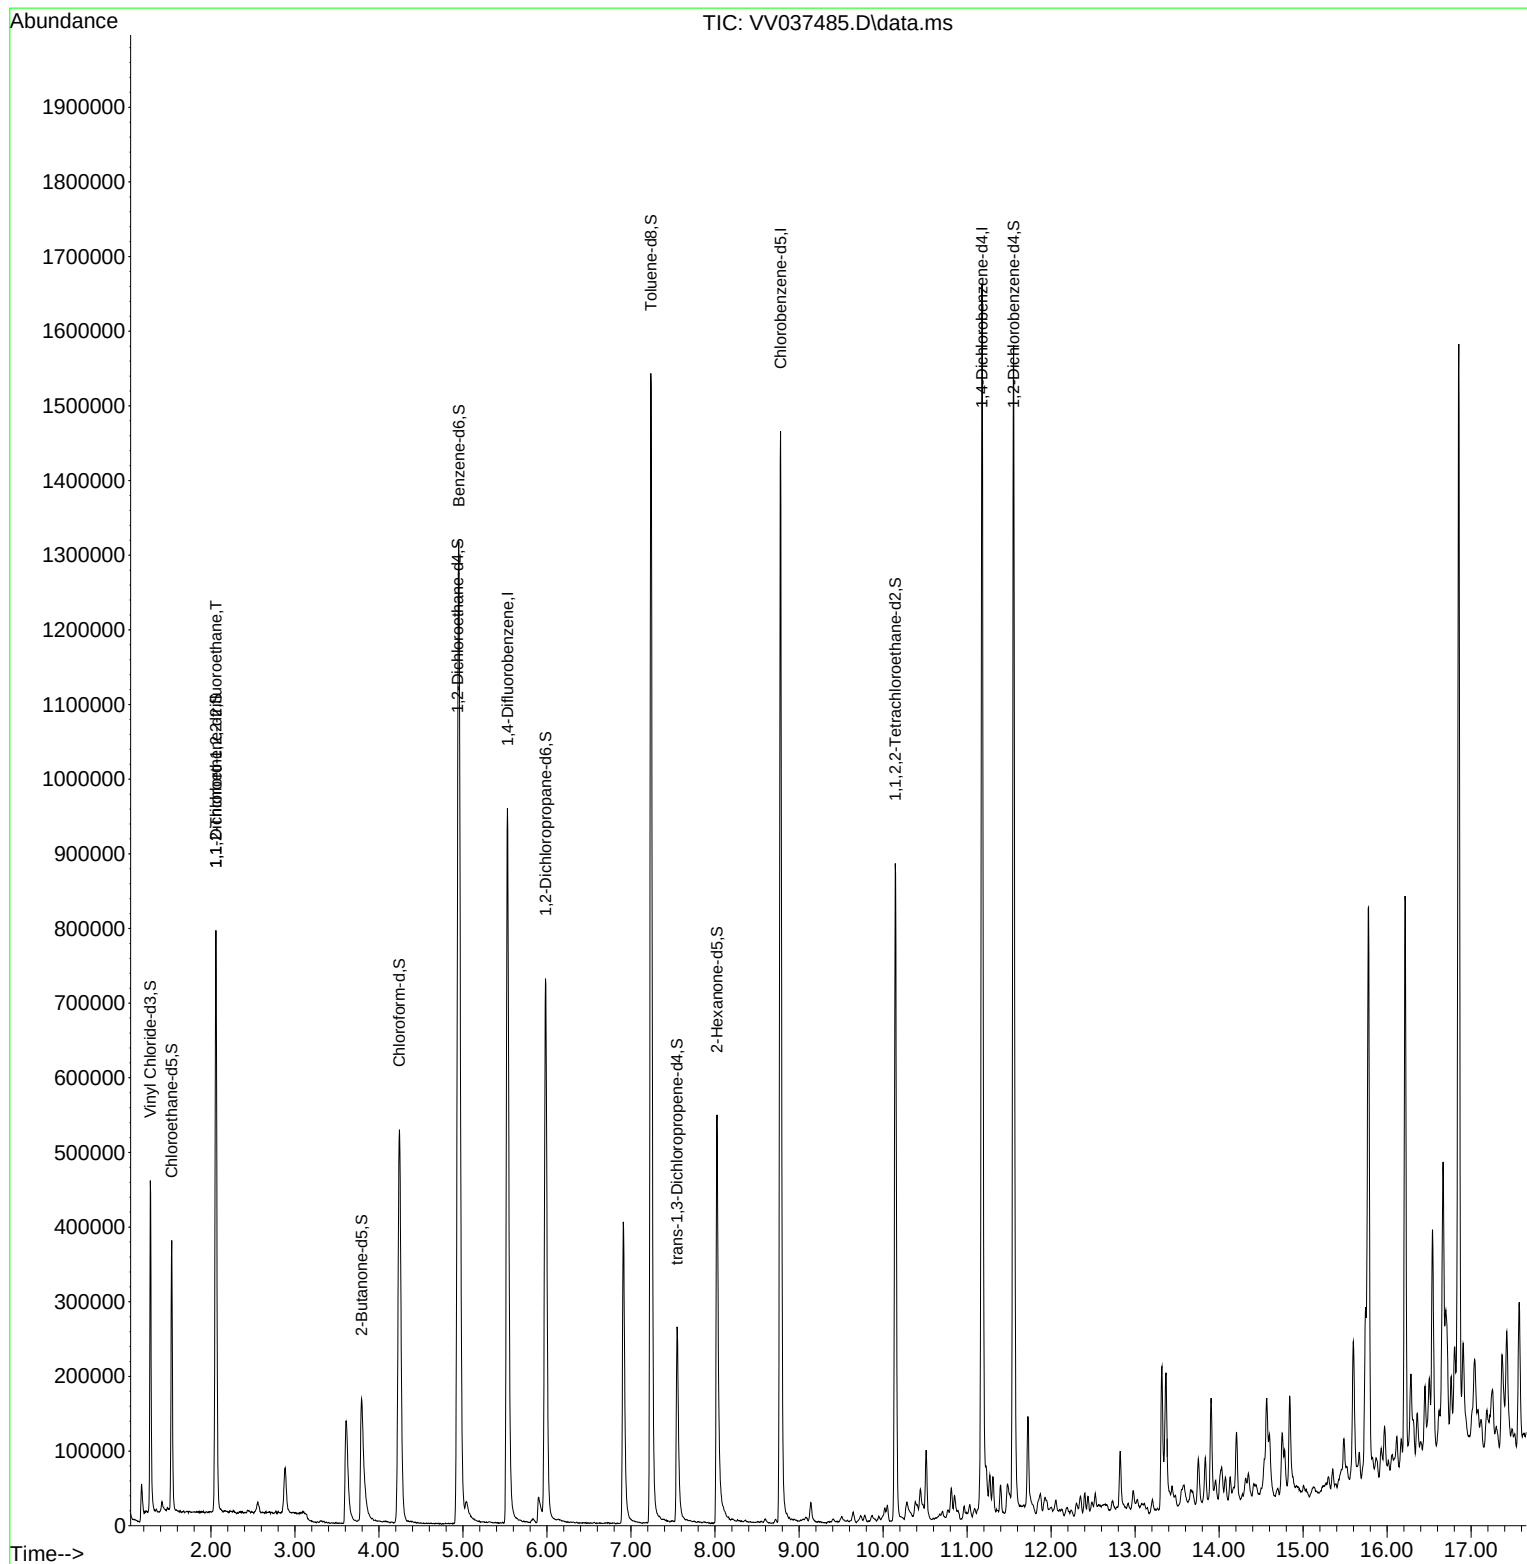

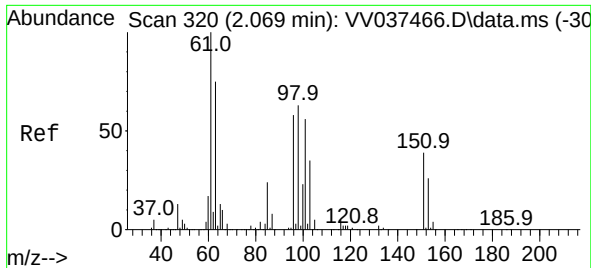

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.704 ug/L
 RT: 2.059 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV037485.D
 Acq: 23 Sep 2024 16:16

Instrument :
 MSVOA_V
 ClientSampleId :

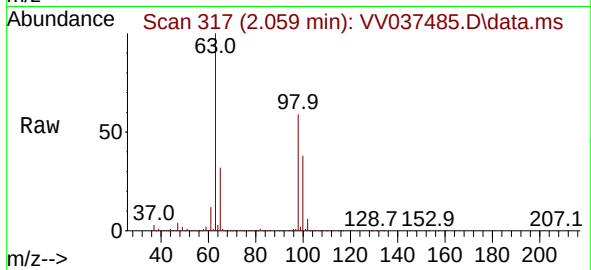

Tgt Ion:	101	Resp:	4195
Ion	Ratio	Lower	Upper
101	100		
85	6.1	35.6	53.4#
151	2.4	55.0	82.4#

