




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037476.D
 Acq On : 23 Sep 2024 13:03
 Operator : SY/MD
 Sample : P4083-01ME
 Misc : 5.36G/5mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ES1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 24 03:58:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/24/2024
 Supervised By :Mahesh Dadoda 09/24/2024

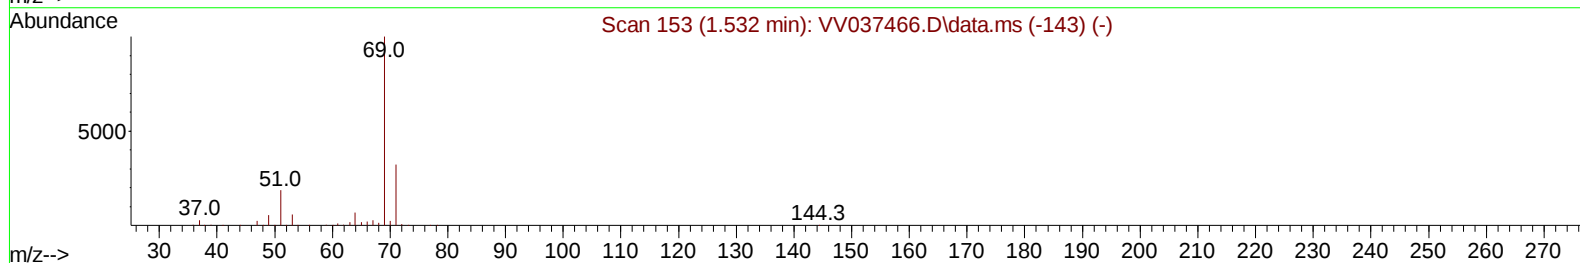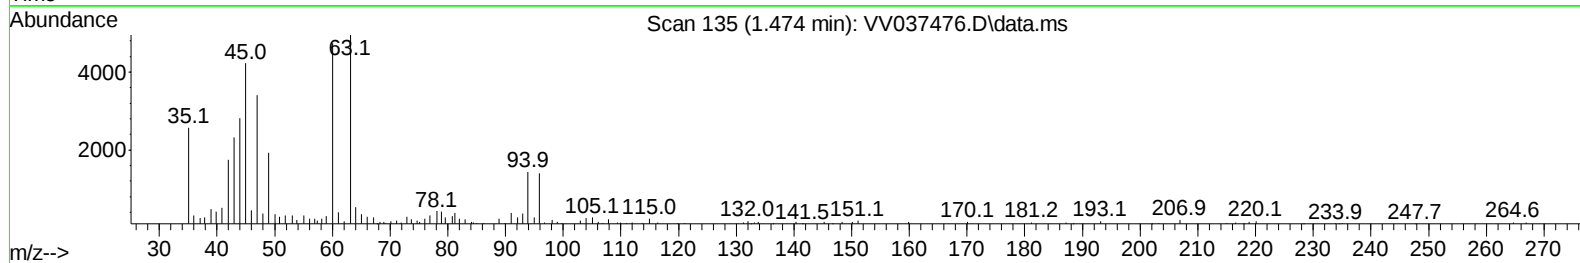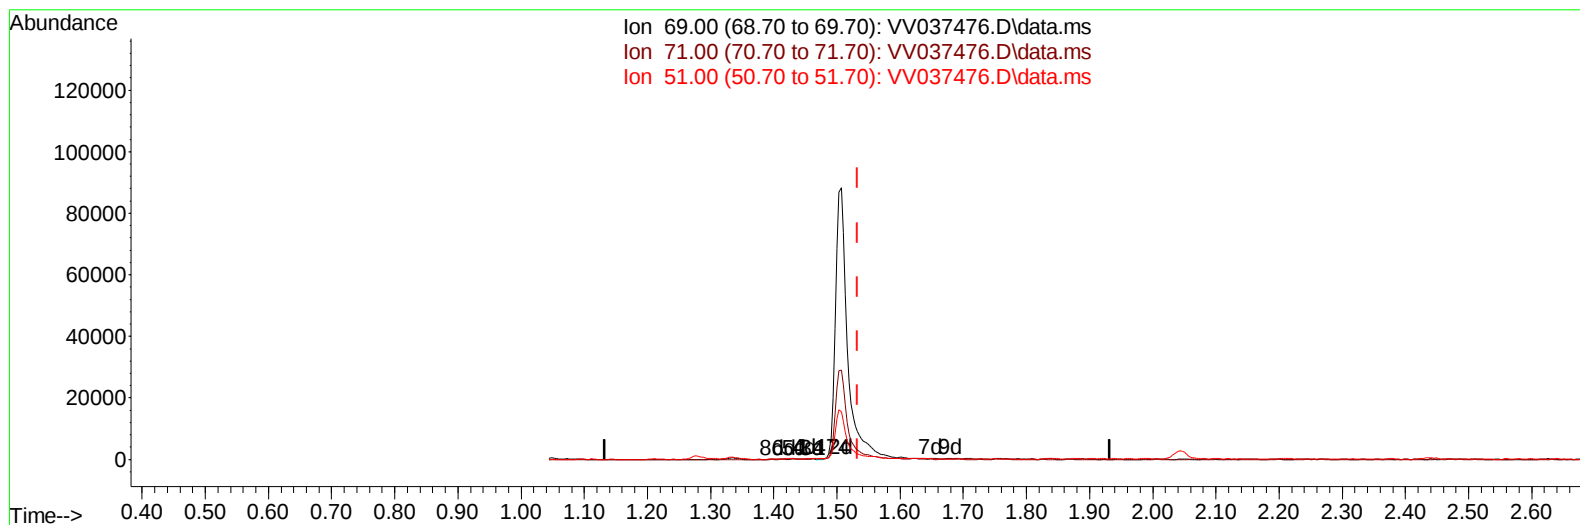

TIC: VV037476.D\data.ms

(7) Chloroethane-d5 (S)

1.474min (-0.058) 0.03 ug/L

response	133	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	30.60	27.07
51.00	25.10	24.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037476.D
 Acq On : 23 Sep 2024 13:03
 Operator : SY/MD
 Sample : P4083-01ME
 Misc : 5.36G/5mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ES1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 24 03:58:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/24/2024
 Supervised By :Mahesh Dadoda 09/24/2024

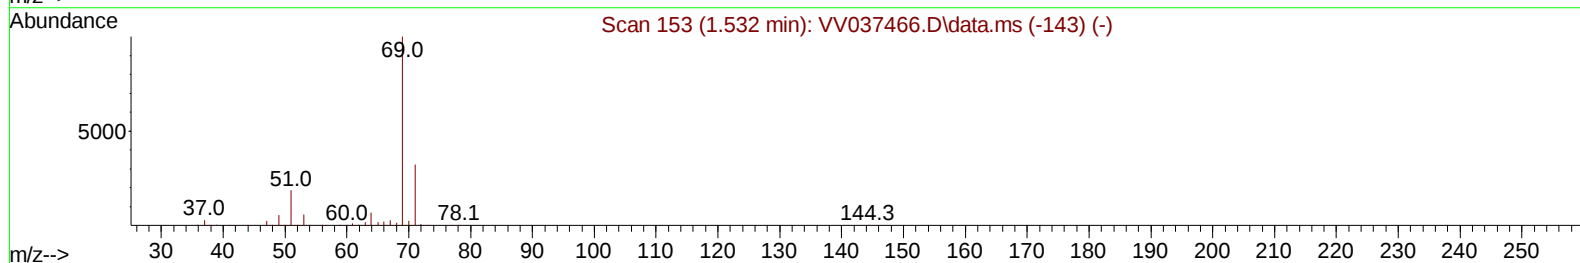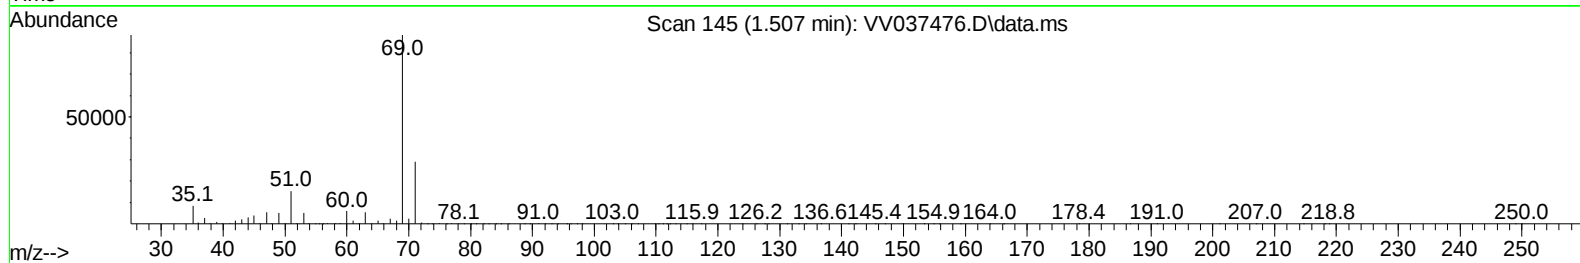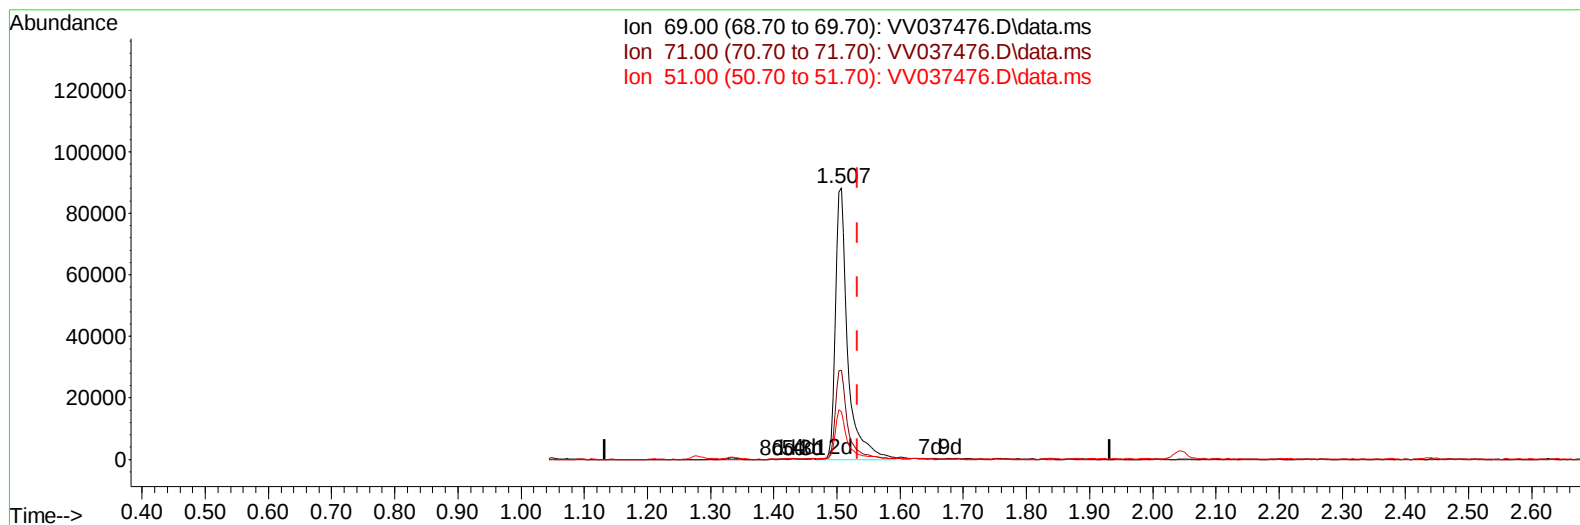

TIC: VV037476.D\data.ms

(7) Chloroethane-d5 (S)

1.507min (-0.026) 28.58 ug/L m

response 118736

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	30.60	0.03#
51.00	25.10	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037476.D
 Acq On : 23 Sep 2024 13:03
 Operator : SY/MD
 Sample : P4083-01ME
 Misc : 5.36G/5mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ES1ME

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/24/2024
 Supervised By :Mahesh Dadoda 09/24/2024

Quant Time: Sep 24 03:58:47 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.526	114		587597	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117		579871	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152		277658	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		255112	47.462	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	94.920%	
7) Chloroethane-d5	1.507	69		118736m	28.582	ug/L	-0.03
Spiked Amount 50.000	Range 70	- 130		Recovery	=	57.160%#	
11) 1,1-Dichloroethene-d2	2.043	65		116625	51.623	ug/L	-0.02
Spiked Amount 50.000	Range 60	- 125		Recovery	=	103.240%	
21) 2-Butanone-d5	3.799	46		203710	97.867	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	97.870%	
24) Chloroform-d	4.240	84		474283	56.378	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	112.760%	
26) 1,2-Dichloroethane-d4	4.934	65		293091	55.324	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	110.640%	
32) Benzene-d6	4.947	84		958016	54.699	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	109.400%	
36) 1,2-Dichloropropane-d6	5.982	67		309507	56.420	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	112.840%	
41) Toluene-d8	7.236	98		842052	53.271	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	106.540%	
43) trans-1,3-Dichloroprop...	7.548	79		132097	52.049	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	104.100%	
47) 2-Hexanone-d5	8.027	63		135144	90.267	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	90.270%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84		342547	51.486	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	102.980%	
66) 1,2-Dichlorobenzene-d4	11.554	152		323300	58.138	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	116.280%	
Target Compounds							
15) Methyl Acetate	2.371	43		29446	7.868	ug/L	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
Data File : VV037476.D
Acq On : 23 Sep 2024 13:03
Operator : SY/MD
Sample : P4083-01ME
Misc : 5.36G/5mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4ES1ME

Manual IntegrationsAPPROVED

Quant Time: Sep 24 03:58:47 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:56:17 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/24/2024
Supervised By :Mahesh Dadoda 09/24/2024

