

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
 Data File : VV037484.D
 Acq On : 23 Sep 2024 15:55
 Operator : SY/MD
 Sample : P4024-05ME 2X
 Misc : 10.12G/5mL/100ul/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DDC36ME

Quant Time: Sep 24 04:00:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 24 03:56:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	797510	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	759321	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	417138	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	277189	37.996	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.000%
7) Chloroethane-d5	1.507	69	135014	23.946	ug/L	-0.03
Spiked Amount	50.000	Range	70 - 130	Recovery	=	47.900%#
11) 1,1-Dichloroethene-d2	2.050	65	120710	39.368	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.740%
21) 2-Butanone-d5	3.793	46	258610	91.540	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.540%
24) Chloroform-d	4.240	84	524472	45.935	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.860%
26) 1,2-Dichloroethane-d4	4.934	65	330192	45.922	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.840%
32) Benzene-d6	4.950	84	1075841	46.909	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.820%
36) 1,2-Dichloropropane-d6	5.979	67	347770	48.413	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.820%
41) Toluene-d8	7.236	98	952000	45.994	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.980%
43) trans-1,3-Dichloroprop...	7.548	79	155296	46.729	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.460%
47) 2-Hexanone-d5	8.024	63	208559	106.382	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	106.380%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	491299	56.393	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	112.780%
66) 1,2-Dichlorobenzene-d4	11.554	152	412041	49.320	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.640%
Target Compounds						Qvalue
35) Methylcyclohexane	6.040	83	15016	1.598	ug/L	92
42) Toluene	7.320	91	27919	1.224	ug/L	98
46) Tetrachloroethene	7.902	164	32489	7.829	ug/L	95
52) Ethylbenzene	8.944	91	163639	6.350	ug/L	100
53) m,p-Xylene	9.066	106	307596	32.214	ug/L	100
54) o-Xylene	9.474	106	95090	10.171	ug/L	97
60) Isopropylbenzene	9.860	105	457802	16.929	ug/L	98
62) 1,3,5-Trimethylbenzene	10.468	105	2750659	124.322	ug/L	99
63) 1,2,4-Trimethylbenzene	10.844	105	5370296	243.220	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
Data File : VV037484.D
Acq On : 23 Sep 2024 15:55
Operator : SY/MD
Sample : P4024-05ME 2X
Misc : 10.12G/5mL/100ul/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DDC36ME

Quant Time: Sep 24 04:00:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 24 03:56:17 2024
Response via : Initial Calibration




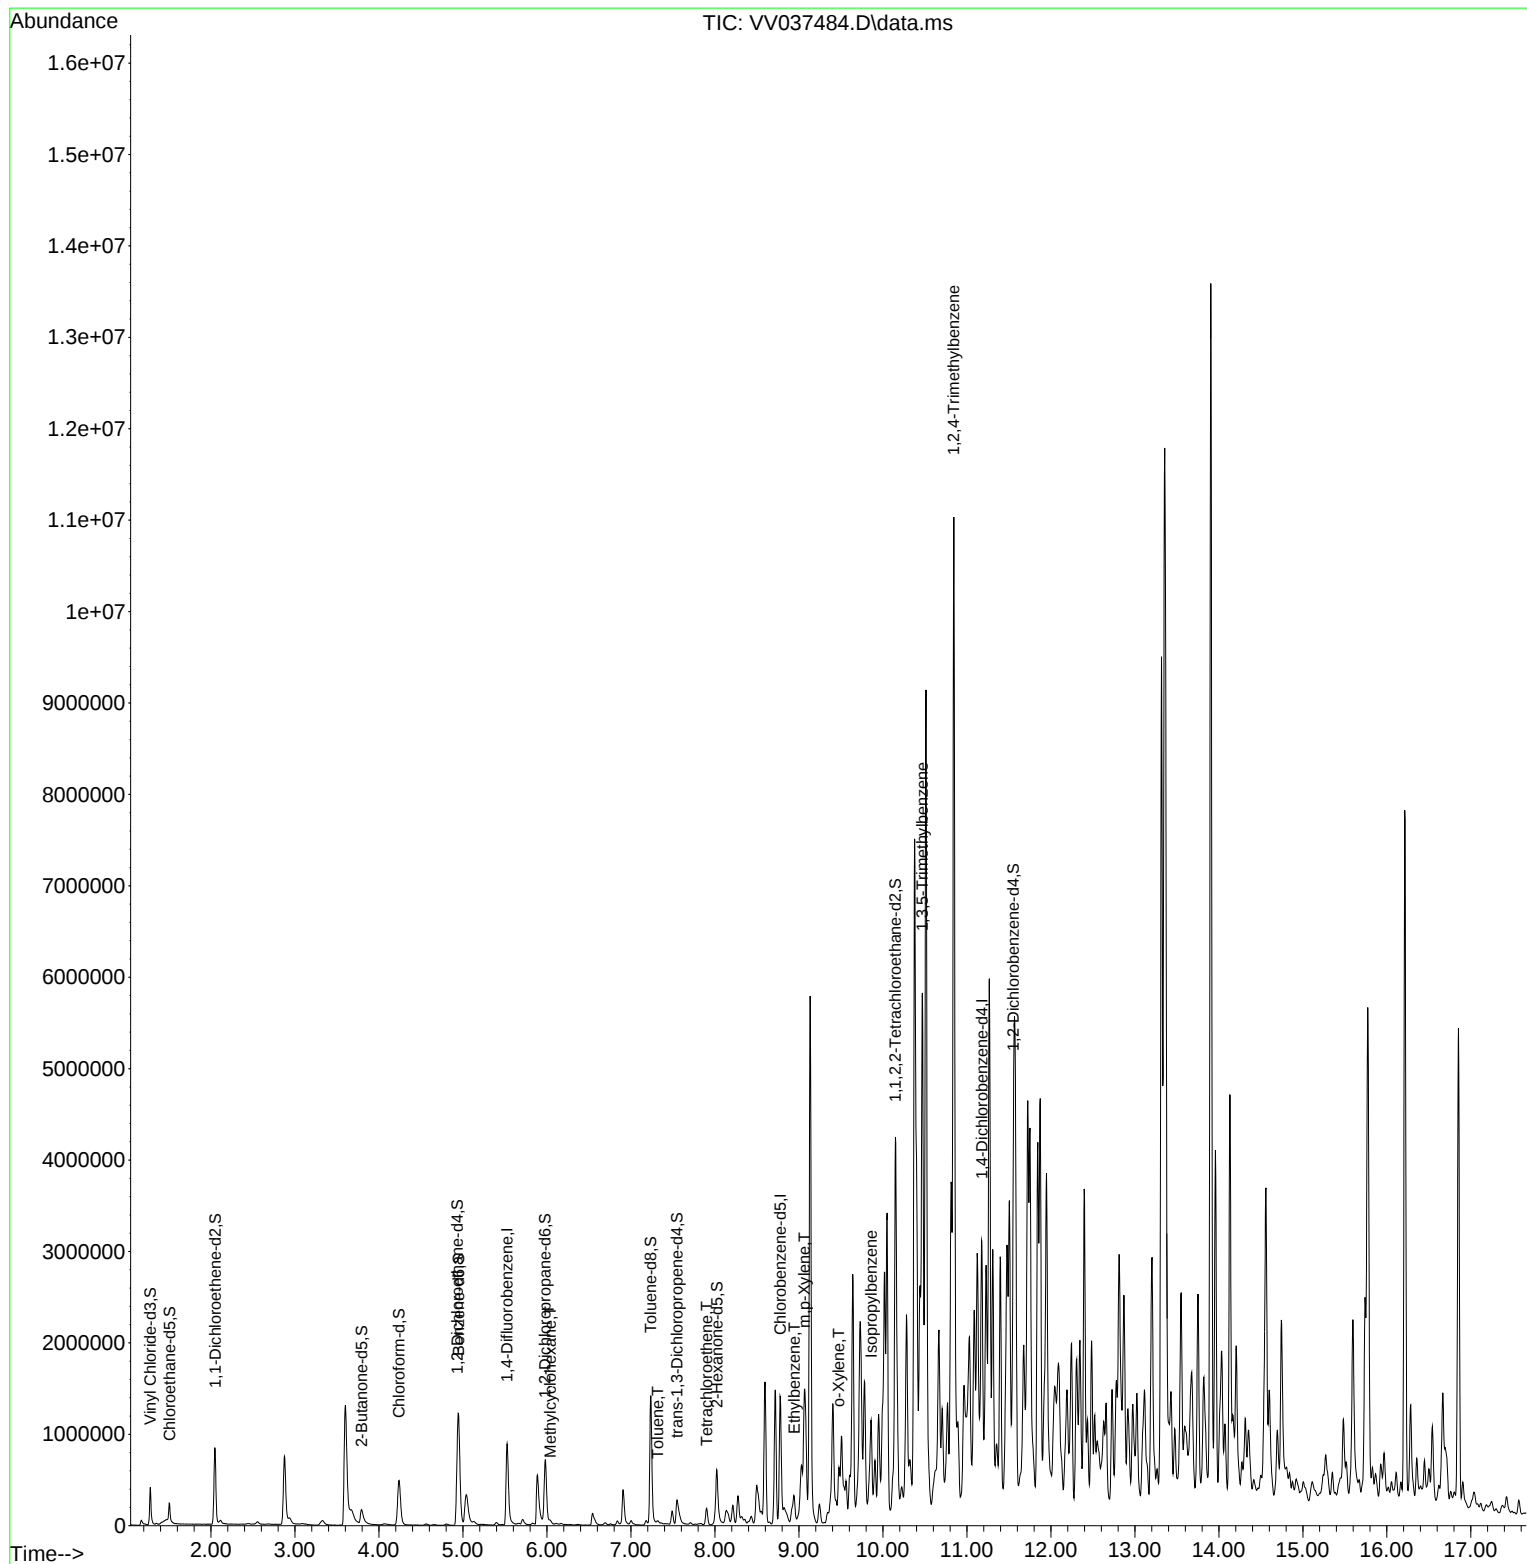


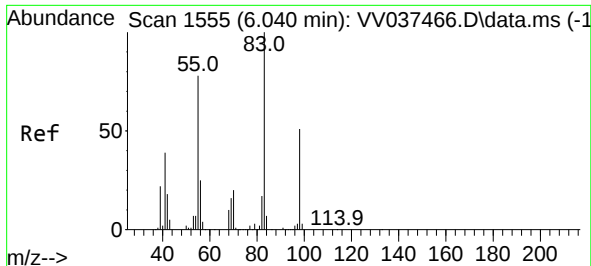

#35
Methylcyclohexane
Concen: 1.598 ug/L
RT: 6.040 min Scan# 11
Delta R.T. -0.000 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55




Instrument :
MSVOA_V
ClientSampleId :
DDC36ME


Tgt Ion: 83 Resp: 15016
Ion Ratio Lower Upper
83 100
55 82.8 61.2 91.8
98 55.9 39.3 58.9

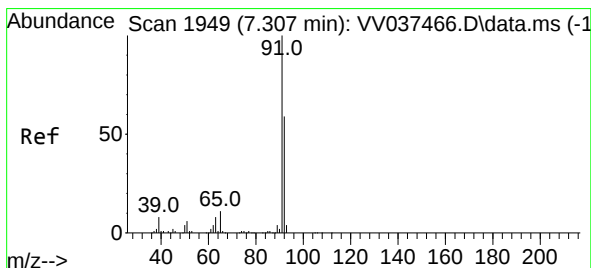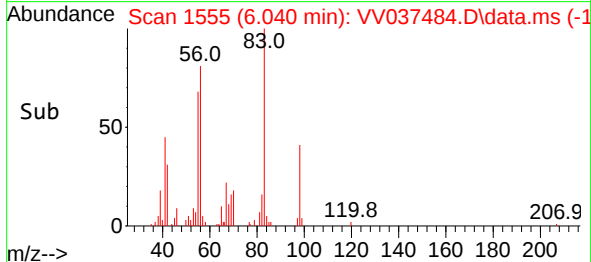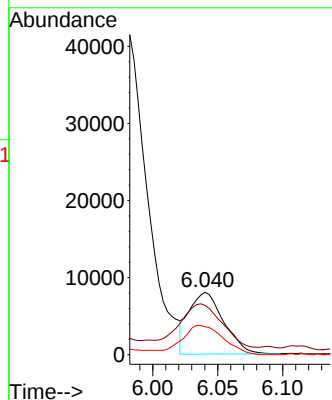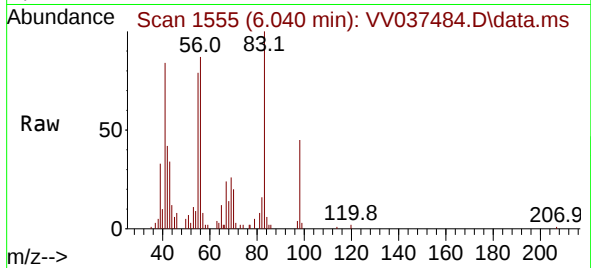

#42
Toluene
Concen: 1.224 ug/L
RT: 7.320 min Scan# 1953
Delta R.T. 0.013 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55

Tgt Ion: 91 Resp: 27919
Ion Ratio Lower Upper
91 100
92 57.1 40.8 75.8


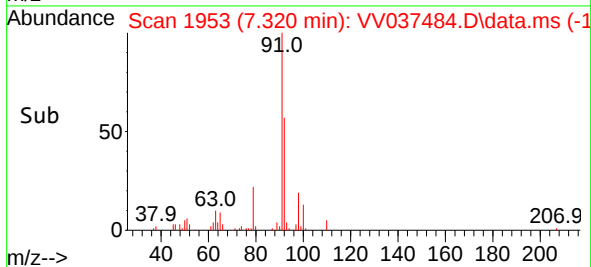
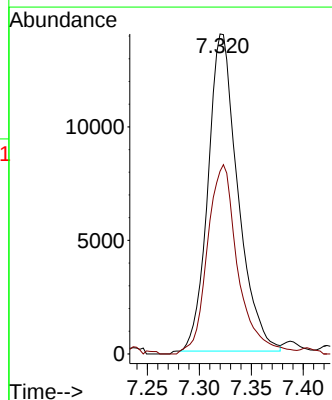
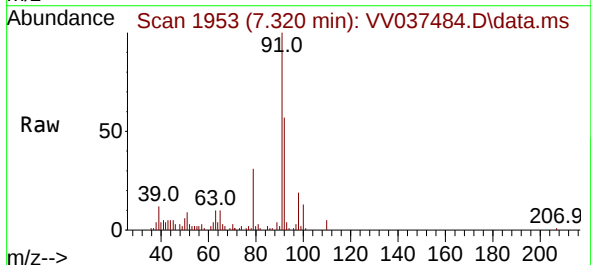


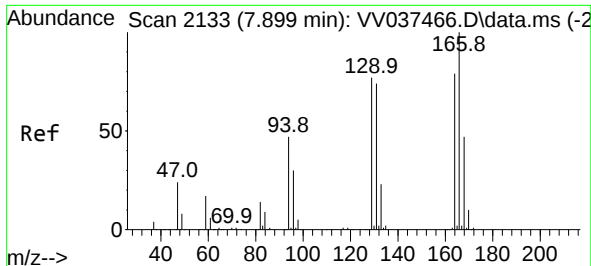

#46
Tetrachloroethene
Concen: 7.829 ug/L
RT: 7.902 min Scan# 2133
Delta R.T. 0.003 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55




Instrument :
MSVOA_V
ClientSampleId :
DDC36ME


Tgt Ion:164	Resp:	32489
Ion Ratio	Lower	Upper
164	100	
129	97.4	67.1 124.7
131	105.8	67.0 124.4
166	127.9	86.2 160.2

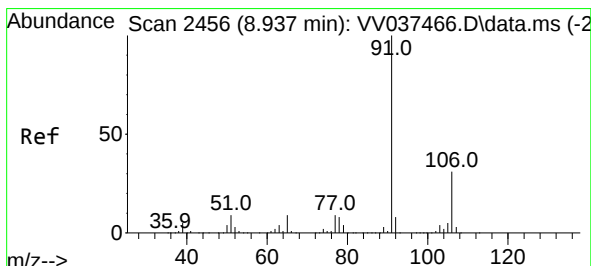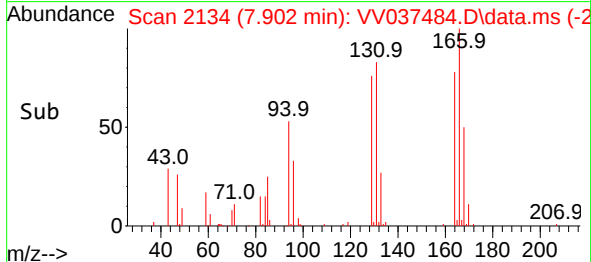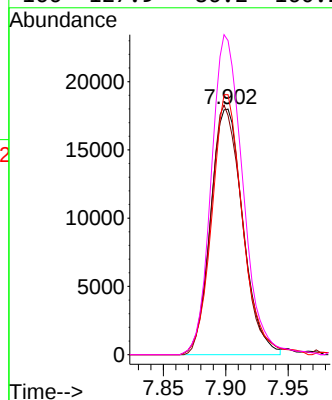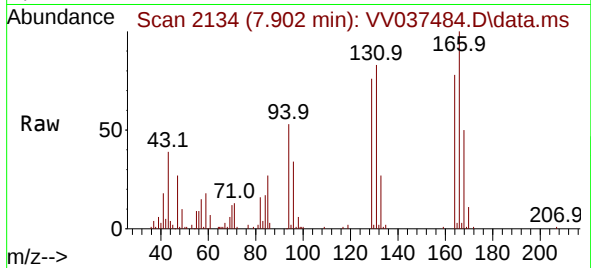

#52
Ethylbenzene
Concen: 6.350 ug/L
RT: 8.944 min Scan# 2458
Delta R.T. 0.006 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55

Tgt Ion: 91	Resp:	163639
Ion Ratio	Lower	Upper
91	100	
106	30.7	21.4 39.8


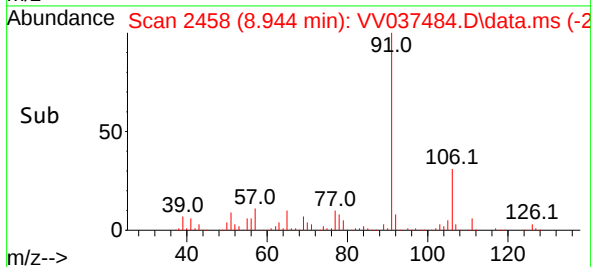
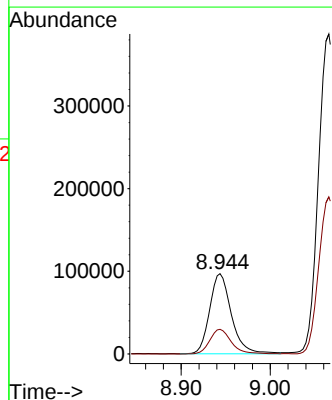
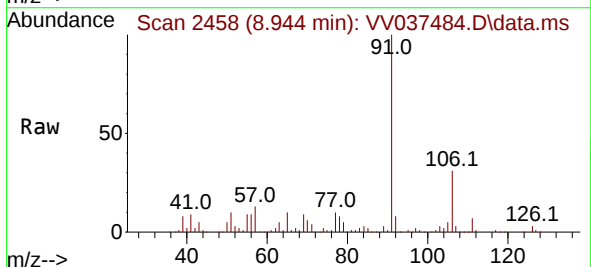


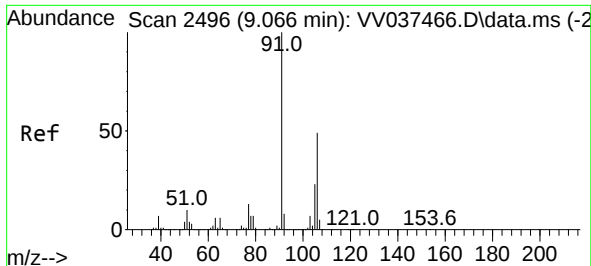

#53
m,p-Xylene
Concen: 32.214 ug/L
RT: 9.066 min Scan# 2496
Delta R.T. -0.000 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55




Instrument :
MSVOA_V
ClientSampleId :
DDC36ME


Tgt Ion:106 Resp: 307596
Ion Ratio Lower Upper
106 100
91 203.6 143.0 265.6

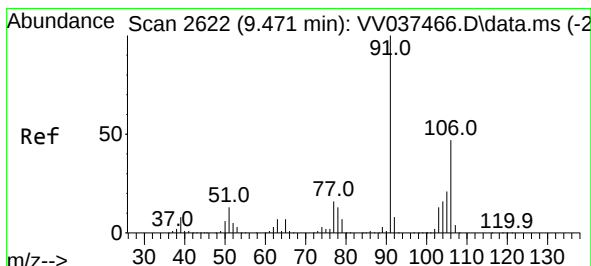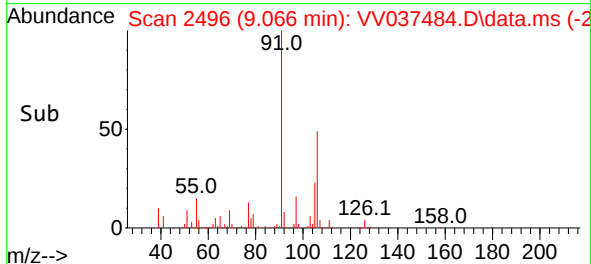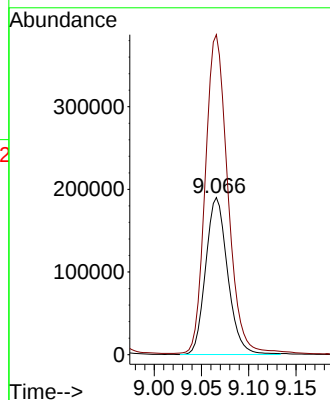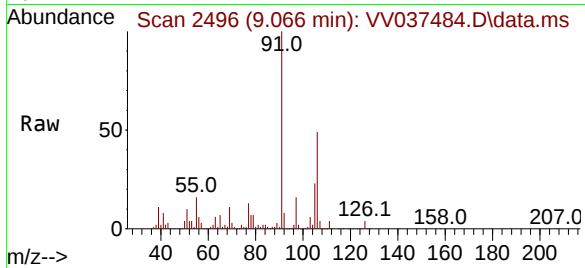

#54
o-Xylene
Concen: 10.171 ug/L
RT: 9.474 min Scan# 2623
Delta R.T. 0.003 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55

Tgt Ion:106 Resp: 95090
Ion Ratio Lower Upper
106 100
91 213.7 153.2 284.6


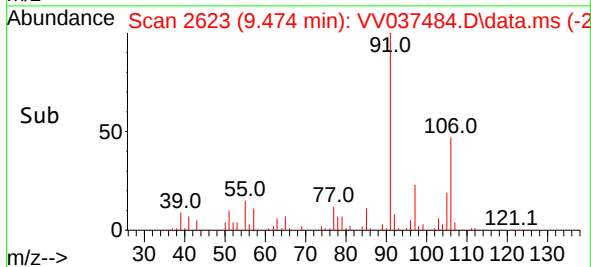
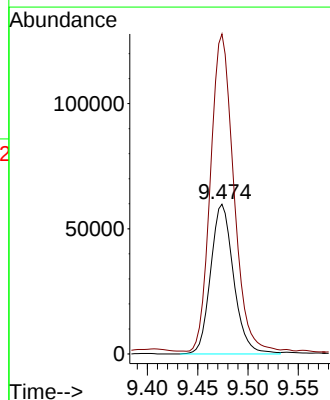
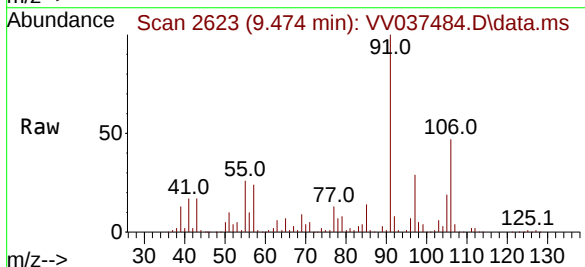


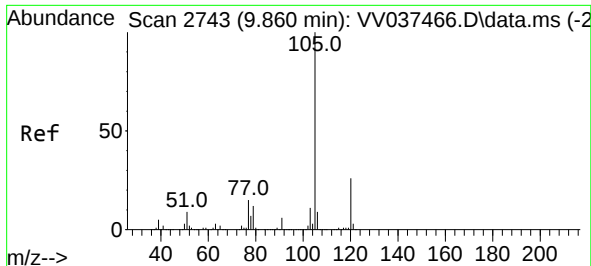

#60
Isopropylbenzene
Concen: 16.929 ug/L
RT: 9.860 min Scan# 21
Delta R.T. -0.000 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55




Instrument :
MSVOA_V
ClientSampleId :
DDC36ME


Tgt Ion:105 Resp: 457802
Ion Ratio Lower Upper
105 100
120 26.0 20.9 31.3
77 18.0 12.6 19.0

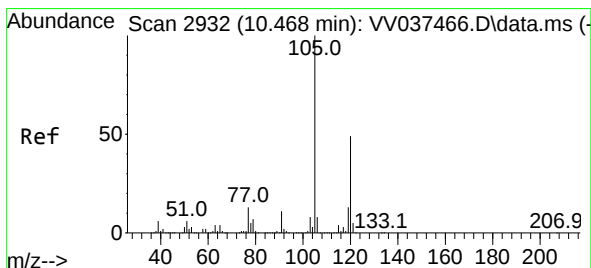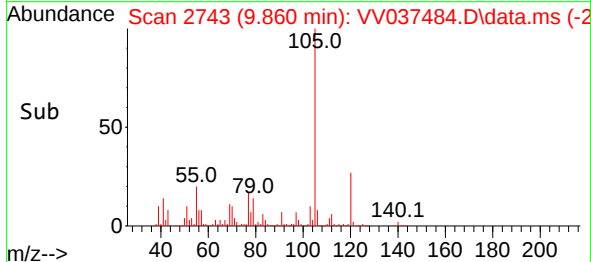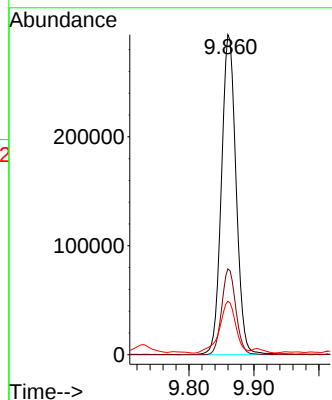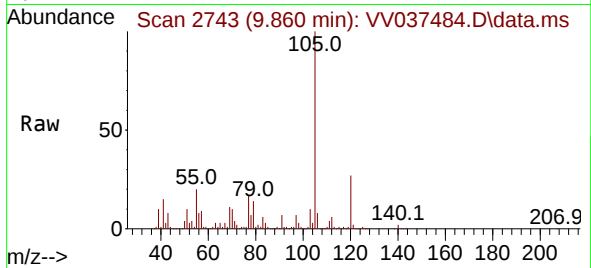

#62
1,3,5-Trimethylbenzene
Concen: 124.322 ug/L
RT: 10.468 min Scan# 2932
Delta R.T. -0.000 min
Lab File: VV037484.D
Acq: 23 Sep 2024 15:55

Tgt Ion:105 Resp: 2750659
Ion Ratio Lower Upper
105 100
120 48.6 38.3 57.5

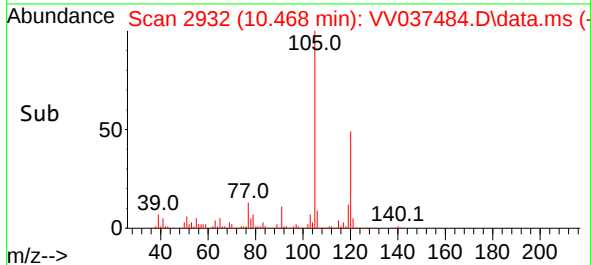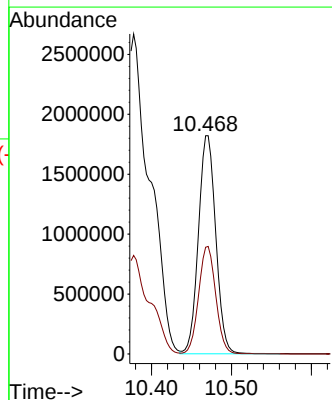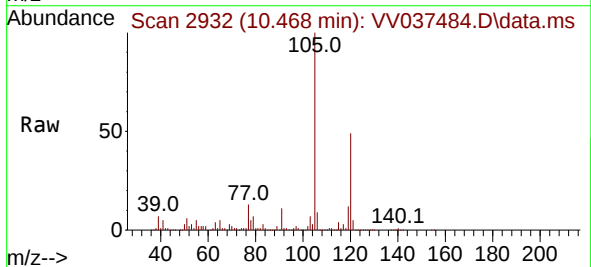

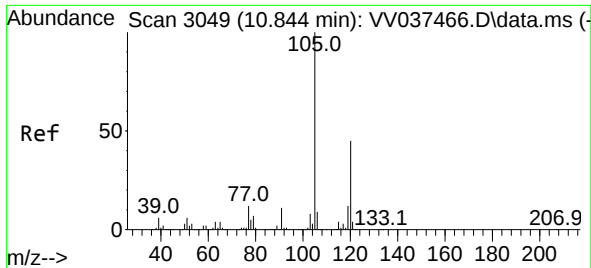

#63
 1,2,4-Trimethylbenzene
 Concen: 243.220 ug/L
 RT: 10.844 min Scan# 3049
 Delta R.T. -0.000 min
 Lab File: VV037484.D
 Acq: 23 Sep 2024 15:55

Instrument :
 MSVOA_V
 ClientSampleId :
 DDC36ME

Tgt Ion:105 Resp: 5370296
 Ion Ratio Lower Upper
 105 100
 120 45.4 35.8 53.6

