
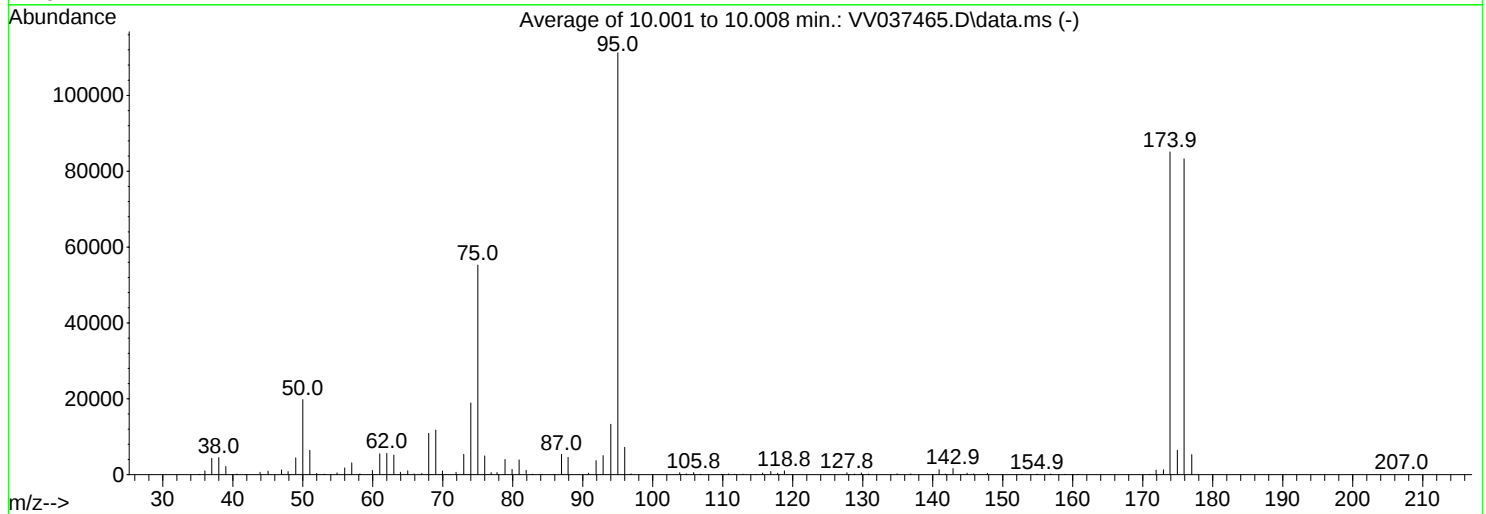


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092324\
Data File : VV037465.D
Acq On : 23 Sep 2024 08:32
Operator : SY/MD
Sample : BFB379
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB379

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Tue Sep 24 03:56:17 2024

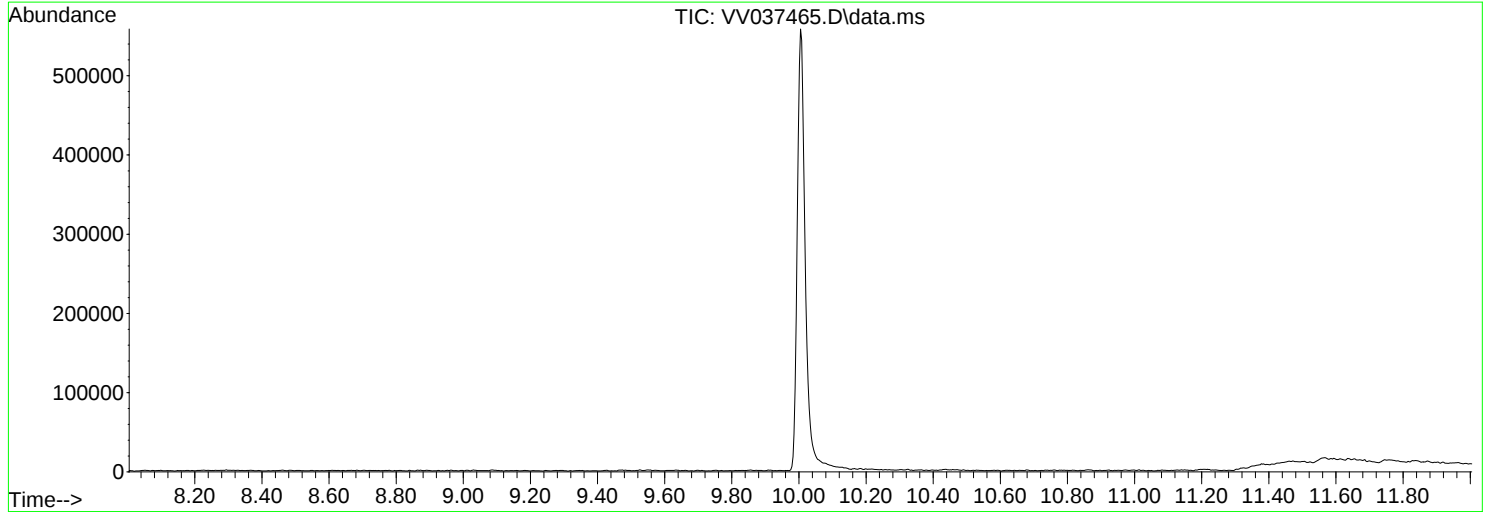

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	19811	PASS
75	95	30	80	49.7	55259	PASS
95	95	100	100	100.0	111224	PASS
96	95	5	9	6.5	7226	PASS
173	174	0.00	2	1.5	1282	PASS
174	95	50	120	76.5	85109	PASS
175	174	5	9	7.5	6408	PASS
176	174	95	105	97.9	83280	PASS
177	176	5	10	6.3	5259	PASS

m/z	Abundance
38.70	117.0
39.90	369.0
42.90	151.0
43.90	627.0
55.30	128.0
72.80	113.0
76.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
36.00	1062.0
37.00	3839.0
38.00	4427.0
39.00	1959.0
39.80	308.0
40.50	173.0
41.80	147.0
43.00	141.0
43.90	1269.0
45.10	882.0
47.00	1254.0
47.90	884.0
49.00	4281.0
50.00	19288.0
51.00	6224.0
52.00	364.0
52.90	160.0
54.90	456.0
56.00	1650.0
57.00	3004.0
58.10	198.0
60.00	1025.0
61.00	5159.0
62.00	5622.0
63.00	5036.0
63.90	656.0
65.00	799.0
66.00	248.0
67.00	264.0
68.00	10381.0
69.00	11553.0
69.90	966.0
71.90	571.0
73.00	4856.0
74.00	18240.0
75.00	53344.0
76.00	4557.0
76.90	673.0
77.80	586.0
78.90	4002.0
79.90	1357.0
80.90	3799.0
81.90	1078.0
85.80	106.0
87.00	5036.0
87.90	4726.0
90.80	310.0
91.90	3436.0
92.90	4755.0
94.00	12877.0
95.00	107888.0
96.00	7163.0
96.90	218.0
103.90	478.0
104.80	175.0
105.80	423.0
106.80	128.0
108.00	113.0
110.90	237.0
111.70	162.0
112.90	121.0
114.70	120.0
115.70	479.0
116.80	729.0
117.80	345.0
118.80	937.0
127.80	507.0
128.70	145.0
129.80	420.0
130.90	137.0
134.90	207.0
136.80	187.0
140.90	1201.0
141.80	132.0
142.90	1514.0
144.90	409.0
145.90	220.0
147.80	313.0
154.90	115.0
156.90	155.0
159.00	129.0
171.90	985.0
173.00	1074.0
173.90	79008.0
174.90	5869.0
175.90	78304.0
177.00	5142.0
177.90	135.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
35.20	124.0
36.00	1047.0
37.00	4402.0
38.00	4714.0
39.00	2215.0
39.90	352.0
40.60	168.0
41.80	132.0
43.00	130.0
43.90	1281.0
45.00	951.0
46.90	1330.0
47.90	876.0
49.00	4568.0
50.00	20608.0
51.00	6663.0
52.00	378.0
53.10	197.0
54.90	513.0
56.00	1882.0
57.00	3300.0
58.10	210.0
59.90	1099.0
61.00	5700.0
62.00	5866.0
63.00	5487.0
64.00	634.0
65.00	1040.0
65.90	233.0
67.00	325.0
68.00	11131.0
69.00	12239.0
69.90	1028.0
71.90	639.0
73.00	5544.0
74.00	19664.0
75.00	57304.0
76.00	5095.0
76.90	741.0
77.70	532.0
78.90	4164.0
79.90	1441.0
80.90	4007.0
81.90	1186.0
82.80	152.0
84.20	108.0
85.80	167.0
87.00	5503.0
87.90	4666.0
90.80	357.0
91.90	3845.0
92.90	5164.0
94.00	13829.0
95.00	115128.0
96.00	7444.0
96.90	238.0
103.80	504.0
104.80	209.0
105.90	566.0
106.80	123.0
107.90	116.0
109.90	109.0
110.80	222.0
111.70	166.0
112.90	147.0
115.70	429.0
116.80	837.0
117.90	404.0
118.80	1048.0
124.00	113.0
127.70	510.0
128.80	168.0
129.80	512.0
130.90	172.0
134.90	286.0
136.80	194.0
140.90	1382.0
141.80	171.0
142.90	1658.0
144.90	384.0
145.80	244.0
147.80	368.0
152.70	112.0
154.90	178.0
156.90	175.0
158.90	140.0
160.70	139.0
171.00	142.0
171.90	1225.0
172.90	1380.0
173.90	87984.0
175.00	6697.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

175.90	86456.0
177.00	5365.0
177.90	109.0
207.00	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
35.20	124.0
36.00	938.0
37.00	4683.0
38.00	4448.0
39.00	2221.0
39.90	396.0
40.70	157.0
43.00	153.0
43.90	1193.0
45.00	921.0
46.90	1276.0
47.90	701.0
49.00	4386.0
50.00	19536.0
51.00	6395.0
52.00	328.0
53.10	239.0
54.90	476.0
56.00	1839.0
57.00	3023.0
58.20	198.0
59.90	1122.0
61.00	5626.0
62.00	5355.0
63.00	4918.0
64.00	601.0
65.00	1185.0
65.80	185.0
67.00	332.0
68.00	11202.0
69.00	11452.0
70.00	964.0
71.90	701.0
73.00	5665.0
74.00	18792.0
75.00	55128.0
76.00	5116.0
76.90	747.0
77.80	491.0
78.90	3899.0
79.90	1394.0
80.90	3820.0
81.90	1134.0
82.80	202.0
84.20	109.0
86.00	189.0
86.90	5495.0
87.90	4239.0
90.80	437.0
91.90	3821.0
92.90	5169.0
94.00	13153.0
95.00	110656.0
96.00	7071.0
96.90	236.0
103.80	531.0
104.80	213.0
105.90	606.0
106.90	108.0
107.80	119.0
109.80	119.0
110.70	228.0
112.90	107.0
114.80	103.0
115.70	395.0
116.90	949.0
117.90	455.0
118.80	1019.0
124.00	102.0
127.70	487.0
128.90	187.0
129.80	501.0
130.80	180.0
134.90	305.0
136.90	243.0
140.90	1345.0
141.80	180.0
142.90	1665.0
144.90	350.0
145.80	231.0
147.80	357.0
149.90	106.0
152.70	106.0
154.90	241.0
156.80	181.0
158.80	184.0
160.70	164.0
171.00	137.0
171.90	1346.0
172.90	1393.0
173.90	88336.0
174.90	6658.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

175.90	85080.0
177.00	5271.0
177.90	114.0
207.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379