

Data File : VV012969.D
Acq On : 25 Sep 2019 11:31
Operator : SY/MD
Sample : K5001-14
Misc : 5.07G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Sep 26 01:13:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 01:10:53 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	686785	25.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	686092	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	322687	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	254097	23.84	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.36%
7) Chloroethane-d5	1.58	69	213348	24.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.04%
10) 1,1-Dichloroethene-d2	2.13	63	330186	18.63	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.52%
20) 2-Butanone-d5	3.93	46	158783	43.15	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.30%
24) Chloroform-d	4.40	84	438689	23.25	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.00%
26) 1,2-Dichloroethane-d4	5.08	65	255974	23.34	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.36%
29) Benzene-d6	5.10	84	909030	23.73	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.92%
33) 1,2-Dichloropropane-d6	6.12	67	288674	24.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.16%
37) Toluene-d8	7.36	98	802396	23.07	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.28%
38) trans-1,3-Dichloropropene-	7.66	79	108682	21.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.52%
39) 2-Hexanone-d5	8.13	63	106186	43.95	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.90%
48) 1,1,2,2-Tetrachloroethane-	10.26	84	245008	21.48	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.92%
61) 1,2-Dichlorobenzene-d4	11.67	152	317929	25.36	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.44%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	11.29	75	36892	4.286 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VV012969.D
Acq On : 25 Sep 2019 11:31
Operator : SY/MD
Sample : K5001-14
Misc : 5.07G/10ML/MSVOA_V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK02

Quant Time: Sep 26 01:13:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 26 01:10:53 2019
Response via : Initial Calibration

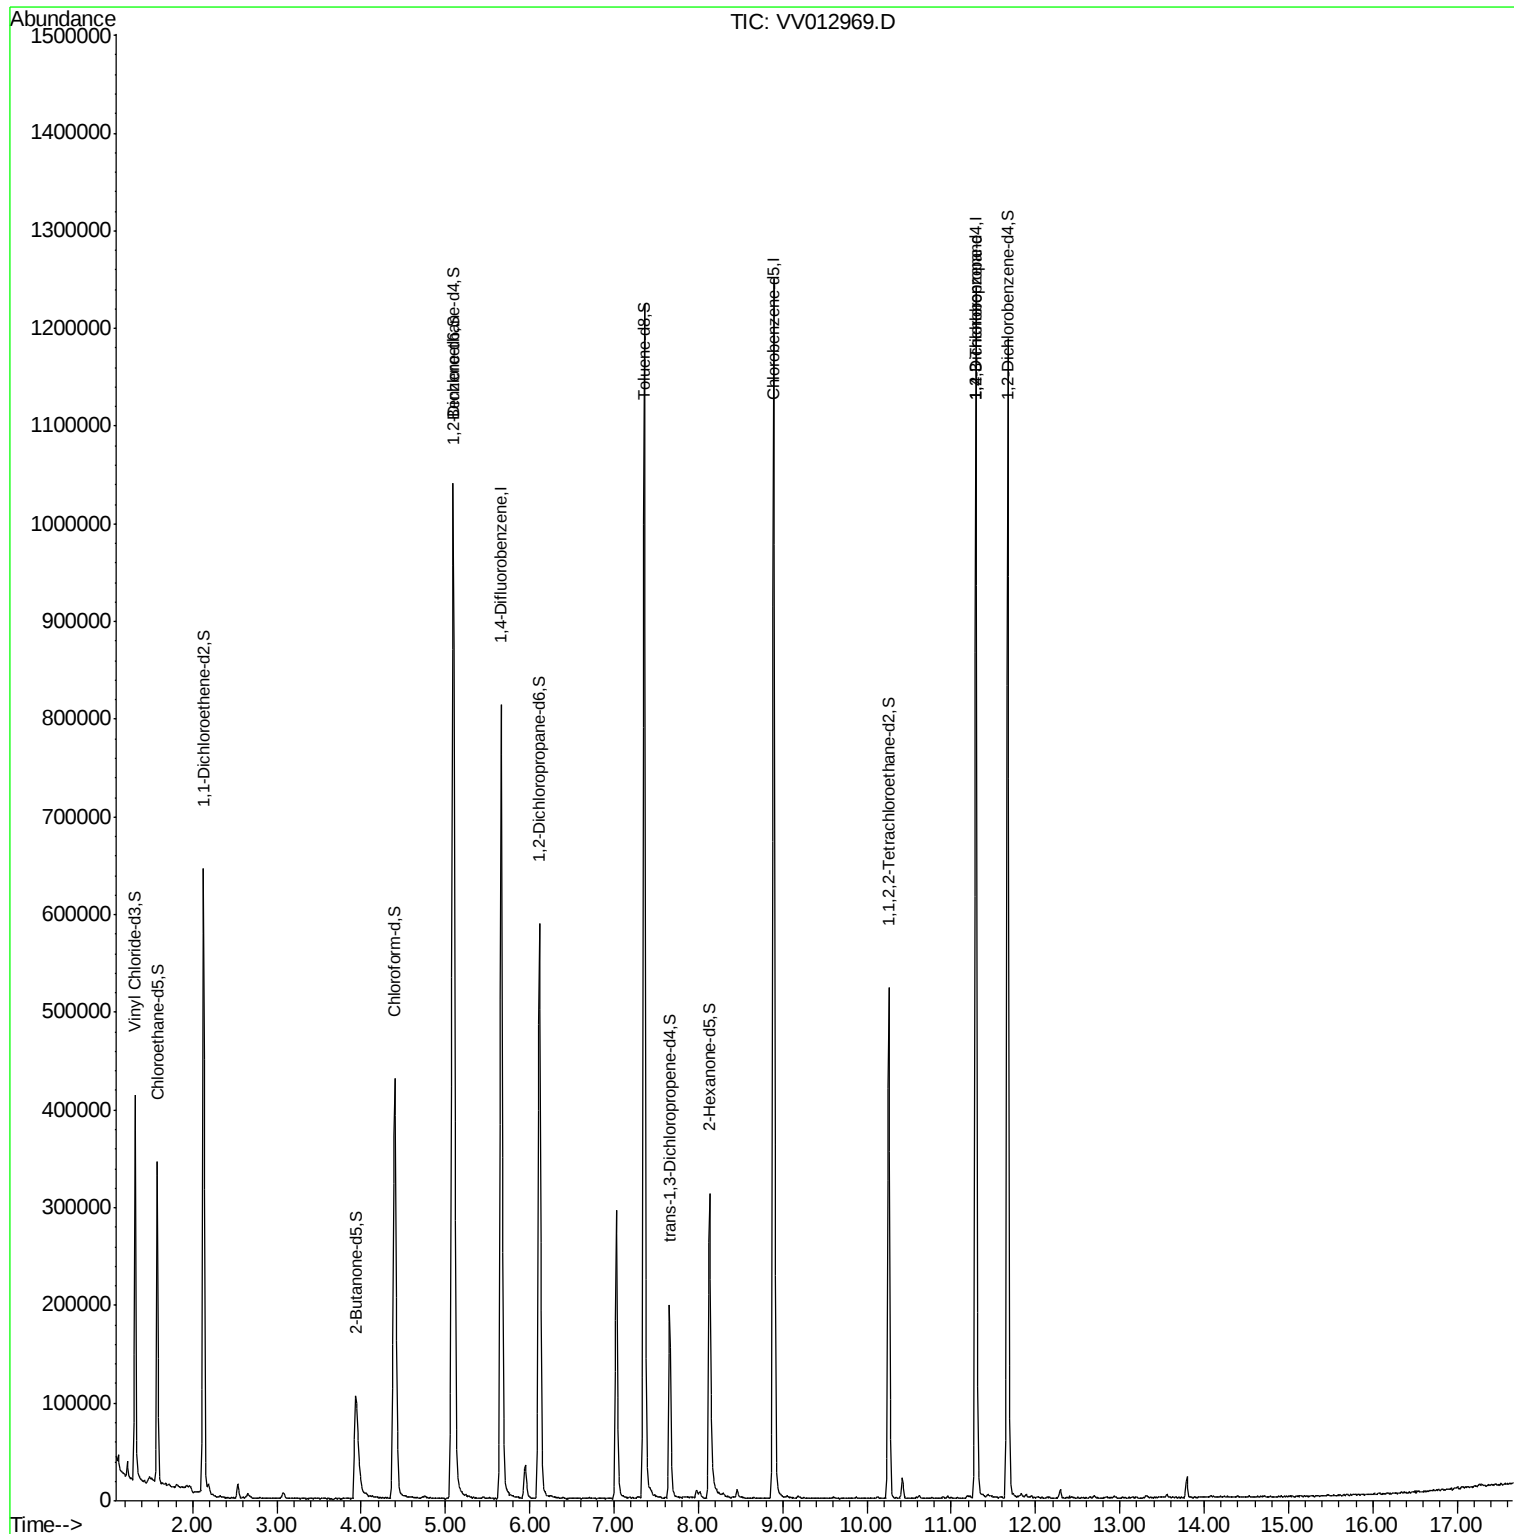

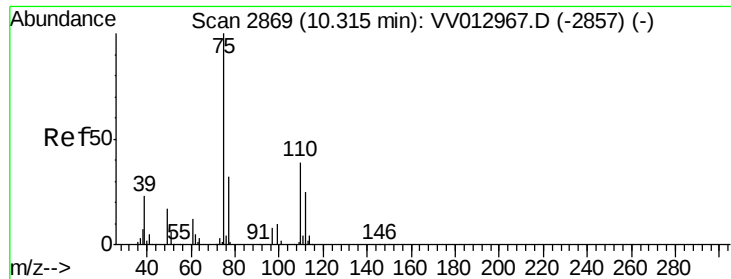

#59
 1,2,3-Trichloropropane
 Concen: 4.286 ug/L
 RT: 11.29 min Scan# 3173
 Delta R.T. 0.98 min
 Lab File: VV012969.D
 Acq: 25 Sep 2019 11:31

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK02

Tgt Ion: 75 Resp: 36892
 Ion Ratio Lower Upper
 75 100
 77 35.9 25.4 38.0

