


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV092519\
Data File : VV012966.D
Acq On : 25 Sep 2019 09:19
Operator : SY/MD
Sample : BFB63
Misc : 5.00G/10ML/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM092319S.M
Title : VOC Analysis
Last Update : Thu Sep 26 01:10:53 2019

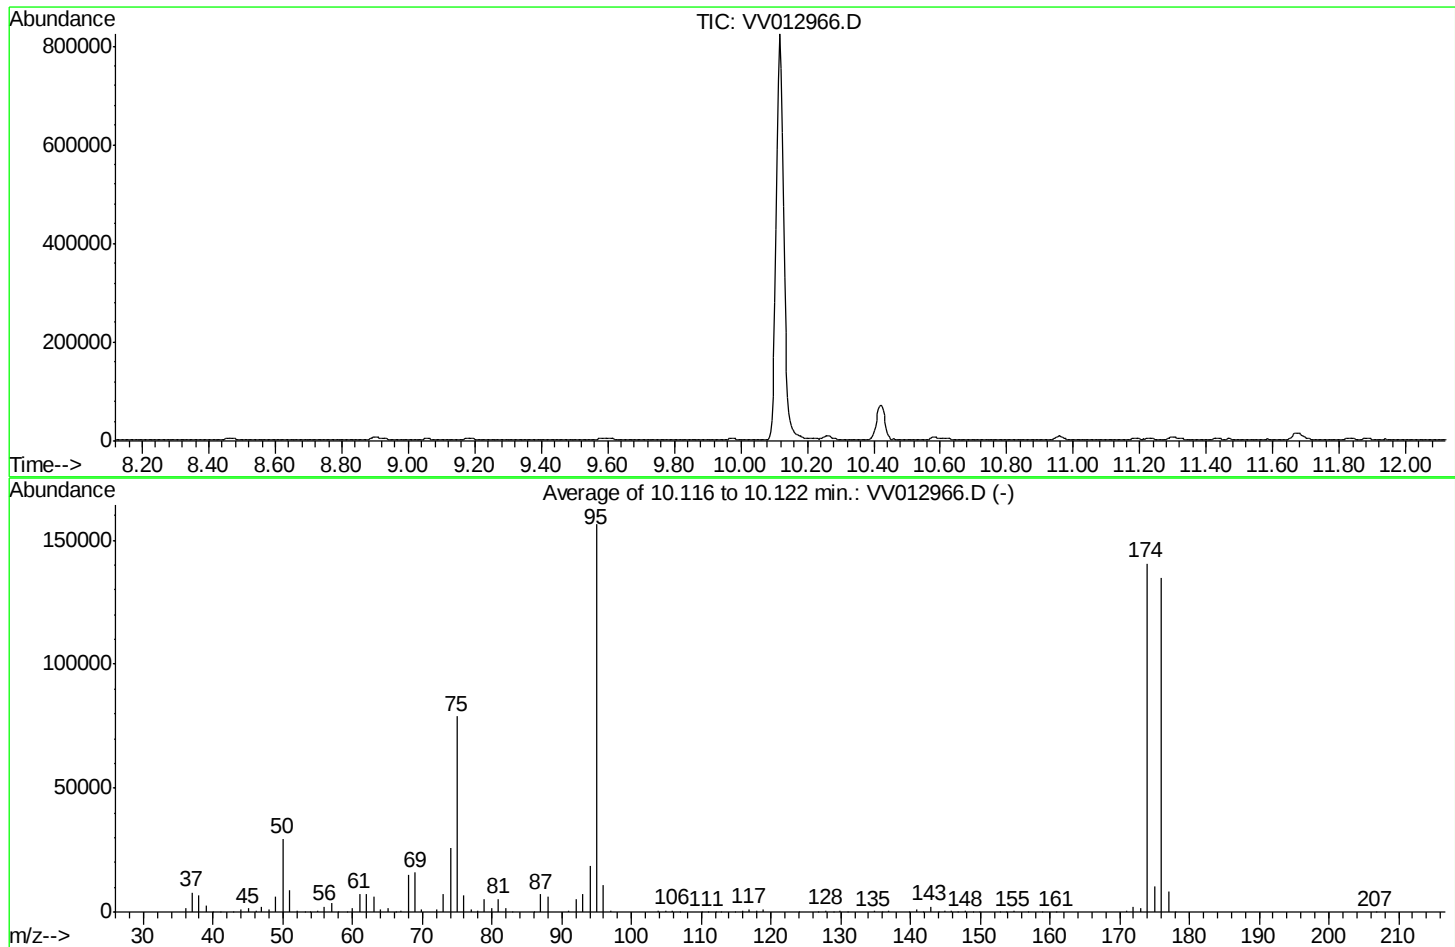

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	29626	PASS
75	95	30	80	50.4	78896	PASS
95	95	100	100	100.0	156437	PASS
96	95	5	9	6.9	10750	PASS
173	174	0.00	2	1.2	1652	PASS
174	95	50	120	89.9	140650	PASS
175	174	5	9	7.5	10497	PASS
176	174	95	101	95.9	134877	PASS
177	176	5	9	6.1	8188	PASS

m/z	Abundance
36.00	1550.0
37.00	8594.0
38.00	6989.0
39.10	2973.0
40.00	1248.0
41.00	139.0
42.90	166.0
44.00	1787.0
45.00	1386.0
46.20	364.0
47.00	2011.0
48.00	957.0
49.00	6754.0
50.00	30416.0
51.00	9390.0
52.00	456.0
53.10	257.0
54.00	143.0
55.00	421.0
56.00	2497.0
57.00	4011.0
58.00	164.0
59.20	138.0
60.00	1633.0
61.00	7699.0
62.00	7810.0
63.00	6560.0
64.00	950.0
65.00	1587.0
66.10	255.0
67.00	605.0
68.00	15194.0
69.00	16331.0
70.00	1350.0
72.10	1099.0
73.00	7254.0
74.00	27296.0
75.00	82000.0
76.00	7282.0
77.00	911.0
77.90	666.0
78.90	5304.0
80.00	1476.0
80.90	5484.0
81.90	1297.0
82.90	208.0
86.00	194.0
87.00	7244.0
88.00	6502.0
90.90	644.0
92.00	5282.0
93.00	7233.0
94.00	18600.0
95.00	160960.0
96.00	11422.0
97.00	377.0
103.90	704.0
104.90	259.0
105.90	707.0
106.90	220.0
110.10	116.0
110.90	109.0
112.90	131.0
115.00	176.0
115.90	510.0
116.90	1169.0
117.90	644.0
118.90	908.0
123.90	145.0
128.00	635.0
128.90	249.0
129.80	595.0
131.00	274.0
134.80	342.0
135.90	151.0
137.00	338.0
139.90	112.0
140.90	1365.0
141.90	254.0
142.90	2137.0
143.90	152.0
144.90	845.0
145.80	395.0
146.90	160.0
147.90	457.0
149.90	238.0
152.80	168.0
154.80	440.0
156.80	249.0
158.80	219.0
161.00	168.0
171.00	307.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

171.90	2301.0
173.00	1678.0
173.90	141248.0
175.00	10643.0
175.90	134464.0
177.00	8356.0
177.90	186.0
206.70	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	1515.0
37.00	8031.0
38.00	6850.0
39.10	3006.0
40.00	1278.0
41.00	140.0
42.80	142.0
44.00	1847.0
45.00	1355.0
46.10	344.0
47.00	2008.0
48.00	875.0
49.00	6590.0
50.00	30664.0
51.00	9157.0
52.00	361.0
53.10	254.0
54.00	151.0
55.00	440.0
56.00	2410.0
57.00	3947.0
58.00	169.0
59.20	111.0
60.00	1502.0
61.00	7539.0
62.00	7641.0
63.00	6627.0
64.00	1008.0
65.00	1682.0
66.10	252.0
67.00	570.0
68.00	15306.0
69.00	16392.0
70.00	1322.0
72.00	1011.0
73.00	7256.0
74.00	27008.0
75.00	81688.0
76.00	7037.0
77.00	937.0
77.90	772.0
78.90	5301.0
80.00	1441.0
80.90	5499.0
81.90	1373.0
82.90	224.0
85.90	252.0
87.00	7427.0
88.00	6145.0
90.90	593.0
92.00	5367.0
93.00	7252.0
94.00	19120.0
95.00	161472.0
96.00	11060.0
97.00	414.0
103.80	617.0
104.80	301.0
105.90	615.0
106.90	201.0
110.10	118.0
111.00	129.0
112.10	115.0
112.90	102.0
114.90	194.0
115.90	560.0
116.90	1293.0
117.90	551.0
118.90	958.0
124.00	137.0
127.90	593.0
128.90	270.0
129.80	588.0
131.00	244.0
134.80	314.0
136.90	280.0
139.90	125.0
140.90	1293.0
141.90	286.0
142.90	2212.0
144.00	128.0
144.90	781.0
145.80	356.0
146.90	153.0
147.90	483.0
149.00	109.0
149.90	213.0
152.80	202.0
154.80	440.0
156.80	210.0
158.90	235.0
161.00	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

171.00	287.0
171.90	2326.0
173.00	1713.0
173.90	145472.0
175.00	10791.0
175.90	139392.0
177.00	8471.0
178.00	174.0
206.70	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	1329.0
37.00	6977.0
38.00	6319.0
39.00	2723.0
40.00	1327.0
41.10	136.0
42.80	136.0
44.00	1706.0
45.00	1220.0
46.10	287.0
47.00	1740.0
47.90	747.0
49.00	5931.0
50.00	27800.0
51.00	8532.0
52.10	318.0
53.10	229.0
53.90	121.0
55.00	457.0
56.00	2112.0
57.00	3716.0
57.90	179.0
60.00	1244.0
61.00	6799.0
62.00	6711.0
63.00	6008.0
64.00	1012.0
65.00	1661.0
66.10	227.0
66.90	439.0
68.00	14252.0
69.00	14953.0
69.90	1171.0
72.00	892.0
73.00	6539.0
74.00	23792.0
75.00	73000.0
76.00	6239.0
77.00	925.0
77.90	751.0
78.90	4710.0
80.00	1378.0
80.90	4972.0
81.90	1322.0
82.90	218.0
85.90	277.0
87.00	6641.0
88.00	5615.0
90.90	542.0
92.00	4670.0
93.00	6673.0
94.00	17472.0
95.00	146880.0
96.00	9769.0
97.00	320.0
103.80	465.0
104.80	286.0
105.90	527.0
106.90	145.0
110.00	105.0
111.00	142.0
112.00	122.0
112.90	108.0
114.80	192.0
115.90	553.0
116.90	1244.0
118.00	483.0
118.90	923.0
126.70	104.0
127.90	545.0
128.90	245.0
129.80	505.0
131.00	198.0
134.80	278.0
136.80	224.0
139.80	134.0
140.90	1158.0
141.90	246.0
142.90	2104.0
144.00	113.0
144.90	655.0
145.80	301.0
146.80	121.0
147.90	449.0
149.00	123.0
150.00	147.0
152.90	170.0
153.80	106.0
154.80	402.0
156.80	185.0
158.90	234.0
160.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

171.00	257.0
171.90	2087.0
173.00	1566.0
173.90	135232.0
175.00	10057.0
175.90	130776.0
177.00	7739.0
178.00	159.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

Scan 2794 (10.074 min): VV012966.D
BFB63

m/z	Abundance
39.00	139.0
39.90	1075.0
41.00	129.0
44.00	885.0
61.80	110.0
68.80	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63