




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028126.D
 Acq On : 26 Sep 2022 19:09
 Operator : SY/MD
 Sample : N4820-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8P3

Manual IntegrationsAPPROVED

Quant Time: Sep 26 21:32:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 26 21:28:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

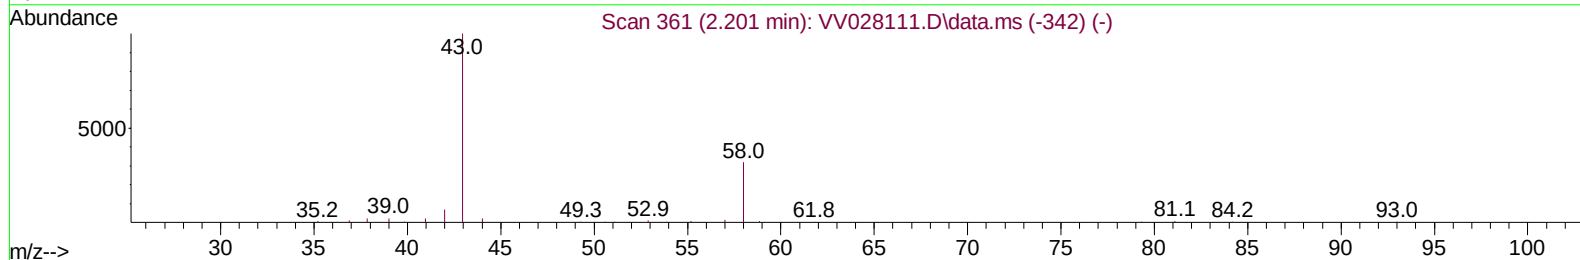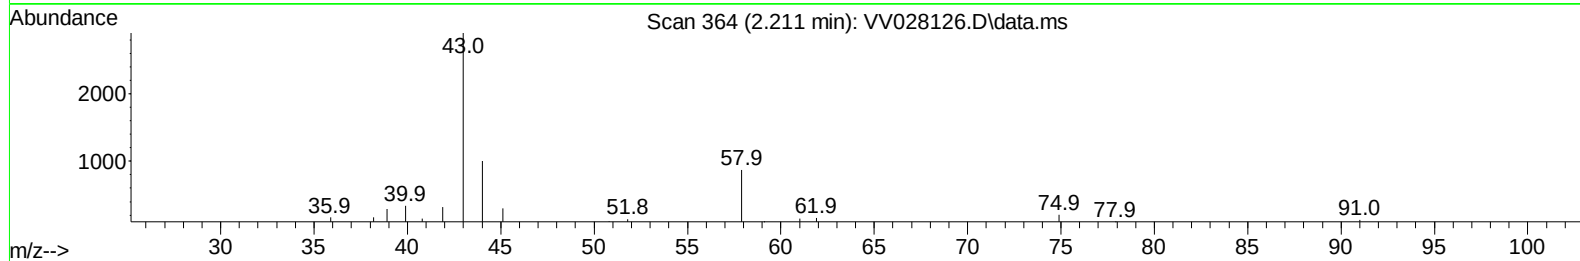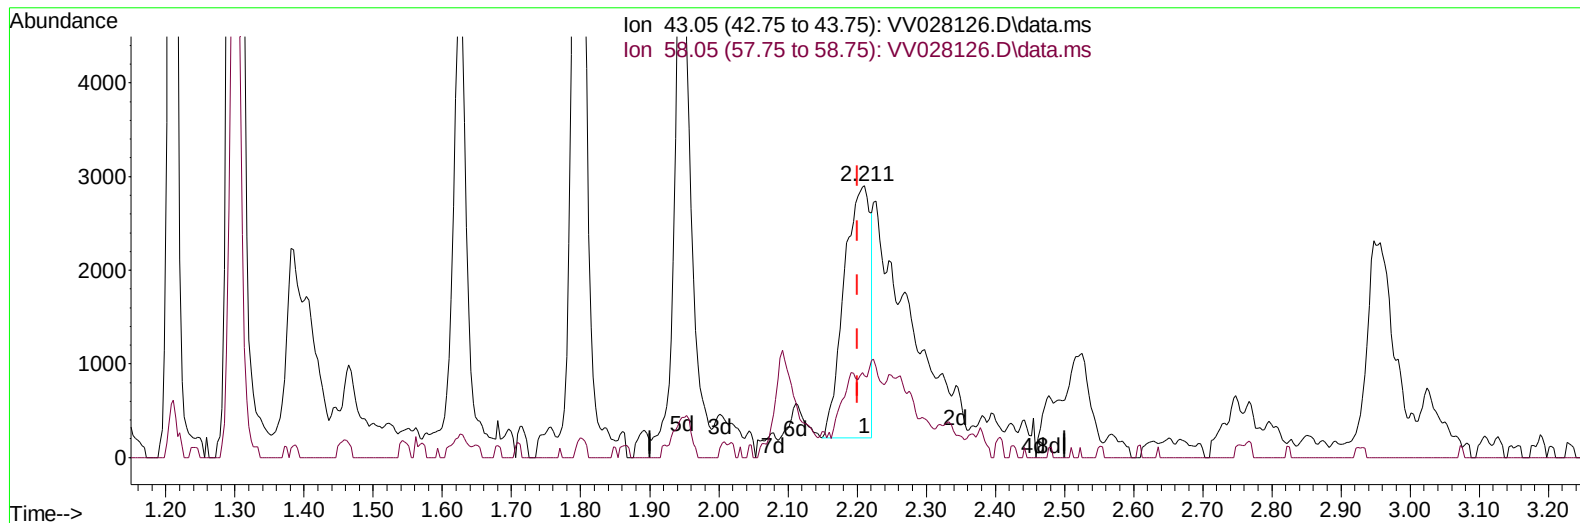

TIC: VV028126.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 3.06 ug/L

response 7039

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	5.65
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028126.D
 Acq On : 26 Sep 2022 19:09
 Operator : SY/MD
 Sample : N4820-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8P3

Manual IntegrationsAPPROVED

Quant Time: Sep 26 21:32:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 26 21:28:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

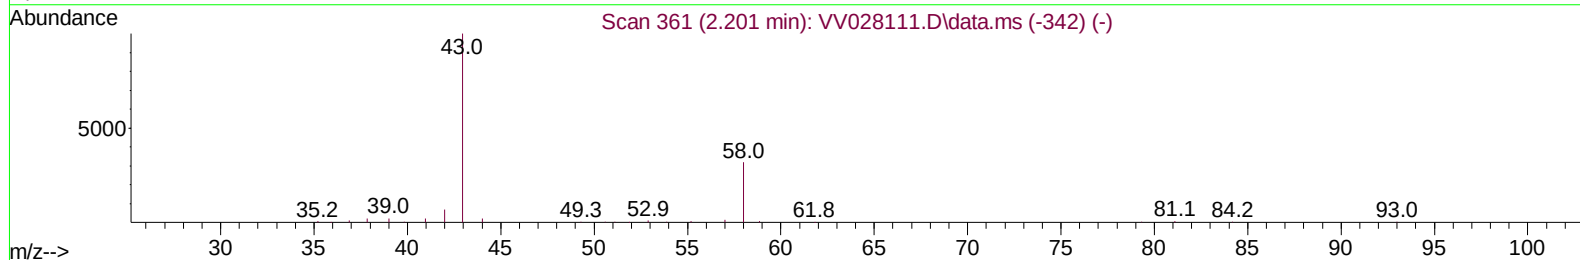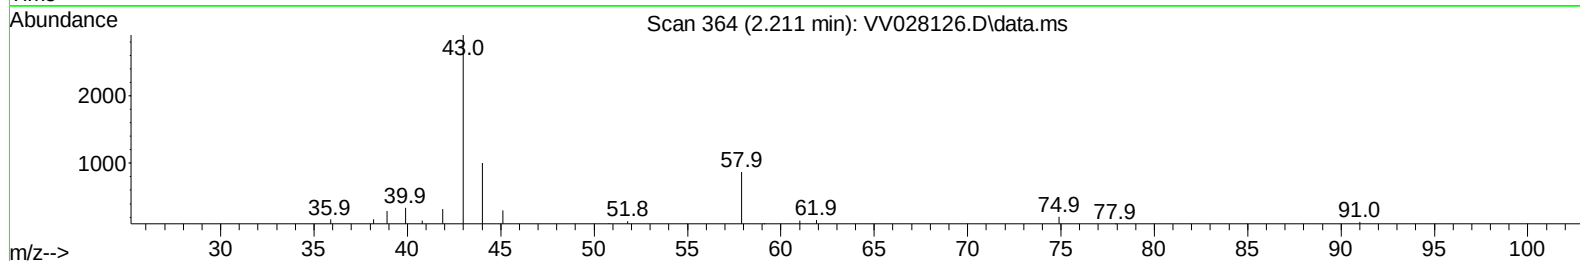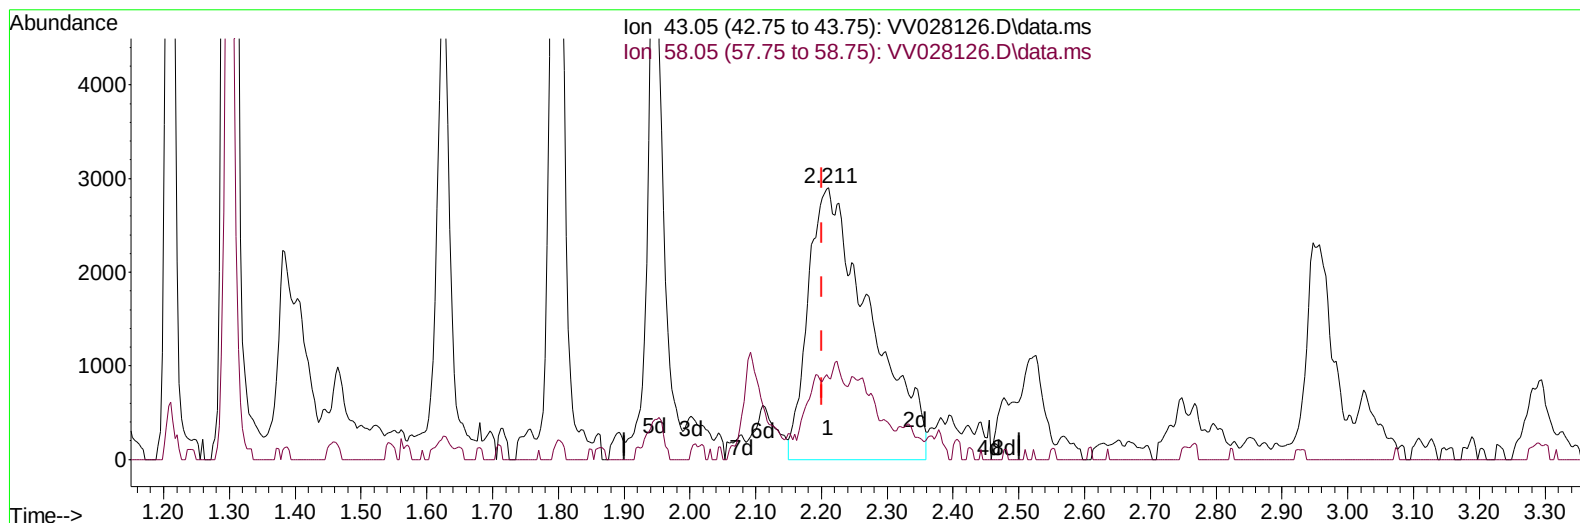

TIC: VV028126.D\data.ms

(13) Acetone (T)

2.211min (+ 0.010) 8.25 ug/L m

response 18969

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	2.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028126.D
 Acq On : 26 Sep 2022 19:09
 Operator : SY/MD
 Sample : N4820-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8P3

Manual IntegrationsAPPROVED

Quant Time: Sep 26 21:32:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 26 21:28:54 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
 Supervised By :Mahesh Dadoda 09/27/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	170548	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	177955	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	96268	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	59362	3.357	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	67.200%	
7) Chloroethane-d5	1.561	69	54189	3.855	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	77.000%	
11) 1,1-Dichloroethene-d2	2.098	63	77138	2.515	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	50.400%#	
20) 2-Butanone-d5	3.915	46	131942	44.201	ug/L	0.01
Spiked Amount 50.000	Range 40	- 130	Recovery	=	88.400%	
24) Chloroform-d	4.342	84	121396	4.303	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	86.000%	
26) 1,2-Dichloroethane-d4	5.031	65	58338	4.345	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	87.000%	
32) Benzene-d6	5.043	84	220092	3.772	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	75.400%	
36) 1,2-Dichloropropane-d6	6.066	67	75694	4.161	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	83.200%	
41) Toluene-d8	7.313	98	174210	3.298	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	66.000%#	
43) trans-1,3-Dichloroprop...	7.622	79	24533	3.734	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	74.600%	
46) 2-Hexanone-d5	8.088	63	123402	44.997	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	90.000%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	56685	4.559	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	91.200%	
66) 1,2-Dichlorobenzene-d4	11.619	152	85055	4.504	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	90.000%	
Target Compounds					Qvalue	
13) Acetone	2.211	43	18969m	8.250	ug/L	
14) Carbon disulfide	2.281	76	2894	0.128	ug/L #	87
30) Cyclohexane	4.670	56	13756	0.870	ug/L	90
33) Benzene	5.101	78	11060	0.224	ug/L	100
35) Methylcyclohexane	6.124	83	12236	0.725	ug/L	96
51) Chlorobenzene	8.876	112	2684722	77.653	ug/L	99
52) Ethylbenzene	9.011	91	4621	0.085	ug/L	98
53) m,p-Xylene	9.136	106	5931	0.284	ug/L	87
54) o-Xylene	9.545	106	8502	0.412	ug/L	95
60) Isopropylbenzene	9.927	105	128073	2.267	ug/L #	86
64) 1,3-Dichlorobenzene	11.181	146	6876	0.245	ug/L	89
65) 1,4-Dichlorobenzene	11.268	146	176375	6.270	ug/L	98
67) 1,2-Dichlorobenzene	11.641	146	15565	0.586	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028126.D
Acq On : 26 Sep 2022 19:09
Operator : SY/MD
Sample : N4820-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8P3

Manual IntegrationsAPPROVED

Quant Time: Sep 26 21:32:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 26 21:28:54 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 09/27/2022
Supervised By :Mahesh Dadoda 09/27/2022

