

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028112.D
 Acq On : 26 Sep 2022 11:25
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Quant Time: Sep 26 21:29:49 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 26 21:28:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.606	114	185124	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	182883	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	84087	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	84497	4.403	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	88.000%	
7) Chloroethane-d5	1.561	69	74088	4.855	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	97.200%	
11) 1,1-Dichloroethene-d2	2.098	63	106857	3.210	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	64.200%	
20) 2-Butanone-d5	3.902	46	163565	50.481	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.960%	
24) Chloroform-d	4.336	84	151832	4.958	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.200%	
26) 1,2-Dichloroethane-d4	5.021	65	72460	4.972	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	99.400%	
32) Benzene-d6	5.037	84	278576	4.646	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.060	67	90046	4.817	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	96.400%	
41) Toluene-d8	7.307	98	214539	3.953	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.000%	
43) trans-1,3-Dichloroprop...	7.619	79	30613	4.533	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	90.600%	
46) 2-Hexanone-d5	8.085	63	135163	47.957	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	95.920%	
56) 1,1,2,2-Tetrachloroeth...	10.211	84	62732	4.909	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.200%	
66) 1,2-Dichlorobenzene-d4	11.619	152	84309	5.112	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.200%	
Target Compounds						
16) Methylene chloride	2.497	84	4079	0.286	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028112.D
Acq On : 26 Sep 2022 11:25
Operator : SY/MD
Sample : VV0926WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Time: Sep 26 21:29:49 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 26 21:28:54 2022
Response via : Initial Calibration

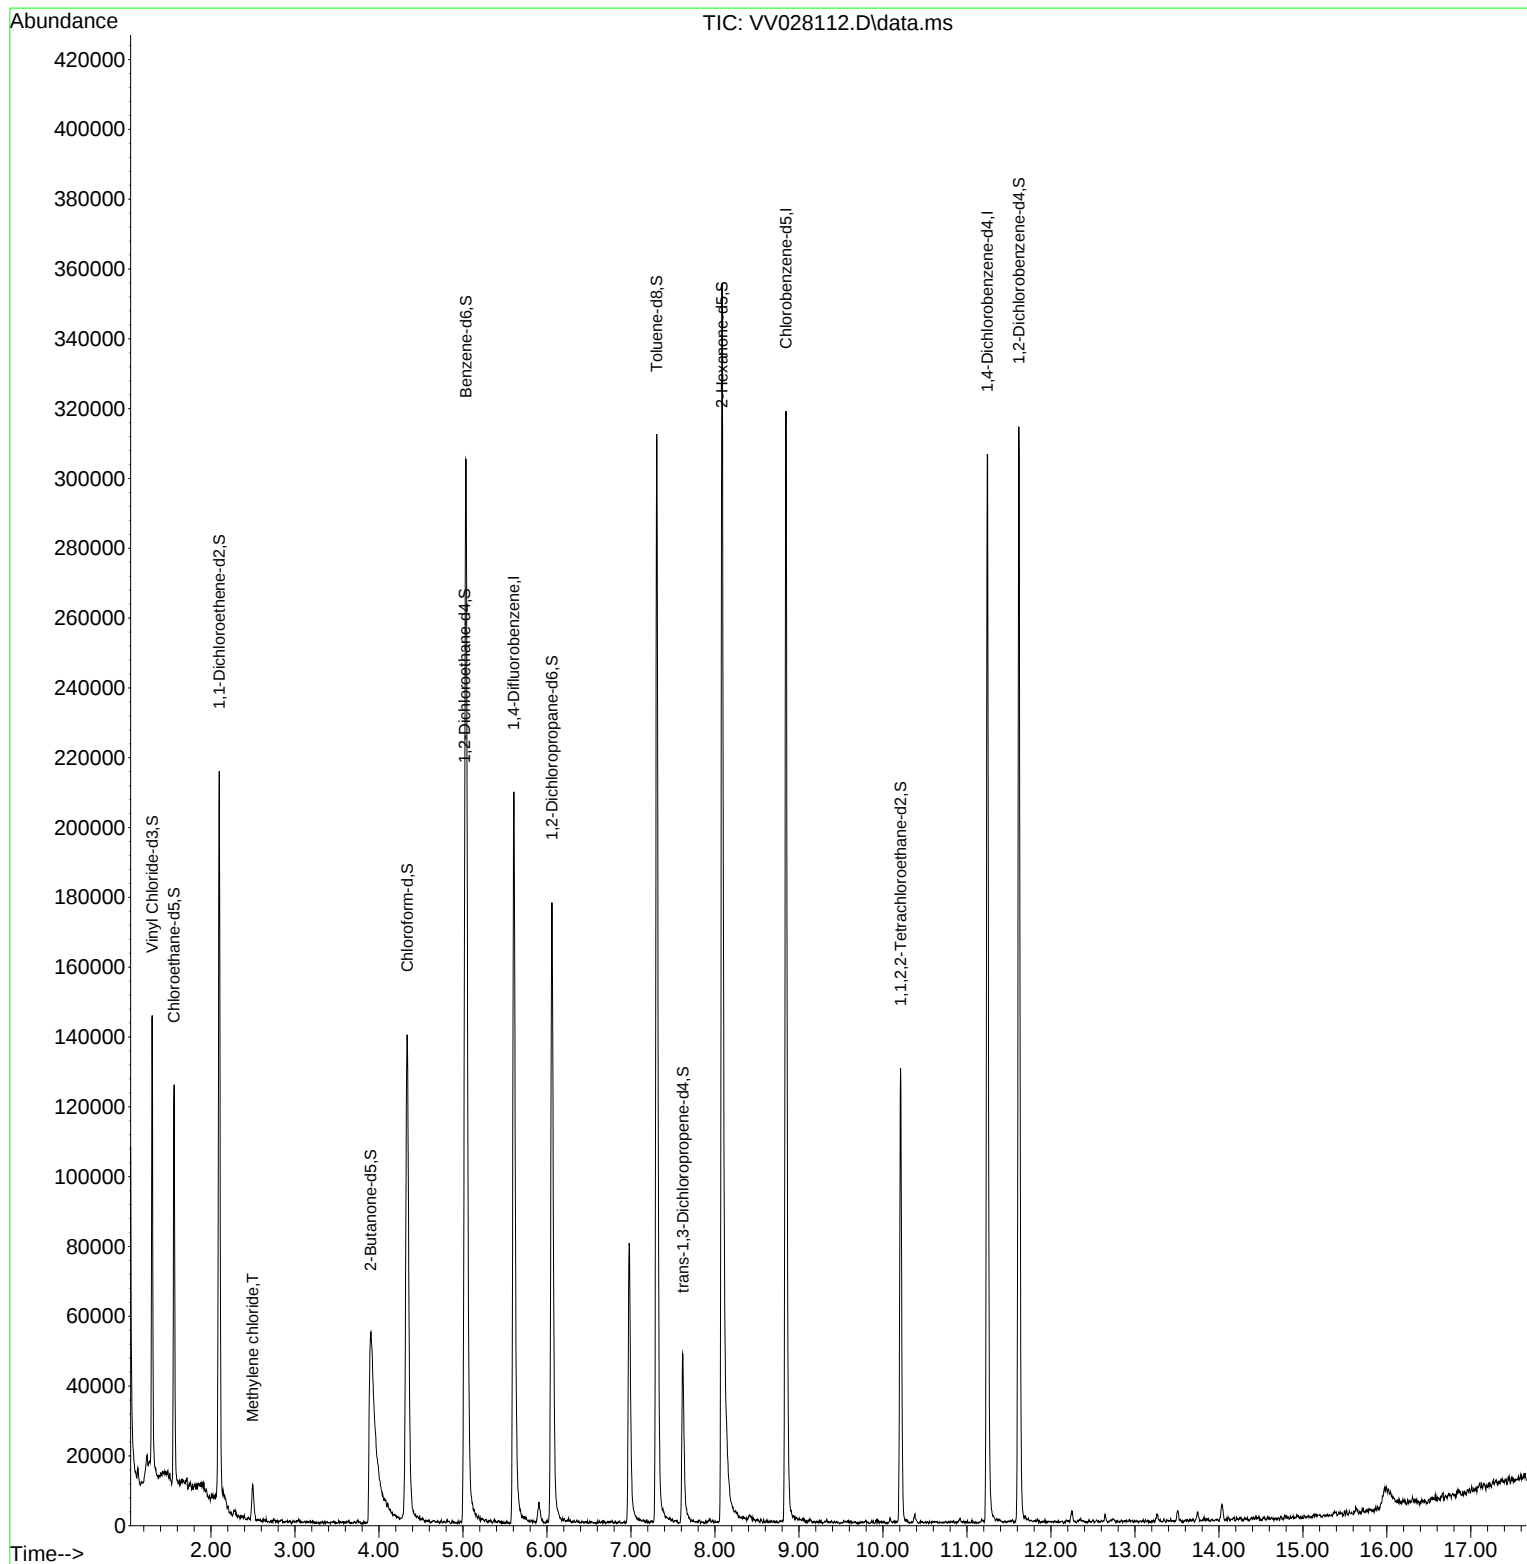

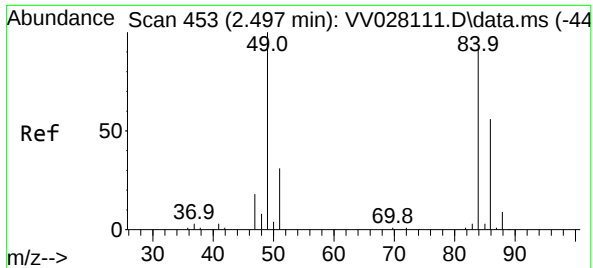

#16
Methylene chloride
Concen: 0.286 ug/L
RT: 2.497 min Scan# 41
Delta R.T. 0.000 min
Lab File: VV028112.D
Acq: 26 Sep 2022 11:25

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Tgt Ion:	84	Resp:	4079
Ion	Ratio	Lower	Upper
84	100		
86	74.3	46.8	86.8
49	134.5	87.5	162.5

