

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028121.D
 Acq On : 26 Sep 2022 17:07
 Operator : SY/MD
 Sample : N4820-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8L8

Quant Time: Sep 26 21:31:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Sep 26 21:28:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	167064	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	168444	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	77836	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.298	65	57596	3.325	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.600%
7) Chloroethane-d5	1.561	69	52367	3.803	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	76.000%
11) 1,1-Dichloroethene-d2	2.098	63	79220	2.637	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	52.800%#
20) 2-Butanone-d5	3.892	46	130203	44.528	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.060%
24) Chloroform-d	4.343	84	115200	4.168	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	83.400%
26) 1,2-Dichloroethane-d4	5.027	65	57841	4.398	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.000%
32) Benzene-d6	5.043	84	208696	3.779	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	75.600%
36) 1,2-Dichloropropane-d6	6.066	67	70800	4.112	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	82.200%
41) Toluene-d8	7.313	98	158008	3.161	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	63.200%#
43) trans-1,3-Dichloroprop...	7.622	79	22193	3.568	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.400%
46) 2-Hexanone-d5	8.088	63	103238	39.770	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.540%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	49803	4.232	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.600%
66) 1,2-Dichlorobenzene-d4	11.622	152	66966	4.386	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.800%
Target Compounds					Qvalue	
13) Acetone	2.185	43	10002	4.441	ug/L	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028121.D
Acq On : 26 Sep 2022 17:07
Operator : SY/MD
Sample : N4820-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CB8L8

Quant Time: Sep 26 21:31:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Sep 26 21:28:54 2022
Response via : Initial Calibration

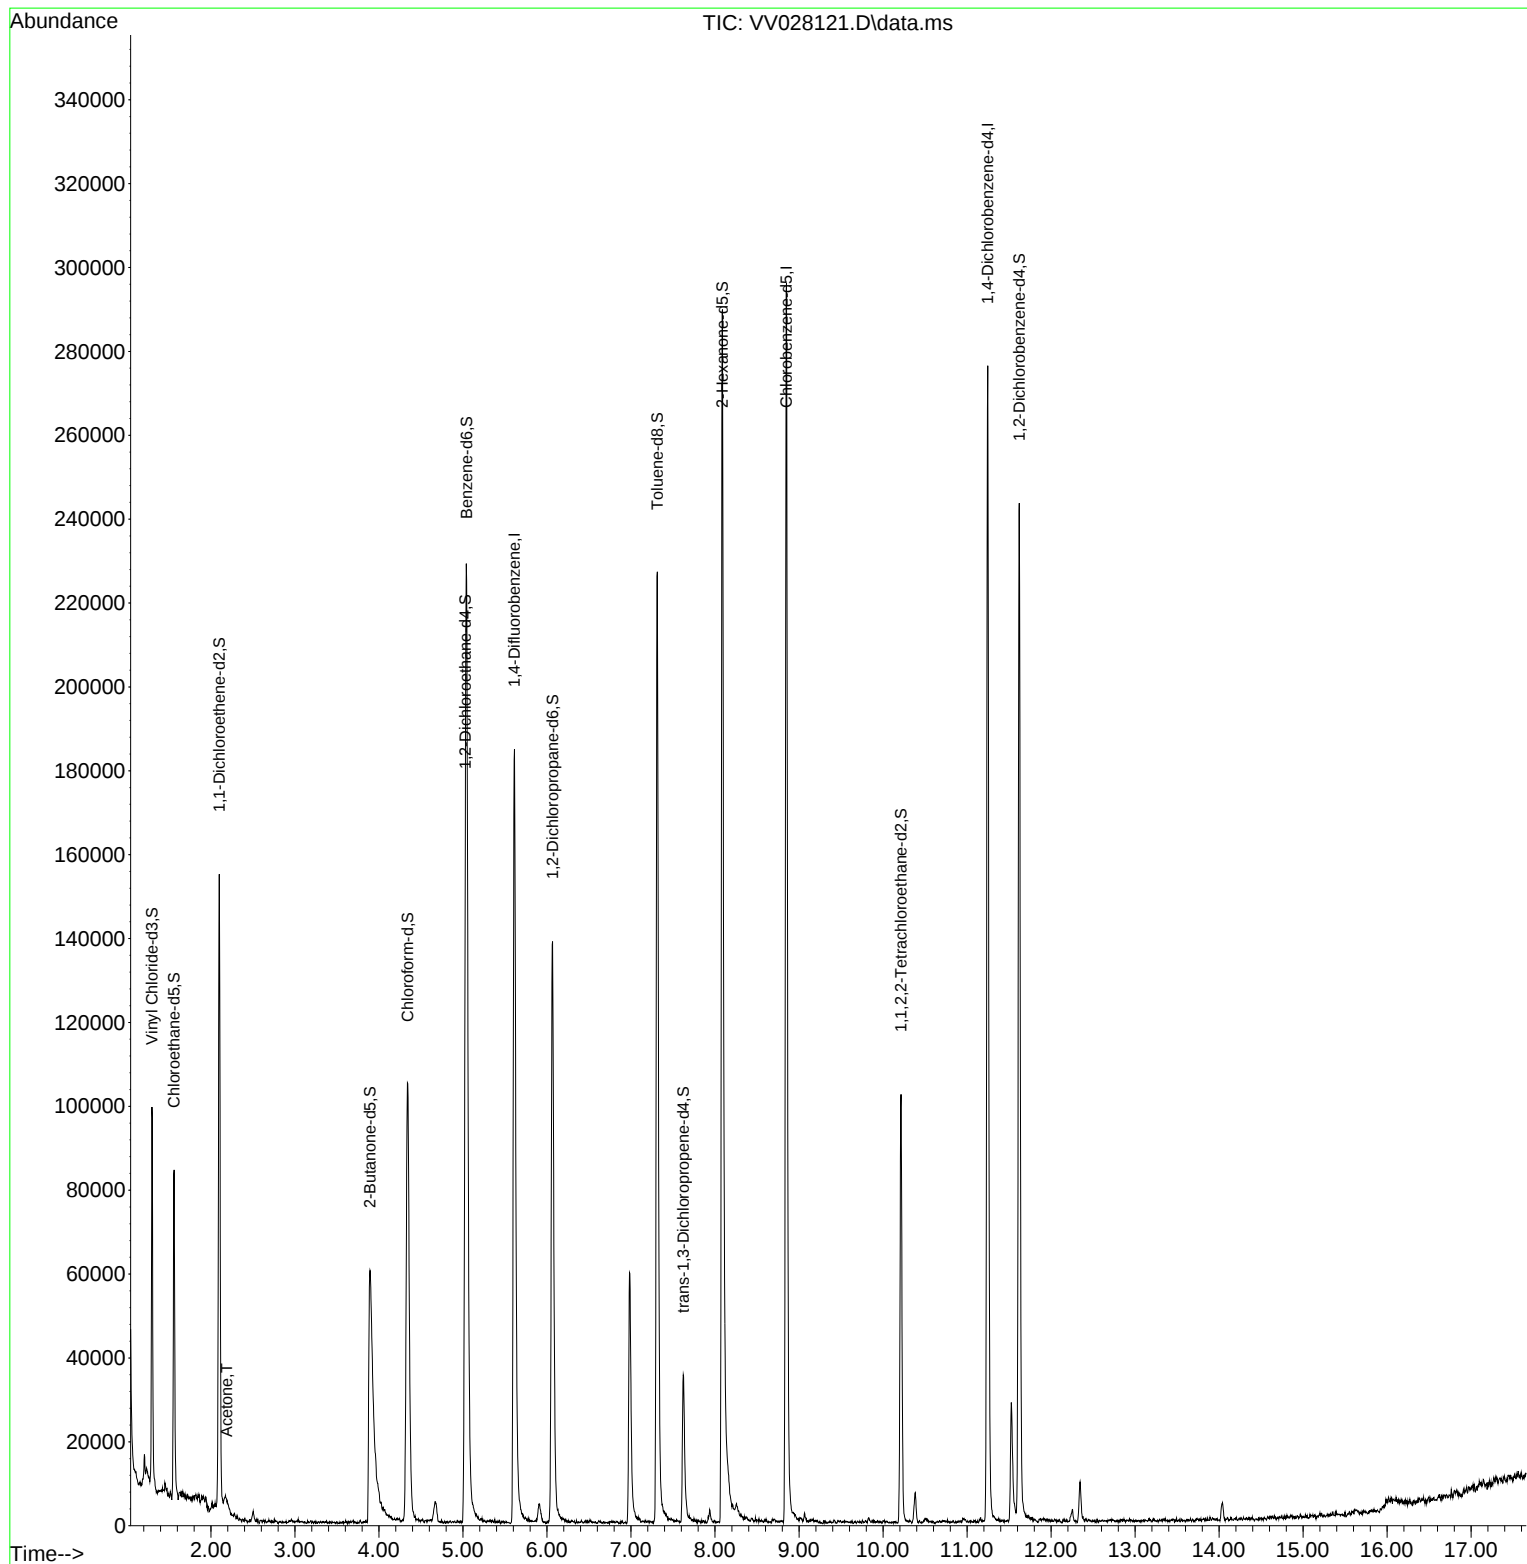

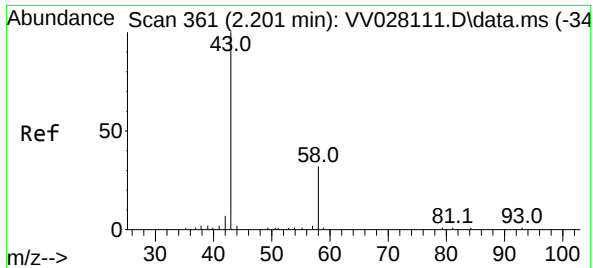

#13
 Acetone
 Concen: 4.441 ug/L
 RT: 2.185 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV028121.D
 Acq: 26 Sep 2022 17:07

Instrument :
 MSVOA_V
 ClientSampleId :
 CB8L8

Tgt Ion: 43 Resp: 10002
 Ion Ratio Lower Upper
 43 100
 58 13.8 0.0 65.6

