

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028112.D
 Acq On : 26 Sep 2022 11:25
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028112.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	93	rVB	130049	134275	17.63%	2.222%
2	1.561	155	162	173	rBV	113331	127443	16.73%	2.109%
3	2.098	318	329	341	rBV	207625	289285	37.98%	4.787%
4	2.497	444	453	466	rVB2	10380	18849	2.47%	0.312%
5	3.905	876	891	933	rBV2	54808	275331	36.15%	4.556%
6	4.336	1006	1025	1048	rBV2	138467	350804	46.06%	5.805%
7	5.034	1227	1242	1271	rBV2	304560	761592	100.00%	12.602%
8	5.606	1408	1420	1444	rBV	209587	431555	56.66%	7.141%
9	5.905	1504	1513	1523	rBV10	5685	10270	1.35%	0.170%
10	6.060	1548	1561	1591	rBV	177600	376847	49.48%	6.236%
11	6.979	1835	1847	1871	rBV2	80127	156295	20.52%	2.586%
12	7.307	1935	1949	1970	rBV	311805	554308	72.78%	9.172%
13	7.616	2035	2045	2059	rBV	48650	89988	11.82%	1.489%
14	8.085	2178	2191	2230	rBV	354948	732888	96.23%	12.127%
15	8.847	2416	2428	2452	rBV	318115	531249	69.76%	8.790%
16	10.211	2838	2852	2869	rBV	130189	208460	27.37%	3.449%
17	11.243	3162	3173	3193	rBV	305950	486347	63.86%	8.047%
18	11.619	3278	3290	3309	rBV	313629	498646	65.47%	8.251%
19	14.037	4031	4042	4052	rBV2	4903	9130	1.20%	0.151%




Sum of corrected areas: 6043562

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028112.D
Acq On : 26 Sep 2022 11:25
Operator : SY/MD
Sample : VV0926WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

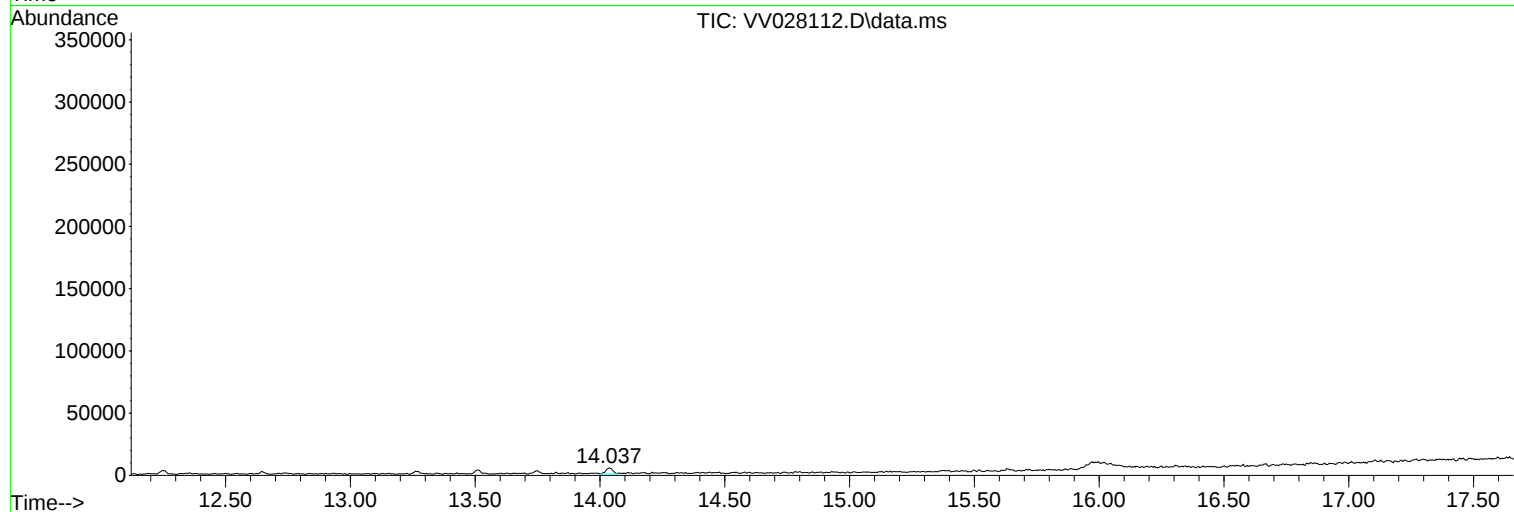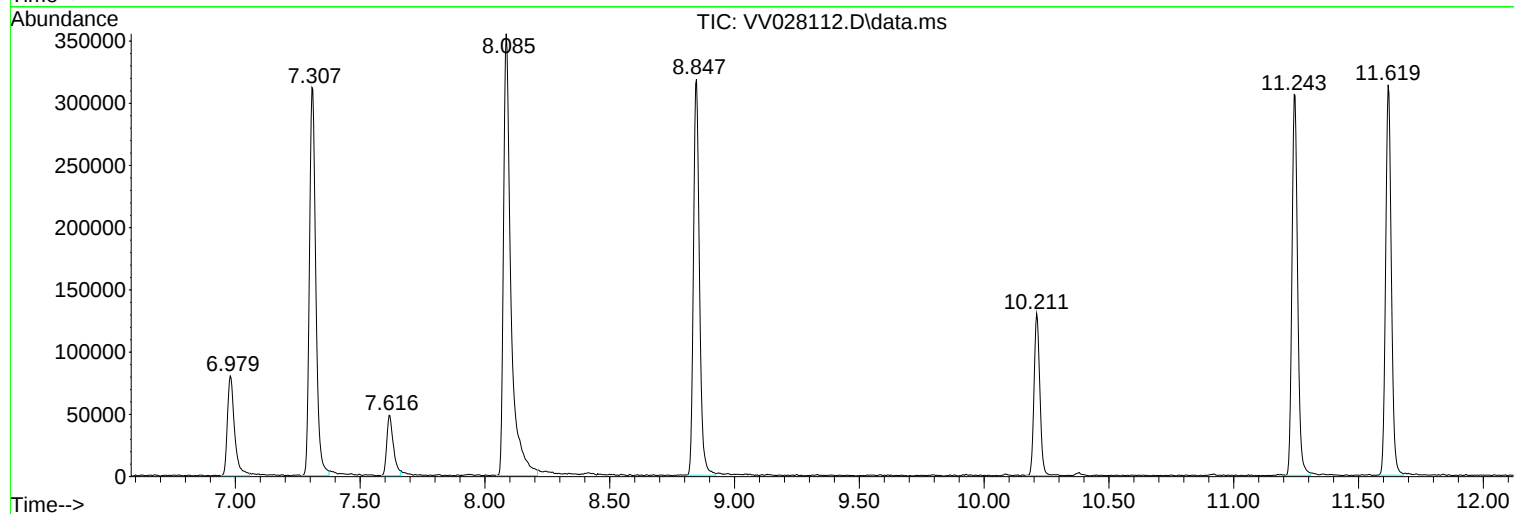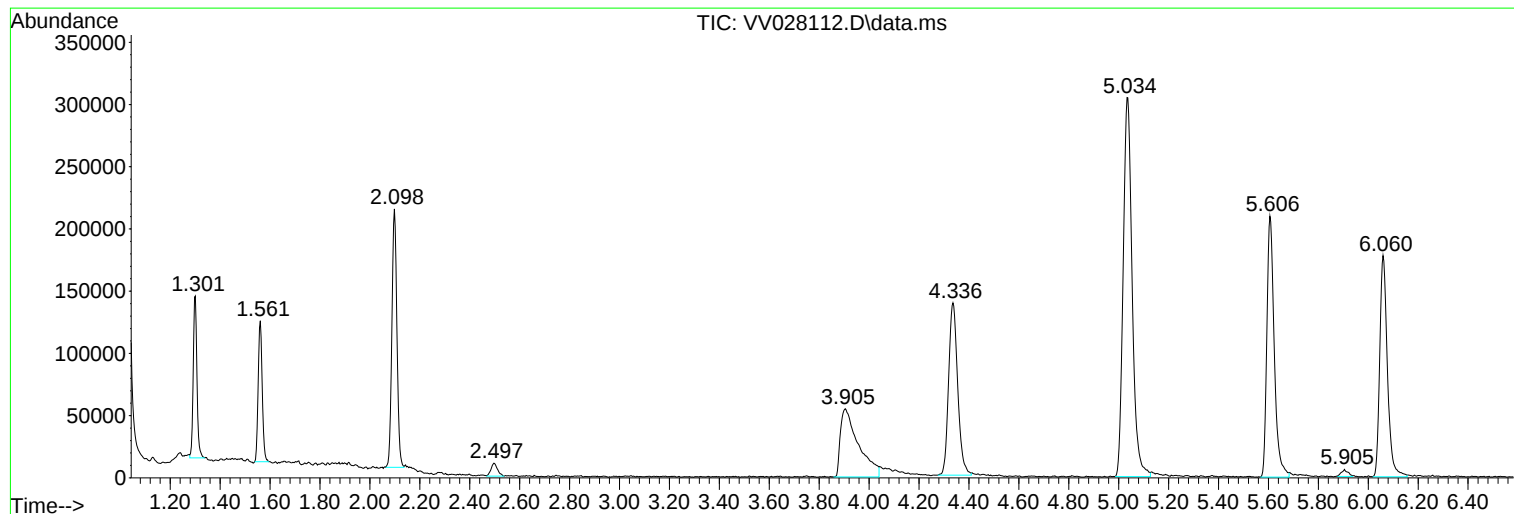

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028112.D
Acq On : 26 Sep 2022 11:25
Operator : SY/MD
Sample : VV0926WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028112.D
Acq On : 26 Sep 2022 11:25
Operator : SY/MD
Sample : VV0926WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc