

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
 Data File : VV028120.D
 Acq On : 26 Sep 2022 16:43
 Operator : SY/MD
 Sample : VIBLK295
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK295

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	93	rVB	104711	104760	16.48%	2.006%
2	1.561	155	162	173	rBV	87521	101776	16.01%	1.949%
3	2.101	319	330	344	rBV	162203	232314	36.54%	4.448%
4	2.500	444	454	467	rBV	18602	31830	5.01%	0.609%
5	3.889	875	886	929	rBV	77185	269424	42.38%	5.159%
6	4.343	1007	1027	1053	rBV2	116740	297107	46.73%	5.689%
7	5.040	1227	1244	1273	rBV2	249503	633151	99.59%	12.123%
8	5.613	1409	1422	1445	rBV	178018	374488	58.91%	7.171%
9	5.908	1505	1514	1530	rVB	4382	9940	1.56%	0.190%
10	6.066	1546	1563	1581	rBV	154682	319837	50.31%	6.124%
11	6.986	1838	1849	1867	rBV2	66768	127415	20.04%	2.440%
12	7.313	1939	1951	1976	rBV	254769	461964	72.67%	8.845%
13	7.622	2037	2047	2066	rBV2	38219	74419	11.71%	1.425%
14	8.085	2177	2191	2237	rBV	328872	635731	100.00%	12.173%
15	8.850	2417	2429	2449	rBV	281172	475086	74.73%	9.097%
16	10.214	2840	2853	2867	rBV	112148	180886	28.45%	3.464%
17	10.381	2896	2905	2916	rBV	6405	9960	1.57%	0.191%
18	11.246	3163	3174	3194	rBV	276297	433521	68.19%	8.301%
19	11.622	3279	3291	3309	rBV	266076	423822	66.67%	8.115%
20	12.246	3476	3485	3496	rBV2	4447	7381	1.16%	0.141%
21	15.927	4615	4630	4631	rBV2	10534	17794	2.80%	0.341%




Sum of corrected areas: 5222606

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028120.D
Acq On : 26 Sep 2022 16:43
Operator : SY/MD
Sample : VIBLK295
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

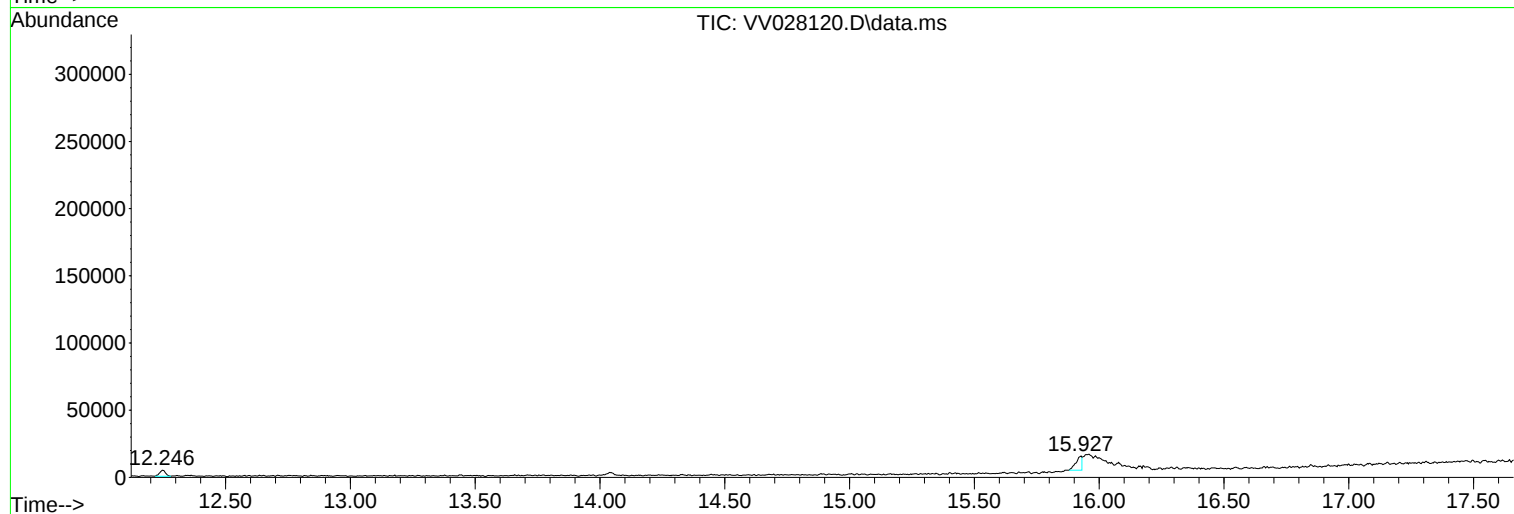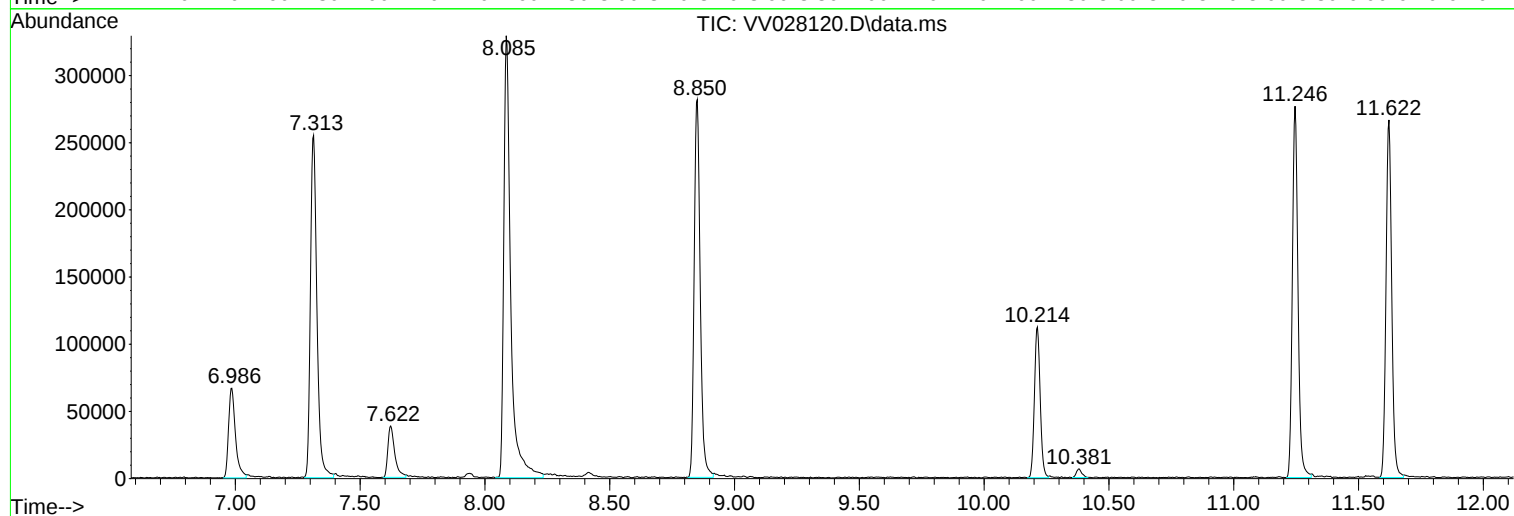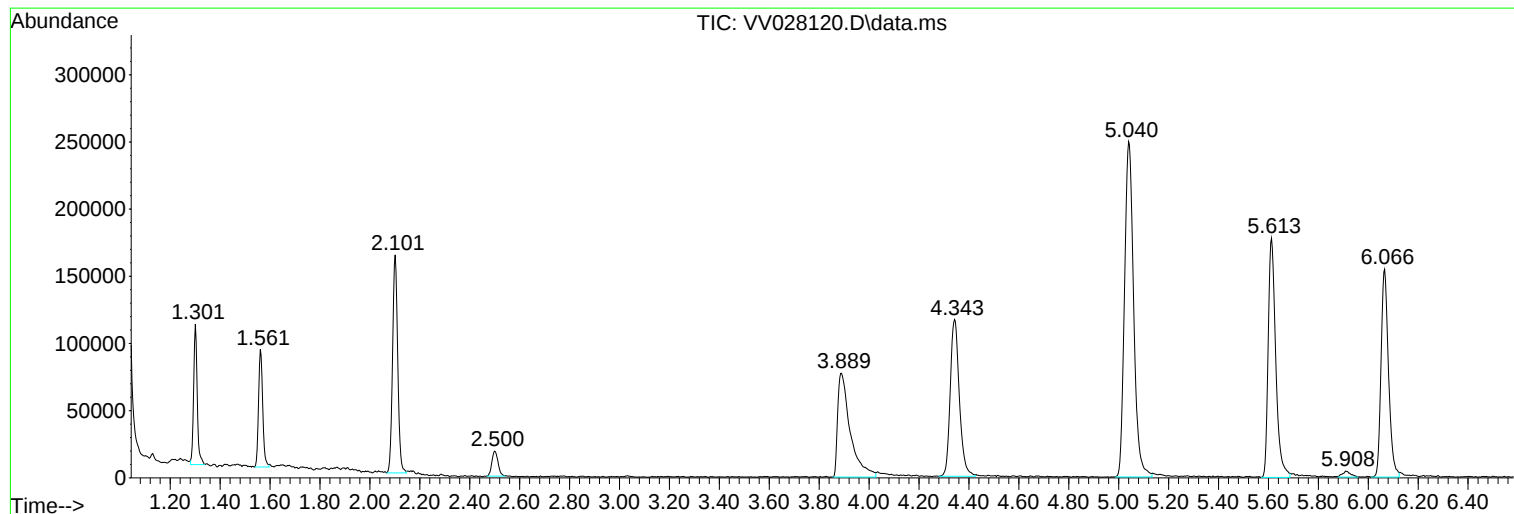

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028120.D
Acq On : 26 Sep 2022 16:43
Operator : SY/MD
Sample : VIBLK295
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092622\
Data File : VV028120.D
Acq On : 26 Sep 2022 16:43
Operator : SY/MD
Sample : VIBLK295
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK295

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------