




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV092624\  
 Data File : VV037572.D  
 Acq On : 27 Sep 2024 00:48  
 Operator : SY/MD  
 Sample : P4184-18  
 Misc : 5mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EY044

Manual IntegrationsAPPROVED

Quant Time: Sep 27 03:40:08 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Sep 27 02:22:28 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2024  
 Supervised By :Mahesh Dadoda 09/30/2024

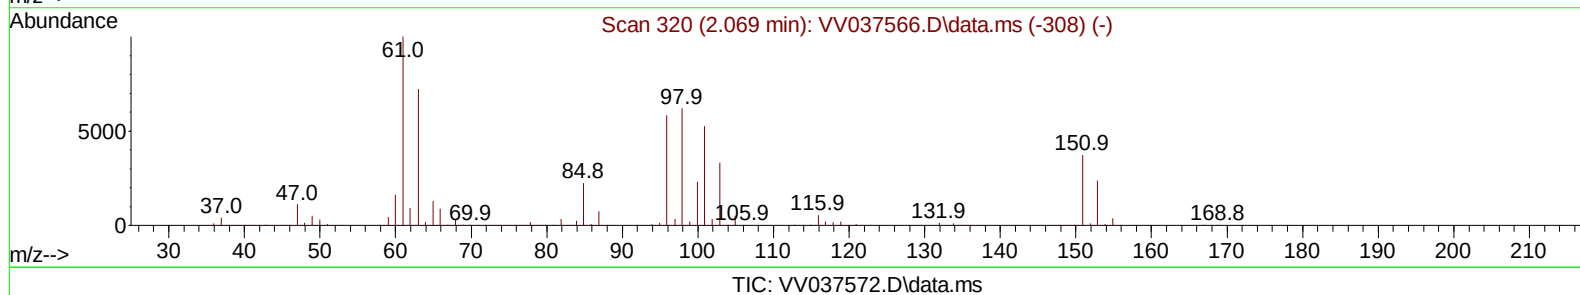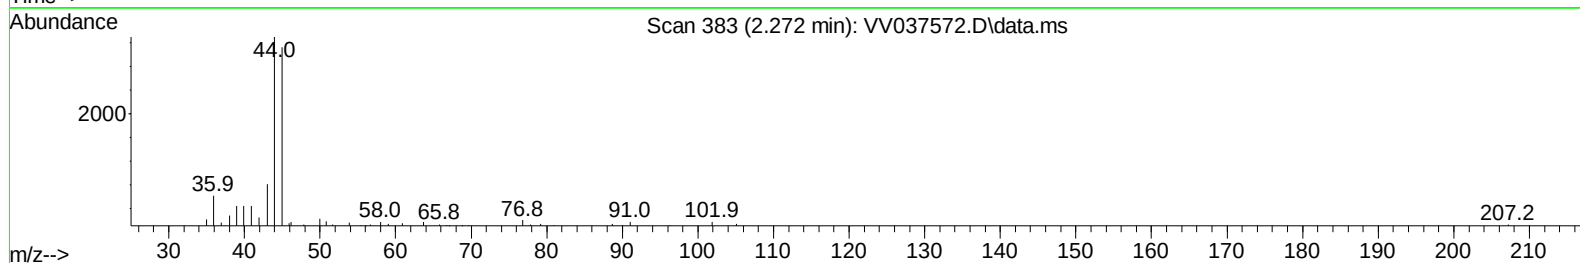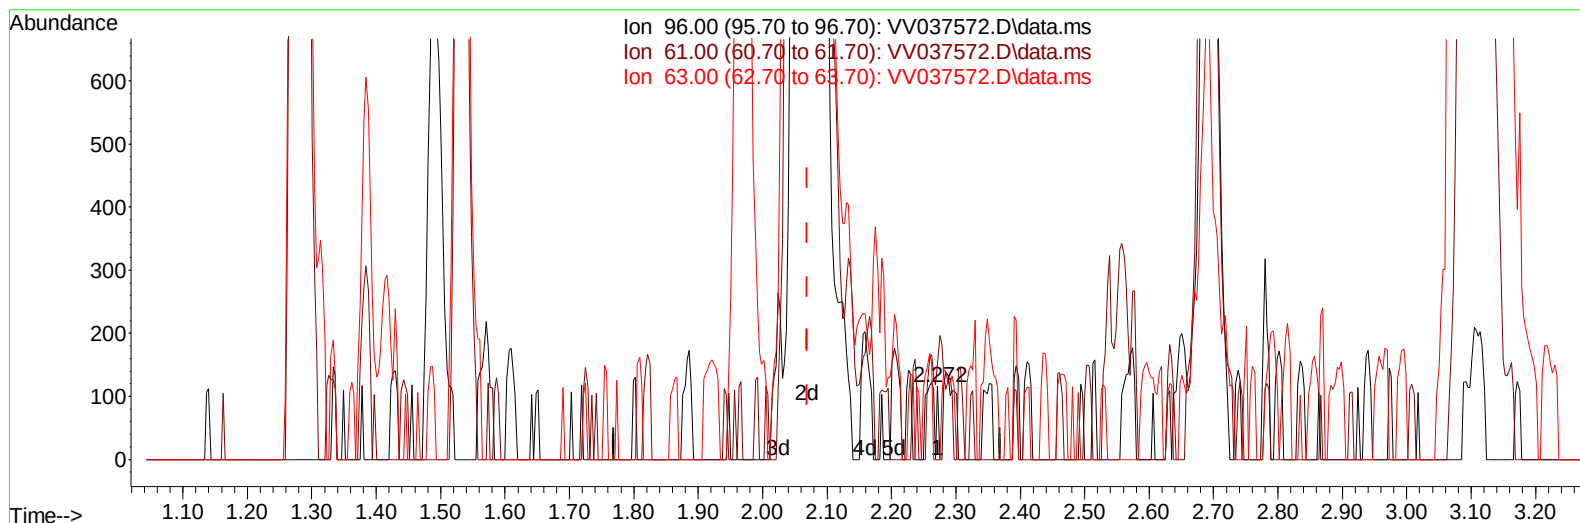

(12) 1,1-Dichloroethene (T)

2.272min (+ 0.202) 0.00 ug/L

response 22

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 96.00 | 100.00 | 100.00 |
| 61.00 | 175.10 | 131.03 |
| 63.00 | 168.60 | 143.10 |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV092624\  
Data File : VV037572.D  
Acq On : 27 Sep 2024 00:48  
Operator : SY/MD  
Sample : P4184-18  
Misc : 5mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EY044

## Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 09/30/2024  
Supervised By :Mahesh Dadoda 09/30/2024

Quant Time: Sep 27 03:40:08 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Sep 27 02:22:28 2024  
Response via : Initial Calibration

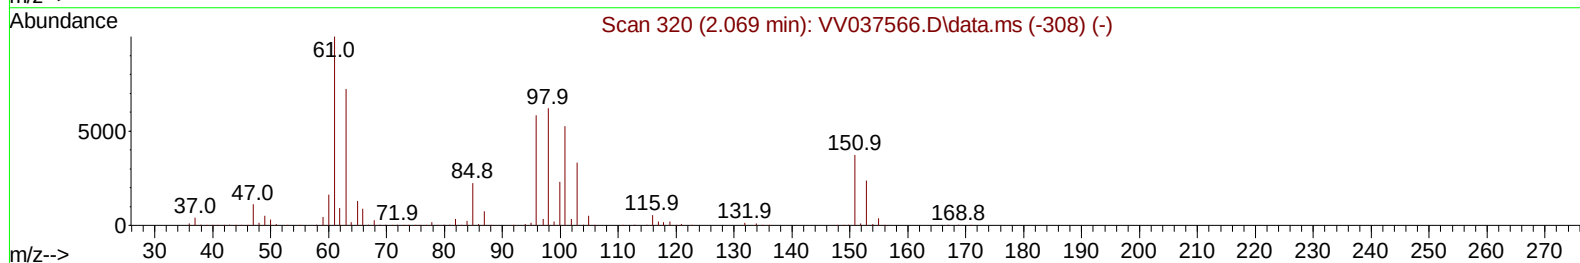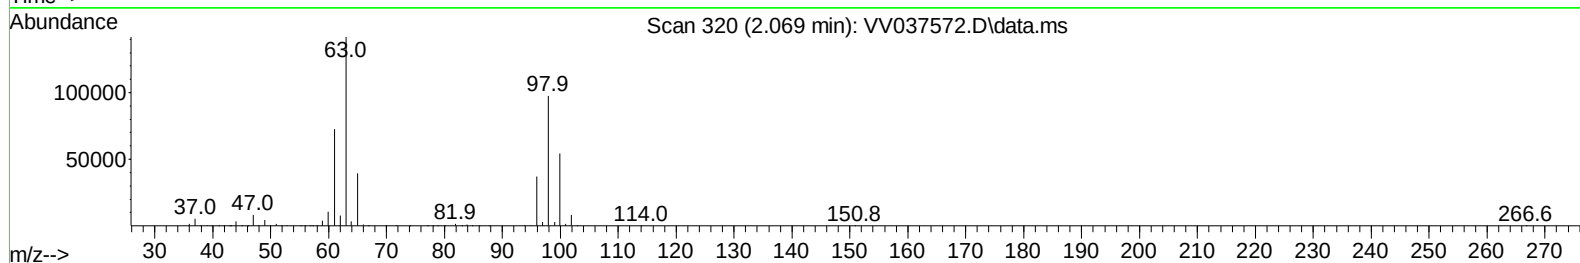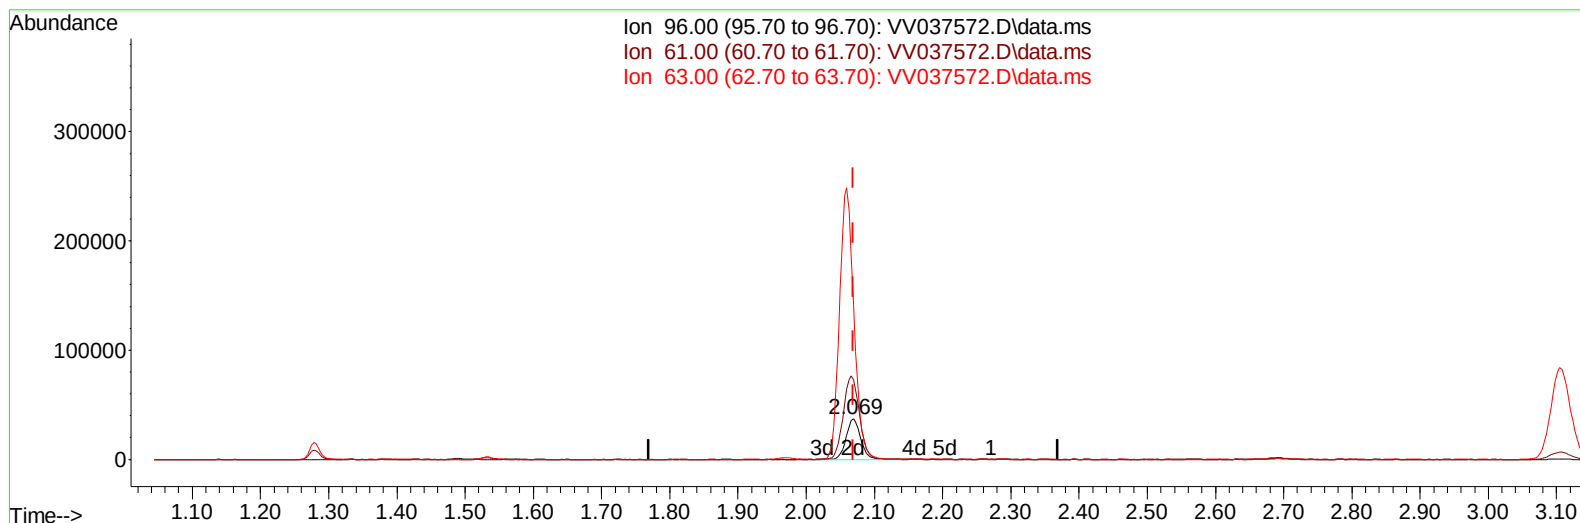

TIC: VV037572.D\data.ms

## (12) 1,1-Dichloroethene (T)

2.069min (-0.000) 12.35 ug/L m

response 54644

| Ion   | Exp%   | Act%    |
|-------|--------|---------|
| 96.00 | 100.00 | 100.00  |
| 61.00 | 175.10 | 196.76  |
| 63.00 | 168.60 | 382.89# |
| 0.00  | 0.00   | 0.00    |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV092624\  
 Data File : VV037572.D  
 Acq On : 27 Sep 2024 00:48  
 Operator : SY/MD  
 Sample : P4184-18  
 Misc : 5mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 EY044

Manual IntegrationsAPPROVED

Quant Time: Sep 27 03:40:08 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Fri Sep 27 02:22:28 2024  
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2024  
 Supervised By :Mahesh Dadoda 09/30/2024

| Compound                      | R.T.     | QIon  | Response | Conc    | Units   | Dev(Min) |
|-------------------------------|----------|-------|----------|---------|---------|----------|
| -----                         |          |       |          |         |         |          |
| Internal Standards            |          |       |          |         |         |          |
| 1) 1,4-Difluorobenzene        | 5.529    | 114   | 664545   | 50.000  | ug/L    | 0.00     |
| 28) Chlorobenzene-d5          | 8.780    | 117   | 630233   | 50.000  | ug/L    | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.178   | 152   | 306348   | 50.000  | ug/L    | 0.00     |
| System Monitoring Compounds   |          |       |          |         |         |          |
| 4) Vinyl Chloride-d3          | 1.278    | 65    | 252299   | 43.249  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 135 | Recovery | =       | 86.500% |          |
| 7) Chloroethane-d5            | 1.532    | 69    | 200474   | 44.273  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 130 | Recovery | =       | 88.540% |          |
| 11) 1,1-Dichloroethene-d2     | 2.060    | 65    | 108378   | 44.468  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery | =       | 88.940% |          |
| 21) 2-Butanone-d5             | 3.793    | 46    | 190296   | 91.584  | ug/L    | 0.00     |
| Spiked Amount 100.000         | Range 40 | - 130 | Recovery | =       | 91.580% |          |
| 24) Chloroform-d              | 4.243    | 84    | 450344   | 43.391  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =       | 86.780% |          |
| 26) 1,2-Dichloroethane-d4     | 4.937    | 65    | 269764   | 44.406  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =       | 88.820% |          |
| 32) Benzene-d6                | 4.953    | 84    | 898120   | 45.541  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 125 | Recovery | =       | 91.080% |          |
| 36) 1,2-Dichloropropane-d6    | 5.982    | 67    | 286126   | 45.563  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 70 | - 120 | Recovery | =       | 91.120% |          |
| 41) Toluene-d8                | 7.236    | 98    | 801223   | 44.805  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery | =       | 89.600% |          |
| 43) trans-1,3-Dichloroprop... | 7.551    | 79    | 122104   | 41.856  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 60 | - 125 | Recovery | =       | 83.720% |          |
| 47) 2-Hexanone-d5             | 8.024    | 63    | 116588   | 87.922  | ug/L    | 0.00     |
| Spiked Amount 100.000         | Range 45 | - 130 | Recovery | =       | 87.920% |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.146   | 84    | 319651   | 43.808  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 65 | - 120 | Recovery | =       | 87.620% |          |
| 66) 1,2-Dichlorobenzene-d4    | 11.554   | 152   | 300128   | 46.493  | ug/L    | 0.00     |
| Spiked Amount 50.000          | Range 80 | - 120 | Recovery | =       | 92.980% |          |
| Target Compounds              |          |       |          |         |         |          |
|                               |          |       |          |         |         | Qvalue   |
| 12) 1,1-Dichloroethene        | 2.069    | 96    | 54644m   | 12.351  | ug/L    |          |
| 13) Acetone                   | 2.114    | 43    | 38852    | 19.074  | ug/L    | 100      |
| 19) 1,1-Dichloroethane        | 3.105    | 63    | 170282   | 18.989  | ug/L    | 99       |
| 20) cis-1,2-Dichloroethene    | 3.809    | 96    | 94725    | 18.086  | ug/L    | 100      |
| 30) 1,1,1-Trichloroethane     | 4.503    | 97    | 2162404  | 278.583 | ug/L    | 100      |
| 34) Trichloroethene           | 5.828    | 95    | 186456   | 36.836  | ug/L    | 99       |
| 46) Tetrachloroethene         | 7.899    | 164   | 408871   | 105.648 | ug/L    | 99       |
| -----                         |          |       |          |         |         |          |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV092624\  
Data File : VV037572.D  
Acq On : 27 Sep 2024 00:48  
Operator : SY/MD  
Sample : P4184-18  
Misc : 5mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
EY044

Manual IntegrationsAPPROVED

Quant Time: Sep 27 03:40:08 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
Quant Title : VOC Analysis  
QLast Update : Fri Sep 27 02:22:28 2024  
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 09/30/2024  
Supervised By :Mahesh Dadoda 09/30/2024

