

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037542.D
 Acq On : 26 Sep 2024 13:00
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037542.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV	12999	21737	0.72%	0.103%
2	1.278	67	74	92	rVB	441220	465706	15.50%	2.213%
3	1.532	146	153	167	rVB	364497	423873	14.11%	2.014%
4	2.060	307	317	335	rBV	739700	1064918	35.45%	5.060%
5	3.542	775	778	782	rBV3	941	724	0.02%	0.003%
6	3.658	811	814	819	rVB4	668	500	0.02%	0.002%
7	3.683	819	822	824	rBV2	429	250	0.01%	0.001%
8	3.696	824	826	829	rBV3	547	279	0.01%	0.001%
9	3.738	836	839	841	rBV2	726	434	0.01%	0.002%
10	3.796	848	857	899	rBV	134844	413266	13.76%	1.964%
11	4.243	981	996	1028	rVB	480931	1212269	40.36%	5.760%
12	4.645	1119	1121	1124	rBV4	736	446	0.01%	0.002%
13	4.677	1126	1131	1135	rVB5	757	859	0.03%	0.004%
14	4.706	1137	1140	1142	rBV2	593	410	0.01%	0.002%
15	4.732	1143	1148	1149	rBV3	817	650	0.02%	0.003%
16	4.796	1164	1168	1170	rBV4	463	345	0.01%	0.002%
17	4.831	1177	1179	1180	rBV2	469	158	0.01%	0.001%
18	4.841	1180	1182	1185	rBV4	540	429	0.01%	0.002%
19	4.857	1185	1187	1190	rVV3	576	311	0.01%	0.001%
20	4.889	1195	1197	1200	rVB2	687	343	0.01%	0.002%
21	4.950	1200	1216	1251	rBV2	1185415	3003617	100.00%	14.271%
22	5.285	1316	1320	1323	rBV5	969	1091	0.04%	0.005%
23	5.436	1364	1367	1368	rBV2	950	535	0.02%	0.003%
24	5.484	1379	1382	1385	rBV4	954	720	0.02%	0.003%
25	5.529	1385	1396	1430	rBV	757960	1568204	52.21%	7.451%
26	5.982	1525	1537	1570	rBV	660434	1361233	45.32%	6.468%
27	6.294	1632	1634	1635	rBV2	699	326	0.01%	0.002%
28	6.452	1681	1683	1686	rVB2	766	399	0.01%	0.002%
29	6.465	1686	1687	1689	rBV2	489	214	0.01%	0.001%
30	6.535	1707	1709	1712	rBV3	538	295	0.01%	0.001%
31	6.612	1731	1733	1735	rVB2	488	201	0.01%	0.001%
32	6.645	1741	1743	1747	rBV3	618	432	0.01%	0.002%
33	6.667	1747	1750	1753	rBV3	374	281	0.01%	0.001%
34	6.728	1763	1769	1773	rBV6	887	896	0.03%	0.004%
35	6.780	1783	1785	1789	rBV4	581	445	0.01%	0.002%
36	6.841	1799	1804	1808	rVB3	633	564	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037542.D
 Acq On : 26 Sep 2024 13:00
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1815	1825	1848	rBV	347664	662955	22.07%	3.150%
38	7.101	1884	1885	1890	rBV4	1084	698	0.02%	0.003%
39	7.236	1916	1927	1973	rBV	1343483	2375910	79.10%	11.289%
40	7.548	2015	2024	2054	rBV	234467	432517	14.40%	2.055%
41	7.911	2129	2137	2146	rVB	2847	5175	0.17%	0.025%
42	7.960	2150	2152	2154	rBV2	706	368	0.01%	0.002%
43	8.024	2163	2172	2216	rBV2	394143	857747	28.56%	4.075%
44	8.628	2358	2360	2363	rBV3	597	433	0.01%	0.002%
45	8.686	2375	2378	2380	rBV4	980	663	0.02%	0.003%
46	8.780	2395	2407	2432	rBV	1144389	1939571	64.57%	9.216%
47	9.217	2541	2543	2545	rBV2	486	268	0.01%	0.001%
48	9.278	2559	2562	2565	rVB3	1188	671	0.02%	0.003%
49	9.294	2565	2567	2570	rBV2	587	355	0.01%	0.002%
50	9.371	2589	2591	2593	rBV2	815	420	0.01%	0.002%
51	9.394	2596	2598	2601	rBV4	447	315	0.01%	0.001%
52	9.429	2605	2609	2613	rBV4	1155	977	0.03%	0.005%
53	9.487	2621	2627	2628	rBV4	1496	1586	0.05%	0.008%
54	9.603	2660	2663	2665	rVB4	557	286	0.01%	0.001%
55	9.741	2704	2706	2707	rBV2	444	215	0.01%	0.001%
56	9.825	2729	2732	2736	rBV4	469	375	0.01%	0.002%
57	9.844	2736	2738	2740	rBV2	508	297	0.01%	0.001%
58	9.960	2773	2774	2777	rBV3	453	202	0.01%	0.001%
59	9.989	2780	2783	2785	rBV2	854	484	0.02%	0.002%
60	10.001	2785	2787	2789	rBV	580	245	0.01%	0.001%
61	10.017	2790	2792	2794	rBV3	630	239	0.01%	0.001%
62	10.050	2799	2802	2808	rVB3	891	752	0.03%	0.004%
63	10.075	2808	2810	2812	rBV	380	189	0.01%	0.001%
64	10.146	2820	2832	2851	rBV	771807	1218603	40.57%	5.790%
65	10.419	2913	2917	2918	rBV4	736	559	0.02%	0.003%
66	10.455	2926	2928	2929	rBV	424	221	0.01%	0.001%
67	10.522	2948	2949	2952	rVB	936	273	0.01%	0.001%
68	10.571	2962	2964	2965	rBV	999	407	0.01%	0.002%
69	10.590	2969	2970	2973	rVB2	716	260	0.01%	0.001%
70	10.622	2977	2980	2981	rBV3	375	188	0.01%	0.001%
71	10.632	2981	2983	2987	rVB3	634	425	0.01%	0.002%
72	10.664	2987	2993	2994	rBV2	740	640	0.02%	0.003%
73	10.673	2994	2996	2999	rBV4	638	235	0.01%	0.001%
74	10.706	3004	3006	3010	rVB4	783	485	0.02%	0.002%
75	10.731	3011	3014	3018	rBV4	769	606	0.02%	0.003%
76	10.783	3026	3030	3036	rBV5	2010	2106	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037542.D
 Acq On : 26 Sep 2024 13:00
 Operator : SY/MD
 Sample : VV0926WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK213

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.960	3083	3085	3088	rBV3	606	403	0.01%	0.002%
78	11.037	3105	3109	3111	rBV4	930	655	0.02%	0.003%
79	11.091	3122	3126	3128	rBV3	549	403	0.01%	0.002%
80	11.127	3131	3137	3138	rBV4	3983	3807	0.13%	0.018%
81	11.178	3143	3153	3185	rVV	1132994	1819039	60.56%	8.643%
82	11.500	3250	3253	3256	rBV4	878	678	0.02%	0.003%
83	11.554	3258	3270	3295	rBV	1323021	2122665	70.67%	10.086%
84	12.001	3406	3409	3410	rBV2	553	245	0.01%	0.001%
85	12.098	3434	3439	3440	rBV3	1172	881	0.03%	0.004%
86	12.230	3478	3480	3483	rVB3	1017	423	0.01%	0.002%
87	12.275	3492	3494	3495	rBV2	531	225	0.01%	0.001%
88	12.416	3536	3538	3539	rBV	822	352	0.01%	0.002%
89	12.445	3543	3547	3550	rVV4	706	688	0.02%	0.003%
90	12.493	3560	3562	3566	rVB3	865	464	0.02%	0.002%
91	12.583	3584	3590	3593	rBV6	4015	4308	0.14%	0.020%
92	12.956	3701	3706	3709	rBV3	1083	932	0.03%	0.004%
93	13.088	3746	3747	3749	rBV2	734	278	0.01%	0.001%
94	13.207	3778	3784	3796	rVB6	6658	10947	0.36%	0.052%
95	13.316	3815	3818	3822	rVB2	918	490	0.02%	0.002%
96	13.400	3841	3844	3847	rBV4	740	632	0.02%	0.003%
97	13.448	3851	3859	3873	rVV3	9570	19334	0.64%	0.092%
98	13.574	3896	3898	3902	rBV4	1191	849	0.03%	0.004%
99	13.648	3915	3921	3923	rBV3	998	968	0.03%	0.005%
100	14.271	4113	4115	4119	rBV4	930	684	0.02%	0.003%

Sum of corrected areas: 21046631




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037542.D
Acq On : 26 Sep 2024 13:00
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

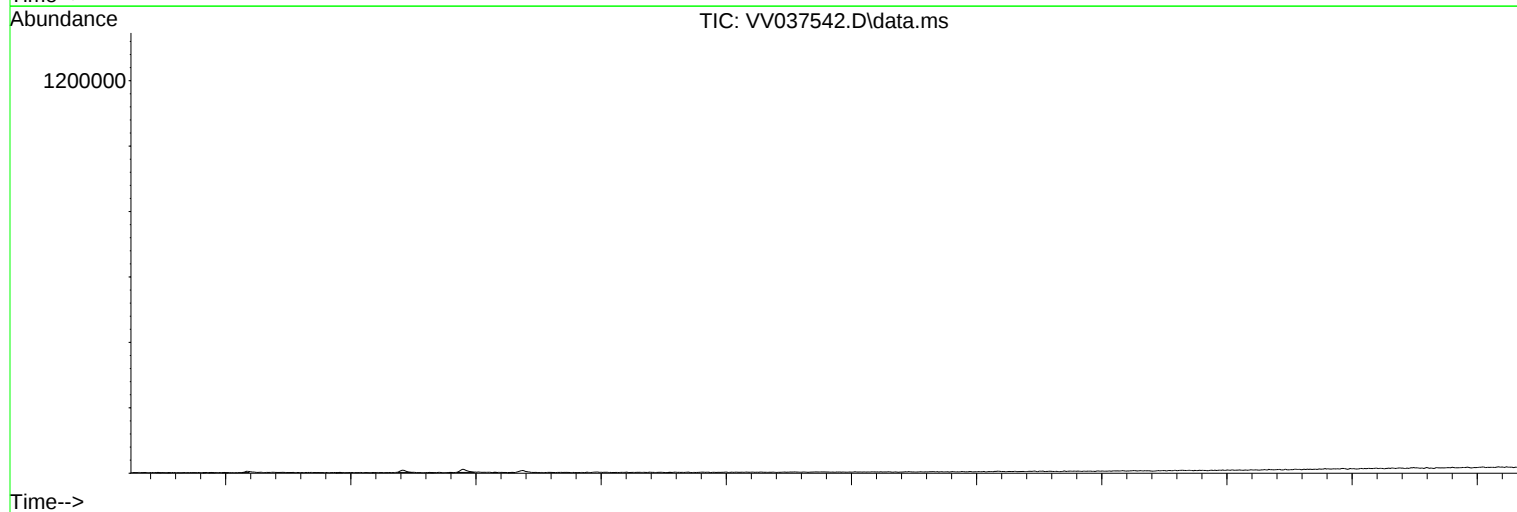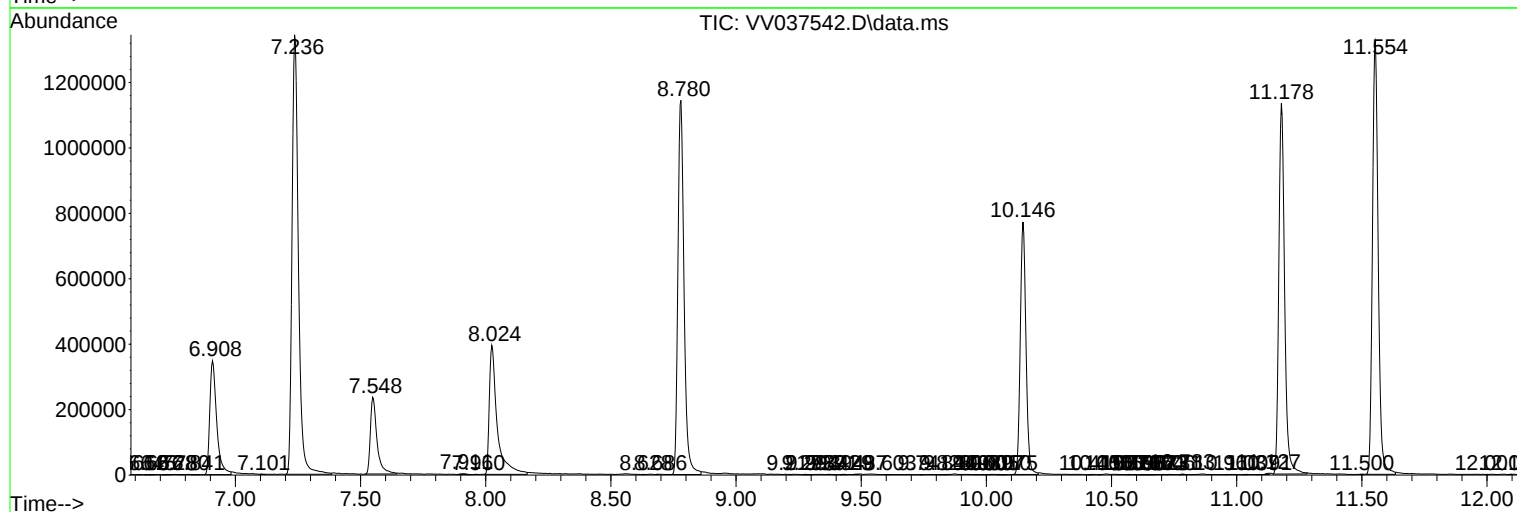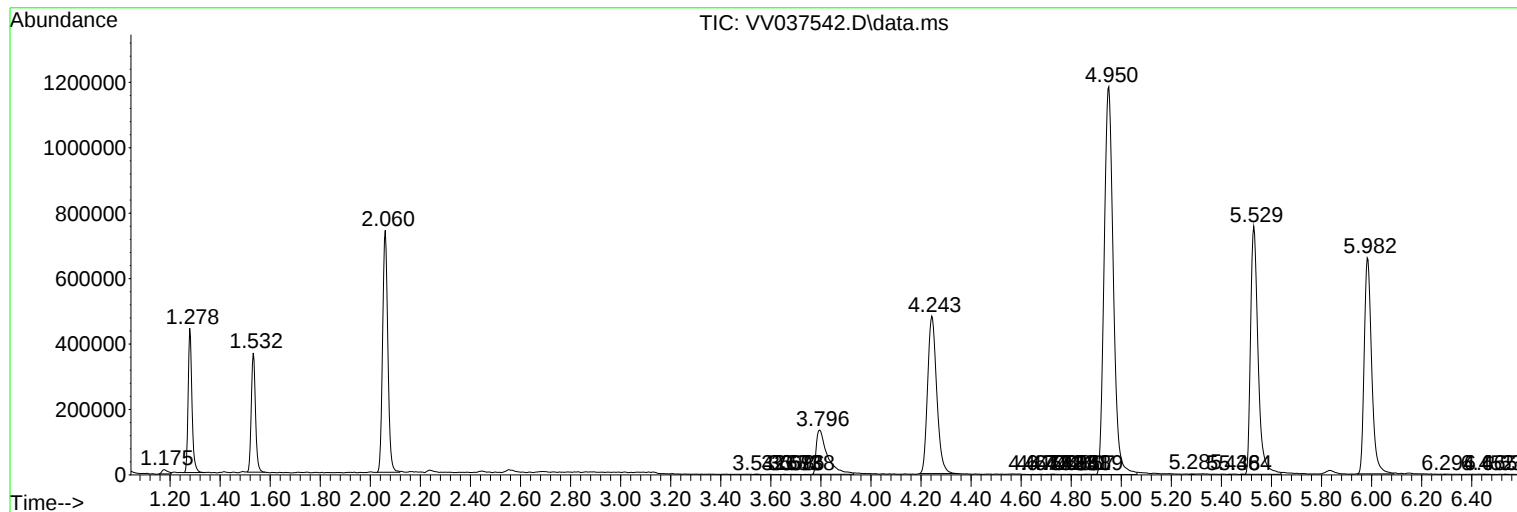

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037542.D
Acq On : 26 Sep 2024 13:00
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037542.D
Acq On : 26 Sep 2024 13:00
Operator : SY/MD
Sample : VV0926WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK213

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc