

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037578.D
 Acq On : 27 Sep 2024 02:58
 Operator : SY/MD
 Sample : P4185-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	52	rBV2	14505	25930	1.07%	0.142%
2	1.278	67	74	89	rVB	354585	377614	15.55%	2.067%
3	1.532	146	153	168	rVB	281249	327064	13.47%	1.790%
4	2.060	307	317	341	rVB	604177	893043	36.77%	4.889%
5	3.510	766	768	771	rBV3	709	388	0.02%	0.002%
6	3.545	776	779	784	rBV4	988	700	0.03%	0.004%
7	3.622	801	803	809	rVB4	656	287	0.01%	0.002%
8	3.658	810	814	816	rBV2	1188	821	0.03%	0.004%
9	3.748	840	842	847	rVB3	403	288	0.01%	0.002%
10	3.796	848	857	881	rBV	110768	312072	12.85%	1.708%
11	4.243	981	996	1024	rBV2	392570	989122	40.73%	5.414%
12	4.506	1061	1078	1101	rBV2	238261	616421	25.38%	3.374%
13	4.683	1130	1133	1137	rBV6	701	562	0.02%	0.003%
14	4.699	1137	1138	1141	rVB	679	211	0.01%	0.001%
15	4.731	1145	1148	1150	rBV3	806	462	0.02%	0.003%
16	4.744	1150	1152	1154	rVB3	790	311	0.01%	0.002%
17	4.780	1162	1163	1165	rVB2	831	252	0.01%	0.001%
18	4.822	1173	1176	1177	rBV2	816	489	0.02%	0.003%
19	4.860	1184	1188	1191	rBV4	598	486	0.02%	0.003%
20	4.950	1200	1216	1247	rBV2	952946	2428531	100.00%	13.294%
21	5.400	1354	1356	1360	rBV3	481	508	0.02%	0.003%
22	5.455	1368	1373	1375	rBV5	722	654	0.03%	0.004%
23	5.529	1385	1396	1427	rBV	707977	1460872	60.15%	7.997%
24	5.937	1518	1523	1524	rBV4	819	610	0.03%	0.003%
25	5.982	1525	1537	1570	rVV	528500	1109438	45.68%	6.073%
26	6.416	1668	1672	1678	rBV5	979	1033	0.04%	0.006%
27	6.445	1678	1681	1683	rVV2	488	323	0.01%	0.002%
28	6.506	1698	1700	1703	rVB	626	231	0.01%	0.001%
29	6.545	1707	1712	1716	rBV4	665	579	0.02%	0.003%
30	6.619	1732	1735	1737	rBV2	522	254	0.01%	0.001%
31	6.635	1737	1740	1741	rBV3	476	231	0.01%	0.001%
32	6.667	1744	1750	1751	rBV4	971	672	0.03%	0.004%
33	6.693	1755	1758	1760	rVV2	666	379	0.02%	0.002%
34	6.722	1764	1767	1768	rBV3	682	316	0.01%	0.002%
35	6.757	1773	1778	1779	rBV3	793	573	0.02%	0.003%
36	6.802	1790	1792	1797	rVB4	954	595	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037578.D
 Acq On : 27 Sep 2024 02:58
 Operator : SY/MD
 Sample : P4185-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.821	1797	1798	1799	rBV4	529	189	0.01%	0.001%
38	6.870	1810	1813	1815	rBV2	1288	802	0.03%	0.004%
39	6.908	1815	1825	1856	rVV	264106	515938	21.24%	2.824%
40	7.239	1917	1928	1957	rBV	1086923	1928193	79.40%	10.555%
41	7.551	2016	2025	2044	rBV	176314	323413	13.32%	1.770%
42	7.905	2124	2135	2151	rBV2	33827	64022	2.64%	0.350%
43	8.024	2161	2172	2215	rBV2	295205	653511	26.91%	3.577%
44	8.664	2370	2371	2373	rBV	731	362	0.01%	0.002%
45	8.780	2395	2407	2440	rBV	1084365	1817761	74.85%	9.950%
46	9.310	2569	2572	2573	rBV3	409	275	0.01%	0.002%
47	9.326	2573	2577	2580	rVB6	737	617	0.03%	0.003%
48	9.374	2589	2592	2593	rBV2	833	572	0.02%	0.003%
49	9.407	2599	2602	2603	rBV	826	547	0.02%	0.003%
50	9.480	2620	2625	2627	rBV3	984	694	0.03%	0.004%
51	9.535	2640	2642	2646	rVB3	847	481	0.02%	0.003%
52	9.571	2649	2653	2655	rBV3	407	364	0.01%	0.002%
53	9.583	2655	2657	2660	rVB4	720	433	0.02%	0.002%
54	9.599	2660	2662	2664	rVB2	508	214	0.01%	0.001%
55	9.616	2664	2667	2670	rBV	646	570	0.02%	0.003%
56	9.632	2670	2672	2674	rVB2	547	261	0.01%	0.001%
57	9.648	2674	2677	2682	rBV3	860	532	0.02%	0.003%
58	9.673	2684	2685	2689	rVV4	830	428	0.02%	0.002%
59	9.706	2693	2695	2699	rVB2	868	596	0.02%	0.003%
60	9.741	2703	2706	2711	rVB7	985	555	0.02%	0.003%
61	9.773	2713	2716	2717	rBV2	399	209	0.01%	0.001%
62	9.866	2740	2745	2746	rBV4	1837	1473	0.06%	0.008%
63	9.924	2760	2763	2766	rVB4	1131	754	0.03%	0.004%
64	9.960	2770	2774	2776	rBV2	724	509	0.02%	0.003%
65	9.972	2776	2778	2780	rVV3	529	227	0.01%	0.001%
66	9.998	2784	2786	2789	rVB3	744	319	0.01%	0.002%
67	10.017	2789	2792	2796	rBV3	376	392	0.02%	0.002%
68	10.066	2805	2807	2810	rVB2	697	356	0.01%	0.002%
69	10.107	2816	2820	2821	rBV4	1553	1140	0.05%	0.006%
70	10.146	2821	2832	2861	rVV	609166	973469	40.08%	5.329%
71	10.419	2914	2917	2919	rBV4	865	422	0.02%	0.002%
72	10.445	2922	2925	2928	rBV3	995	811	0.03%	0.004%
73	10.606	2970	2975	2977	rBV3	787	734	0.03%	0.004%
74	10.683	2995	2999	3002	rBV4	675	654	0.03%	0.004%
75	10.744	3016	3018	3020	rBV2	754	376	0.02%	0.002%
76	10.760	3020	3023	3026	rVB4	842	517	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037578.D
 Acq On : 27 Sep 2024 02:58
 Operator : SY/MD
 Sample : P4185-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.776	3026	3028	3030	rBV2	1002	529	0.02%	0.003%
78	10.863	3047	3055	3057	rBV4	2358	2720	0.11%	0.015%
79	10.969	3087	3088	3092	rBV2	528	271	0.01%	0.001%
80	11.066	3116	3118	3122	rVV	442	346	0.01%	0.002%
81	11.111	3129	3132	3134	rBV3	614	472	0.02%	0.003%
82	11.178	3142	3153	3194	rBV	1046951	1684972	69.38%	9.224%
83	11.554	3258	3270	3297	rBV	1076176	1722307	70.92%	9.428%
84	11.831	3354	3356	3359	rBV2	900	445	0.02%	0.002%
85	11.902	3372	3378	3382	rBV5	1305	1500	0.06%	0.008%
86	12.062	3424	3428	3433	rBV4	960	885	0.04%	0.005%
87	12.123	3445	3447	3448	rBV2	576	207	0.01%	0.001%
88	12.275	3492	3494	3496	rBV2	786	419	0.02%	0.002%
89	12.316	3503	3507	3509	rBV3	732	566	0.02%	0.003%
90	12.345	3514	3516	3520	rBV4	583	278	0.01%	0.002%
91	12.365	3520	3522	3523	rBV2	435	236	0.01%	0.001%
92	12.374	3523	3525	3529	rVB4	1056	557	0.02%	0.003%
93	12.834	3664	3668	3672	rBV4	1344	1226	0.05%	0.007%
94	13.043	3729	3733	3737	rBV4	922	954	0.04%	0.005%
95	13.107	3751	3753	3756	rVB4	1131	502	0.02%	0.003%
96	13.210	3783	3785	3788	rVB3	1077	586	0.02%	0.003%
97	13.397	3841	3843	3846	rBV2	676	349	0.01%	0.002%
98	13.503	3874	3876	3878	rBV	949	369	0.02%	0.002%
99	14.384	4147	4150	4153	rBV4	1032	726	0.03%	0.004%
100	14.525	4192	4194	4197	rBV3	1480	731	0.03%	0.004%

Sum of corrected areas: 18268167




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037578.D
Acq On : 27 Sep 2024 02:58
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

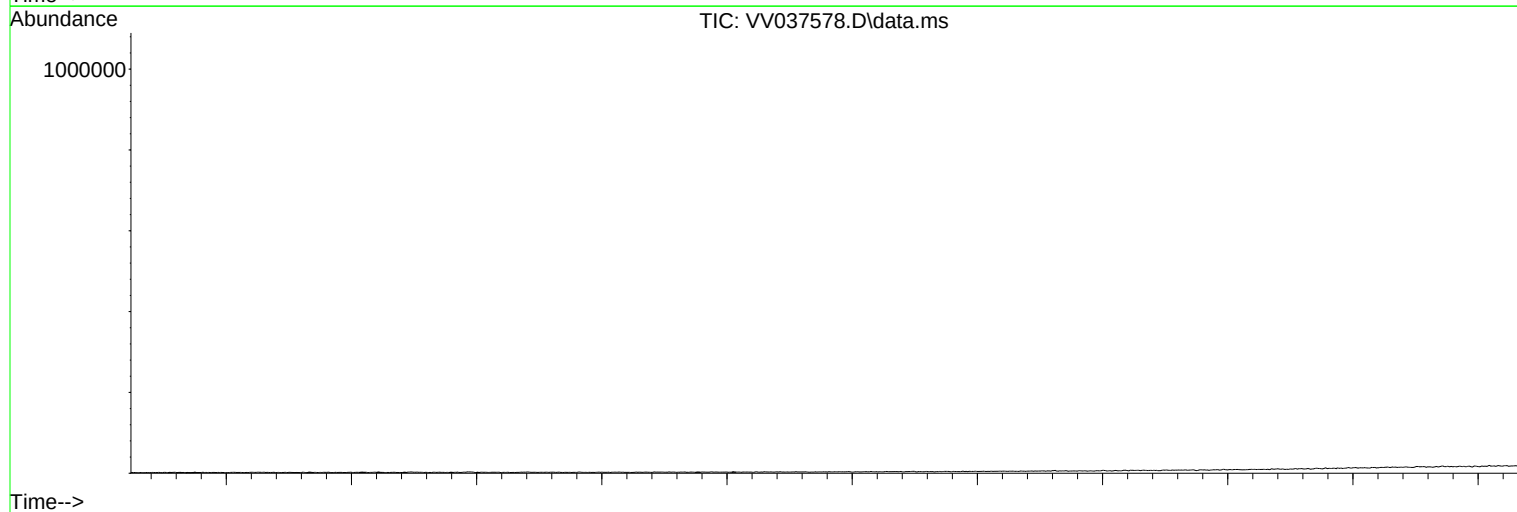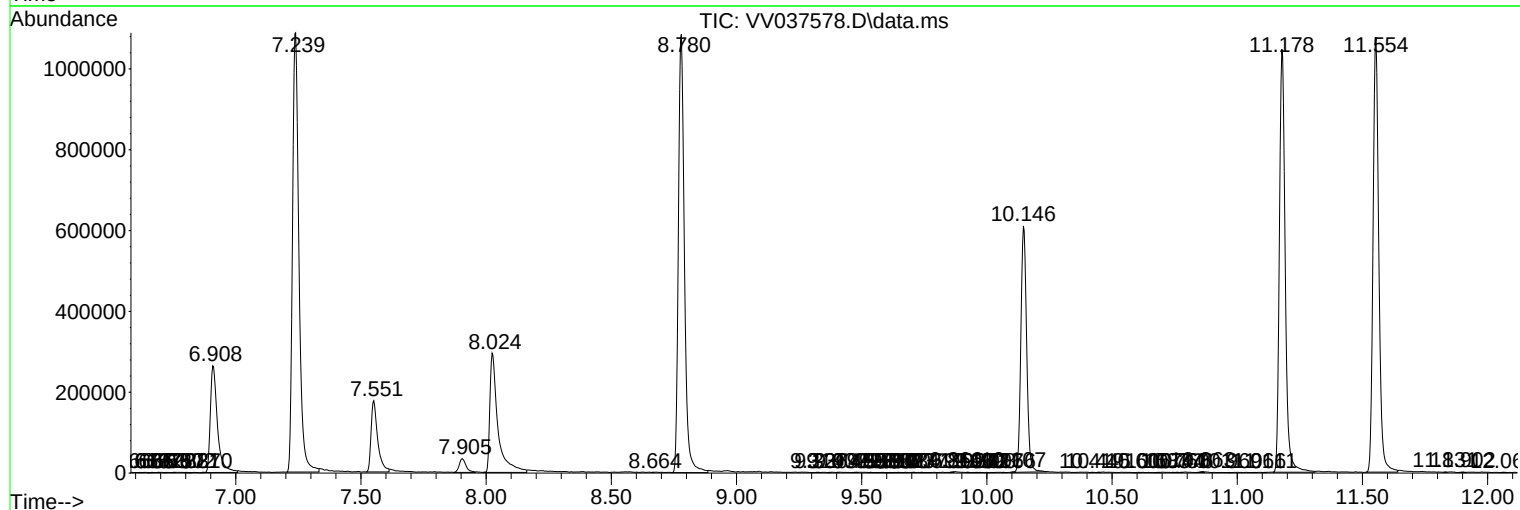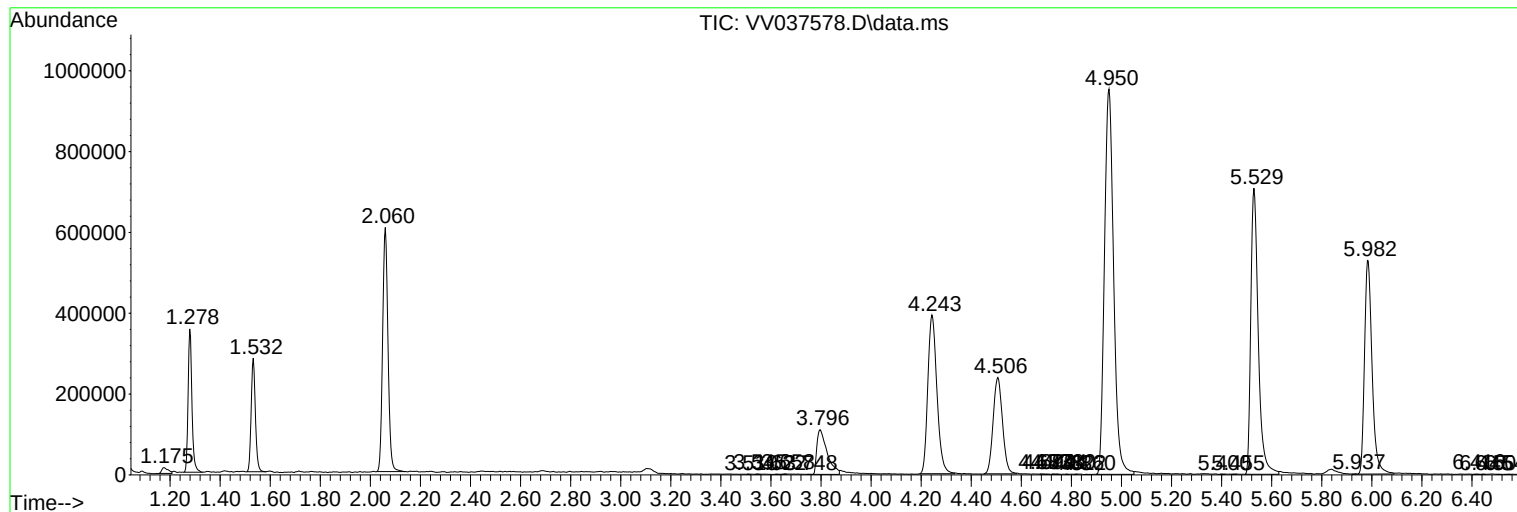

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037578.D
Acq On : 27 Sep 2024 02:58
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037578.D
Acq On : 27 Sep 2024 02:58
Operator : SY/MD
Sample : P4185-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
