

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037586.D
 Acq On : 27 Sep 2024 05:50
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037586.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	54	rBV	20587	36349	1.45%	0.186%
2	1.281	68	75	90	rVB	355745	384876	15.36%	1.971%
3	1.532	146	153	173	rVB	294680	350213	13.98%	1.794%
4	2.059	308	317	332	rBV	611184	877491	35.03%	4.494%
5	3.108	632	643	671	rVB	224170	477766	19.07%	2.447%
6	3.529	770	774	776	rBV4	745	621	0.02%	0.003%
7	3.551	779	781	786	rVV2	952	697	0.03%	0.004%
8	3.583	786	791	797	rVV6	855	961	0.04%	0.005%
9	3.651	809	812	816	rBV4	787	656	0.03%	0.003%
10	3.693	822	825	828	rBV3	648	392	0.02%	0.002%
11	3.751	838	843	847	rVB2	857	926	0.04%	0.005%
12	3.805	847	860	890	rBV3	236356	687418	27.44%	3.521%
13	4.243	980	996	1030	rBV	401549	1023226	40.84%	5.241%
14	4.506	1060	1078	1104	rBV	286878	725786	28.97%	3.717%
15	4.757	1153	1156	1159	rBV3	794	511	0.02%	0.003%
16	4.773	1159	1161	1163	rVV2	538	212	0.01%	0.001%
17	4.837	1179	1181	1183	rVB2	687	277	0.01%	0.001%
18	4.860	1185	1188	1192	rVB4	1010	652	0.03%	0.003%
19	4.895	1195	1199	1200	rBV	409	250	0.01%	0.001%
20	4.950	1200	1216	1251	rBV2	986697	2505187	100.00%	12.831%
21	5.281	1317	1319	1322	rBV2	1036	409	0.02%	0.002%
22	5.400	1351	1356	1360	rBV5	752	709	0.03%	0.004%
23	5.445	1368	1370	1372	rBV	687	430	0.02%	0.002%
24	5.529	1385	1396	1431	rBV	679756	1428553	57.02%	7.317%
25	5.837	1482	1492	1512	rVB5	32835	77838	3.11%	0.399%
26	5.985	1525	1538	1565	rBV	540032	1118670	44.65%	5.730%
27	6.336	1643	1647	1648	rBV2	1348	792	0.03%	0.004%
28	6.394	1662	1665	1669	rBV4	1025	789	0.03%	0.004%
29	6.497	1695	1697	1698	rBV	430	185	0.01%	0.001%
30	6.535	1705	1709	1712	rBV3	801	620	0.02%	0.003%
31	6.635	1737	1740	1742	rBV	702	338	0.01%	0.002%
32	6.654	1742	1746	1751	rVB4	459	422	0.02%	0.002%
33	6.693	1753	1758	1760	rBV3	1263	954	0.04%	0.005%
34	6.725	1765	1768	1769	rBV2	498	306	0.01%	0.002%
35	6.789	1785	1788	1790	rBV	633	344	0.01%	0.002%
36	6.828	1798	1800	1803	rBV4	488	339	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037586.D
 Acq On : 27 Sep 2024 05:50
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.857	1808	1809	1812	rBV2	352	194	0.01%	0.001%
38	6.908	1815	1825	1852	rBV	265425	519808	20.75%	2.662%
39	7.239	1916	1928	1958	rBV	1121329	1990214	79.44%	10.194%
40	7.551	2016	2025	2055	rBV	179743	336529	13.43%	1.724%
41	7.905	2124	2135	2153	rBV2	65206	118646	4.74%	0.608%
42	8.024	2164	2172	2218	rBV2	283534	634418	25.32%	3.249%
43	8.477	2311	2313	2314	rBV2	1066	436	0.02%	0.002%
44	8.545	2328	2334	2336	rBV4	1213	1429	0.06%	0.007%
45	8.660	2368	2370	2372	rBV3	874	457	0.02%	0.002%
46	8.779	2392	2407	2436	rBV	1062071	1766324	70.51%	9.047%
47	9.226	2544	2546	2550	rBV4	894	516	0.02%	0.003%
48	9.275	2558	2561	2567	rVB3	718	570	0.02%	0.003%
49	9.313	2570	2573	2578	rBV4	838	619	0.02%	0.003%
50	9.348	2581	2584	2588	rBV4	668	539	0.02%	0.003%
51	9.397	2597	2599	2601	rBV2	544	324	0.01%	0.002%
52	9.432	2607	2610	2612	rBV2	749	504	0.02%	0.003%
53	9.484	2621	2626	2628	rBV5	1812	1795	0.07%	0.009%
54	9.529	2638	2640	2642	rVB2	879	340	0.01%	0.002%
55	9.541	2642	2644	2647	rBV2	398	177	0.01%	0.001%
56	9.564	2647	2651	2653	rVV4	649	509	0.02%	0.003%
57	9.590	2657	2659	2664	rBV4	551	475	0.02%	0.002%
58	9.615	2664	2667	2671	rBV5	750	528	0.02%	0.003%
59	9.635	2671	2673	2674	rBV2	361	162	0.01%	0.001%
60	9.664	2678	2682	2685	rBV3	558	501	0.02%	0.003%
61	9.728	2700	2702	2703	rBV	437	179	0.01%	0.001%
62	9.760	2710	2712	2715	rBV2	752	378	0.02%	0.002%
63	9.776	2715	2717	2720	rVV2	356	146	0.01%	0.001%
64	9.828	2730	2733	2735	rBV2	351	165	0.01%	0.001%
65	9.902	2755	2756	2759	rVB2	790	304	0.01%	0.002%
66	9.924	2762	2763	2766	rBV3	359	200	0.01%	0.001%
67	10.033	2794	2797	2801	rBV4	882	656	0.03%	0.003%
68	10.053	2801	2803	2804	rBV2	357	124	0.00%	0.001%
69	10.062	2804	2806	2808	rBV2	474	245	0.01%	0.001%
70	10.104	2815	2819	2820	rBV2	822	520	0.02%	0.003%
71	10.146	2820	2832	2858	rVV	625416	982408	39.21%	5.032%
72	10.615	2975	2978	2981	rBV4	1152	936	0.04%	0.005%
73	10.664	2991	2993	2995	rBV2	706	458	0.02%	0.002%
74	10.734	3013	3015	3021	rVB4	1026	804	0.03%	0.004%
75	10.763	3021	3024	3027	rBV3	448	262	0.01%	0.001%
76	10.779	3027	3029	3031	rBV3	1343	786	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
 Data File : VV037586.D
 Acq On : 27 Sep 2024 05:50
 Operator : SY/MD
 Sample : P4185-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.860	3046	3054	3063	rBV6	4053	6703	0.27%	0.034%
78	10.940	3076	3079	3080	rBV3	630	328	0.01%	0.002%
79	11.024	3102	3105	3107	rBV3	633	298	0.01%	0.002%
80	11.078	3120	3122	3125	rVB2	924	579	0.02%	0.003%
81	11.178	3142	3153	3177	rBV	1041426	1657007	66.14%	8.487%
82	11.554	3258	3270	3297	rBV	1101439	1777169	70.94%	9.102%
83	11.840	3357	3359	3360	rBV2	842	392	0.02%	0.002%
84	11.963	3392	3397	3399	rBV4	1226	888	0.04%	0.005%
85	12.165	3458	3460	3463	rBV3	447	231	0.01%	0.001%
86	12.307	3498	3504	3507	rBV5	993	1076	0.04%	0.006%
87	12.461	3550	3552	3553	rBV	760	362	0.01%	0.002%
88	12.503	3561	3565	3567	rVB3	1434	968	0.04%	0.005%
89	12.522	3567	3571	3573	rBV2	773	649	0.03%	0.003%
90	12.593	3591	3593	3597	rBV3	657	441	0.02%	0.002%
91	12.618	3597	3601	3604	rVB3	912	701	0.03%	0.004%
92	12.644	3604	3609	3615	rBV4	1279	1584	0.06%	0.008%
93	12.699	3624	3626	3629	rBV2	885	414	0.02%	0.002%
94	12.988	3714	3716	3719	rBV3	718	397	0.02%	0.002%
95	13.200	3779	3782	3783	rBV2	774	402	0.02%	0.002%
96	13.310	3812	3816	3817	rBV4	645	377	0.02%	0.002%
97	13.380	3836	3838	3845	rVB5	1146	815	0.03%	0.004%
98	13.641	3916	3919	3923	rVB4	706	551	0.02%	0.003%
99	13.686	3931	3933	3937	rBV4	1001	532	0.02%	0.003%
100	13.876	3990	3992	3994	rBV3	881	423	0.02%	0.002%

Sum of corrected areas: 19524037




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037586.D
Acq On : 27 Sep 2024 05:50
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

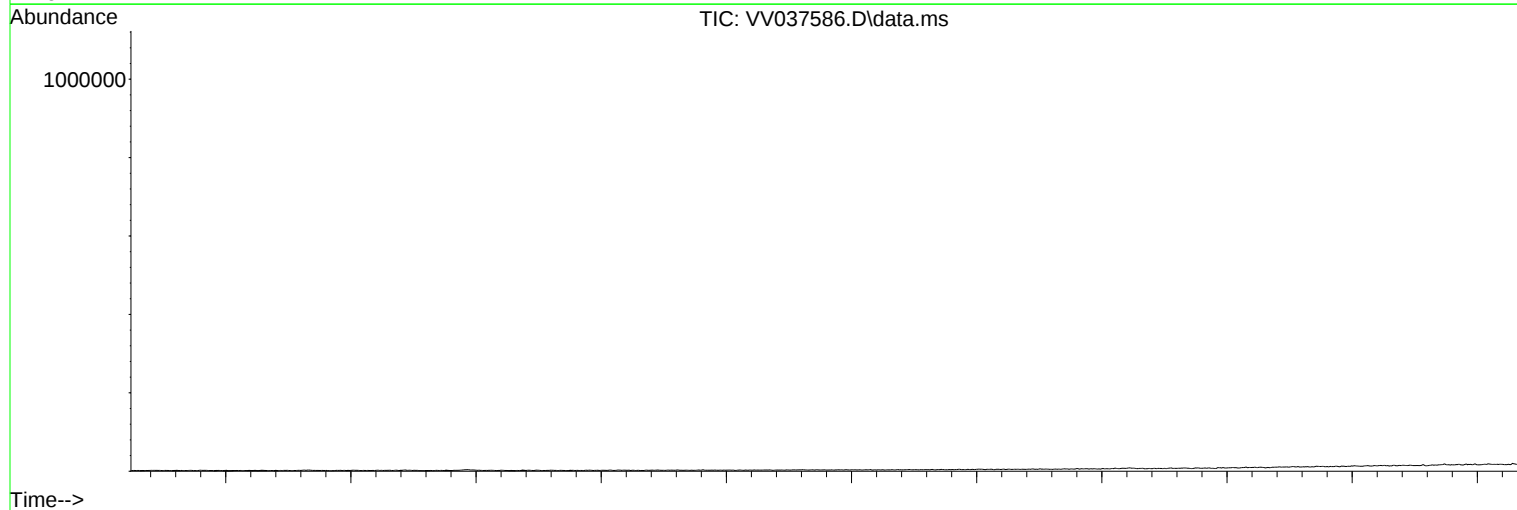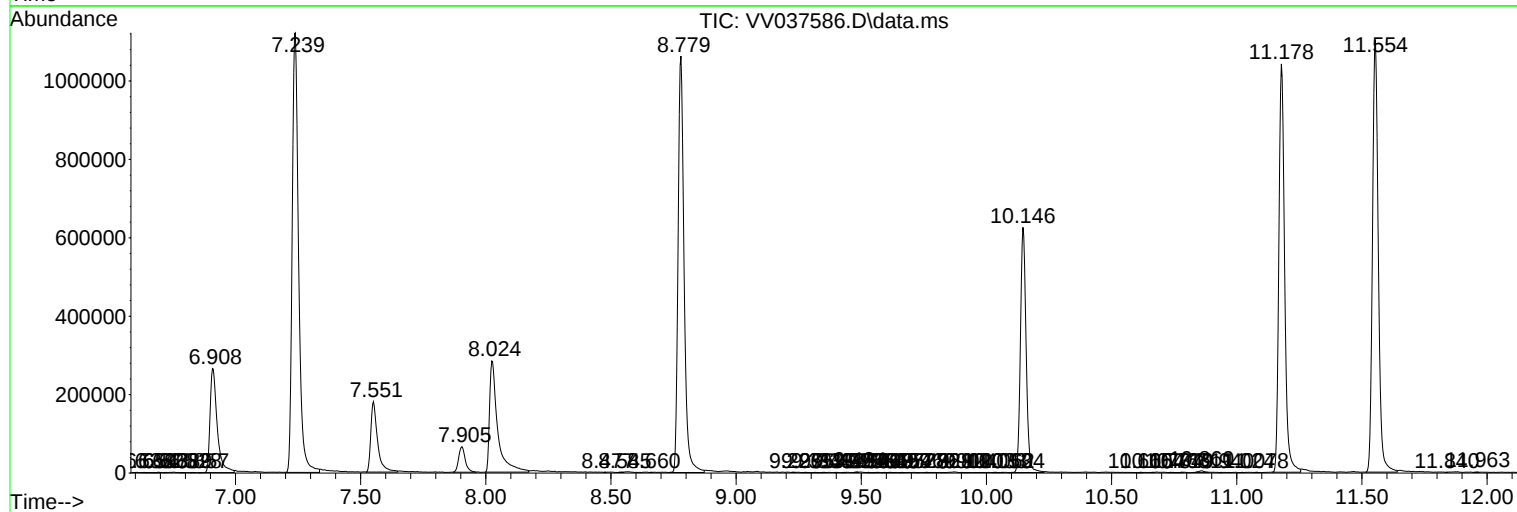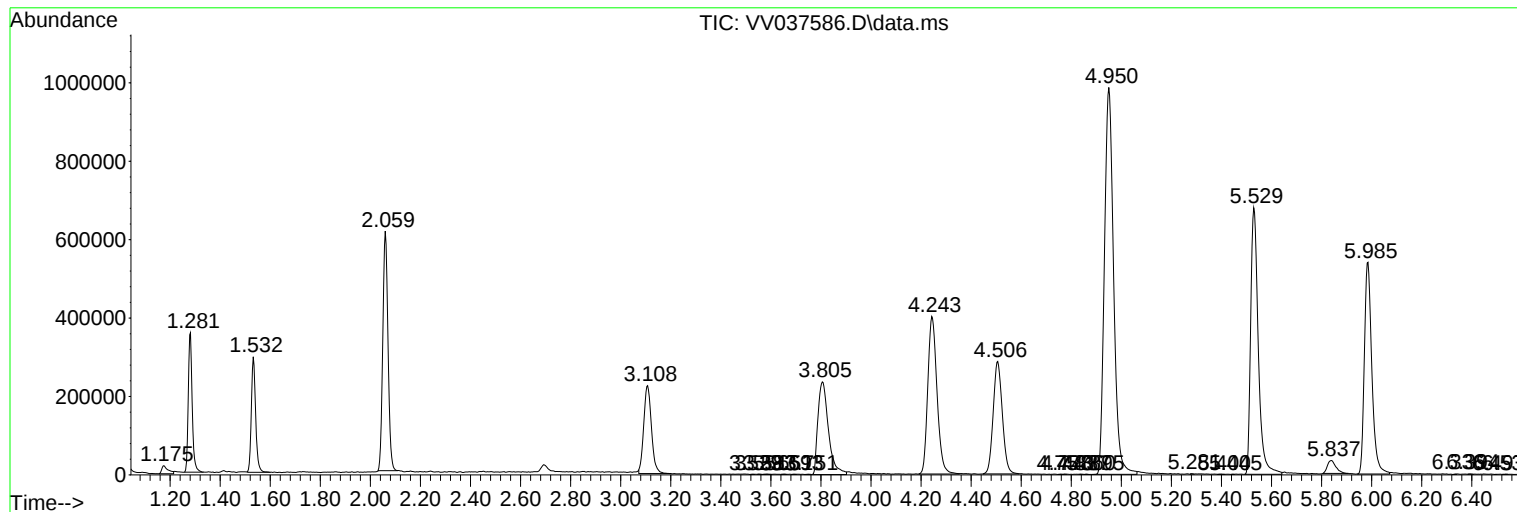

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037586.D
Acq On : 27 Sep 2024 05:50
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037586.D
Acq On : 27 Sep 2024 05:50
Operator : SY/MD
Sample : P4185-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
