
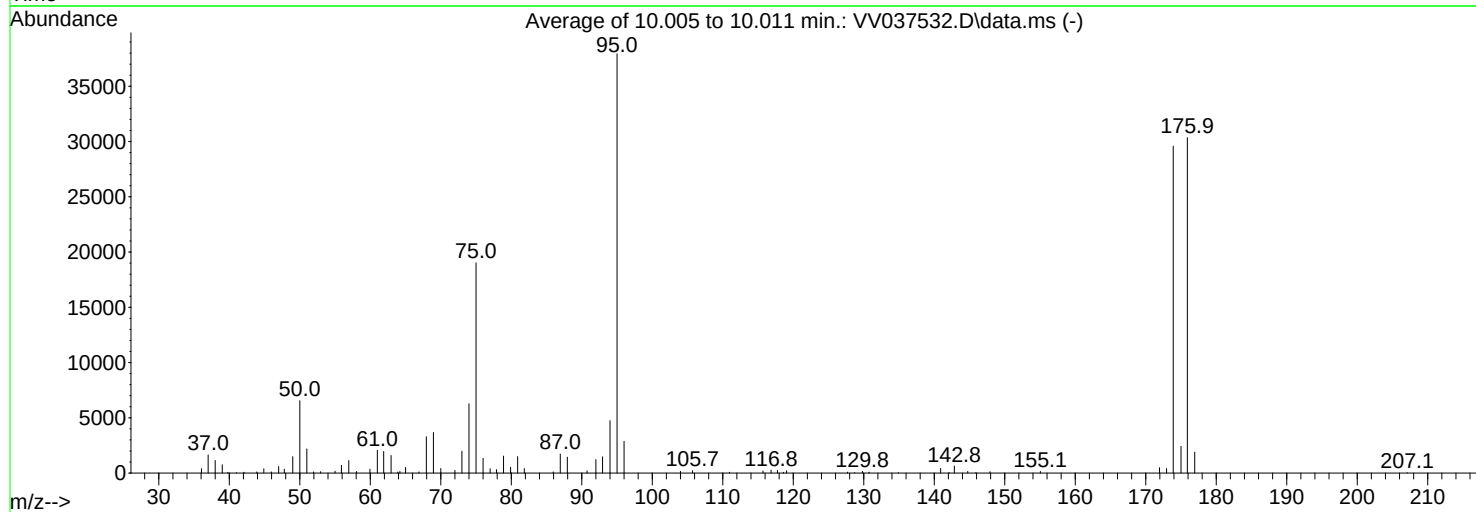


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092624\
Data File : VV037532.D
Acq On : 26 Sep 2024 07:49
Operator : SY/MD
Sample : BFB381
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB381

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Sat Sep 28 00:49:19 2024

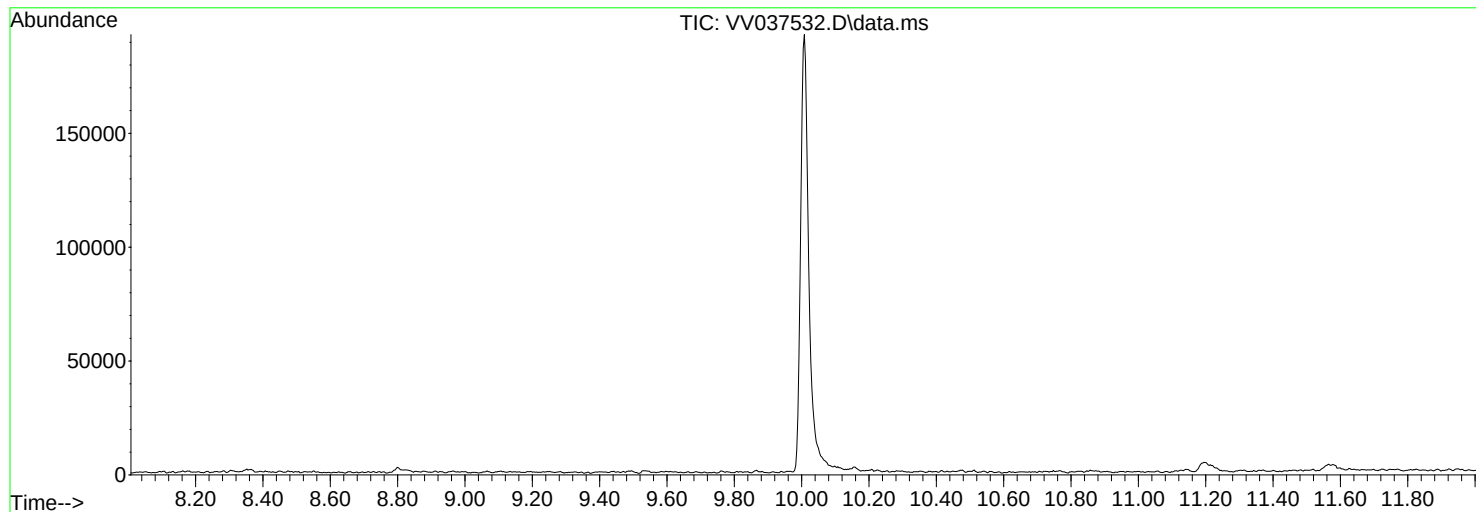

AutoFind: Scans 2788, 2789, 2790; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	6551	PASS
75	95	30	80	50.1	19024	PASS
95	95	100	100	100.0	37944	PASS
96	95	5	9	7.6	2879	PASS
173	174	0.00	2	1.4	409	PASS
174	95	50	120	78.0	29592	PASS
175	174	5	9	8.2	2419	PASS
176	174	95	105	102.6	30352	PASS
177	176	5	10	6.2	1892	PASS

m/z	Abundance
36.30	100.0
38.00	107.0
38.70	109.0
39.80	219.0
43.90	780.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.00	440.0
37.00	1632.0
38.00	1246.0
39.00	743.0
39.80	231.0
43.90	838.0
44.90	514.0
45.90	113.0
46.90	513.0
47.80	340.0
49.00	1522.0
50.00	6640.0
51.00	2301.0
52.90	111.0
55.00	132.0
55.90	743.0
56.90	1143.0
58.10	161.0
59.90	335.0
61.00	2117.0
61.90	2003.0
62.90	1678.0
63.90	274.0
65.00	578.0
66.90	196.0
67.90	3245.0
69.00	3825.0
70.10	442.0
72.00	216.0
73.00	2119.0
74.00	6386.0
75.00	19272.0
76.00	1487.0
77.00	389.0
78.00	257.0
78.90	1541.0
79.90	573.0
80.90	1572.0
81.90	356.0
86.00	109.0
86.90	1914.0
87.90	1205.0
90.70	201.0
92.00	1144.0
92.90	1537.0
94.00	4879.0
95.00	38296.0
96.00	3029.0
104.00	205.0
105.70	241.0
115.70	167.0
116.80	303.0
117.80	193.0
118.60	201.0
119.00	179.0
128.70	133.0
129.80	186.0
130.80	160.0
134.90	104.0
140.90	357.0
142.80	593.0
144.70	131.0
148.00	123.0
155.00	148.0
171.90	416.0
173.00	454.0
173.90	28864.0
175.00	2391.0
175.90	29416.0
177.00	1774.0
207.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.10	427.0
37.00	1708.0
38.00	1263.0
39.00	780.0
39.90	299.0
42.10	110.0
43.90	925.0
44.90	392.0
45.90	110.0
47.00	655.0
47.80	389.0
49.00	1496.0
50.00	6808.0
51.00	2271.0
52.00	148.0
53.00	147.0
55.00	189.0
55.90	725.0
57.00	1159.0
58.00	139.0
59.90	359.0
61.00	2119.0
61.90	2030.0
63.00	1627.0
64.20	232.0
65.00	529.0
66.90	127.0
67.90	3418.0
68.90	3771.0
70.00	407.0
72.00	226.0
73.00	2013.0
74.00	6498.0
75.00	19648.0
76.00	1346.0
77.00	420.0
77.90	314.0
78.90	1601.0
79.90	570.0
80.90	1553.0
81.80	424.0
86.00	131.0
87.00	1780.0
88.00	1529.0
90.70	221.0
92.00	1259.0
93.00	1508.0
94.00	4906.0
95.00	39208.0
96.00	2964.0
104.00	153.0
105.70	228.0
110.90	122.0
115.70	204.0
116.80	277.0
117.70	254.0
119.10	223.0
127.70	107.0
129.80	162.0
130.70	120.0
140.90	437.0
142.10	118.0
142.90	660.0
144.70	139.0
147.90	137.0
155.10	165.0
172.00	507.0
173.90	30456.0
175.00	2440.0
175.90	31568.0
176.90	1985.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381

m/z	Abundance
36.00	327.0
37.00	1585.0
38.00	1242.0
39.00	743.0
39.90	333.0
41.00	111.0
42.10	115.0
43.90	905.0
45.00	267.0
46.00	102.0
47.10	620.0
47.80	326.0
49.00	1436.0
50.00	6206.0
51.00	1985.0
51.90	184.0
53.00	135.0
55.00	206.0
55.90	630.0
57.00	1090.0
58.00	116.0
60.00	373.0
61.00	1944.0
61.90	1819.0
63.00	1483.0
64.20	210.0
65.00	424.0
68.00	3215.0
68.90	3430.0
69.90	393.0
72.00	299.0
73.00	1823.0
74.00	5950.0
75.00	18152.0
76.00	1212.0
77.00	363.0
77.80	378.0
78.90	1467.0
79.90	469.0
80.90	1343.0
81.80	447.0
85.90	106.0
86.90	1495.0
87.90	1589.0
90.80	205.0
92.00	1263.0
93.00	1380.0
94.00	4437.0
95.00	36328.0
96.00	2644.0
104.00	132.0
105.70	177.0
111.00	108.0
115.70	200.0
116.90	232.0
117.70	267.0
119.00	243.0
127.70	143.0
129.80	129.0
140.90	461.0
142.90	663.0
144.80	170.0
145.90	109.0
147.80	126.0
155.00	137.0
172.00	545.0
172.80	387.0
173.00	387.0
173.90	29456.0
175.00	2426.0
175.90	30072.0
176.90	1918.0

Instrument :
MSVOA_V
ClientSampleId :
BFB381