




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028181.D
 Acq On : 29 Sep 2022 12:56
 Operator : SY/MD
 Sample : N4871-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H80

Manual IntegrationsAPPROVED

Quant Time: Oct 03 02:08:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

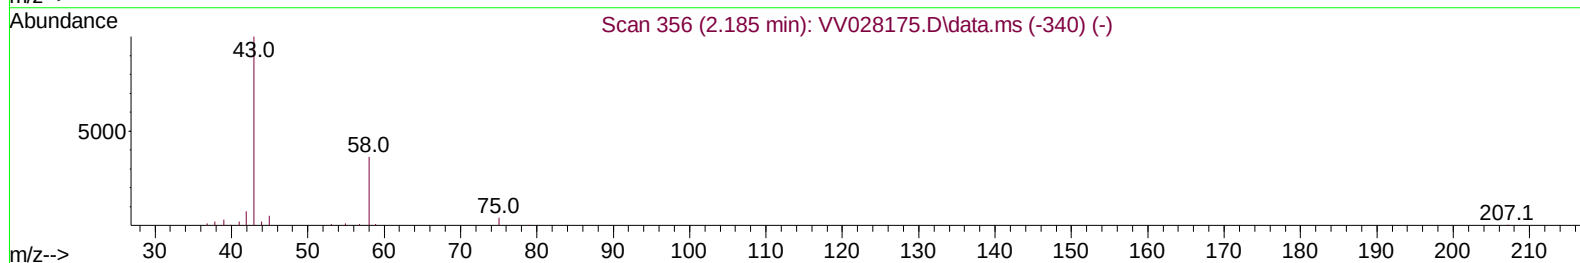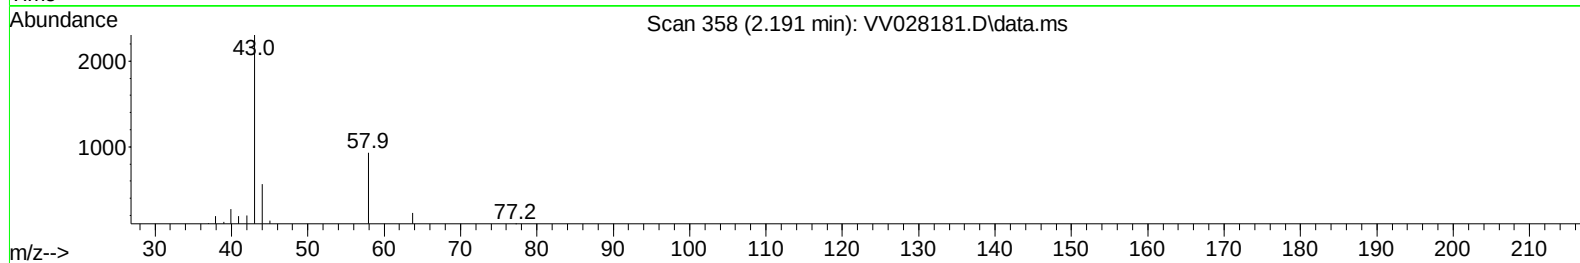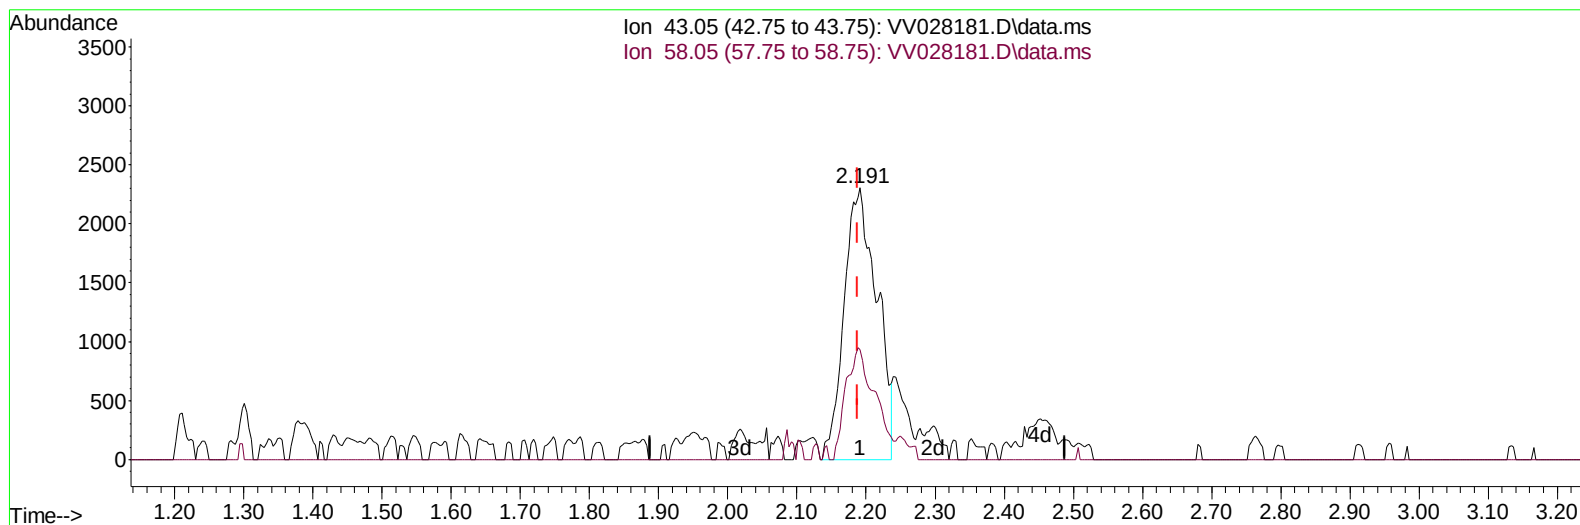

TIC: VV028181.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 3.67 ug/L

response 7565

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	36.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028181.D
 Acq On : 29 Sep 2022 12:56
 Operator : SY/MD
 Sample : N4871-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H80

Manual IntegrationsAPPROVED

Quant Time: Oct 03 02:08:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

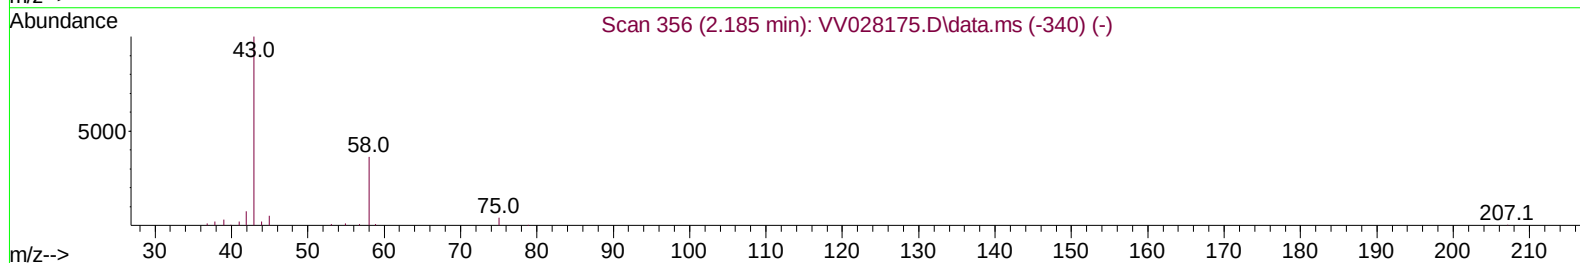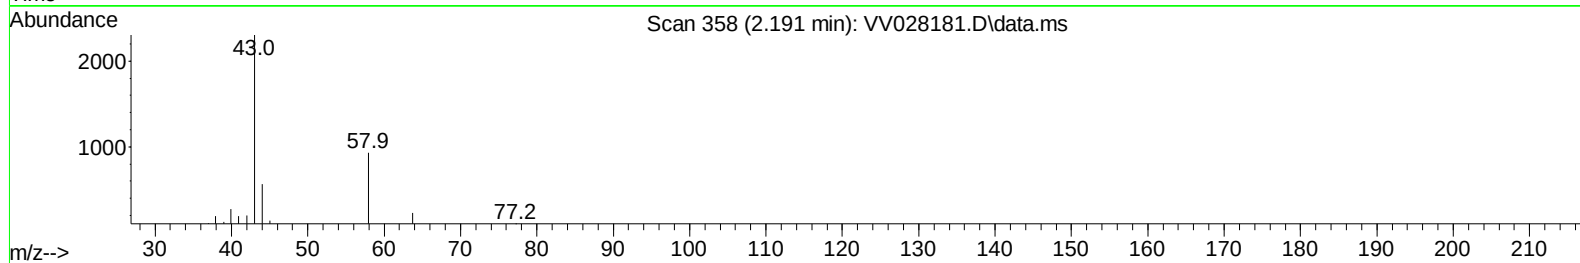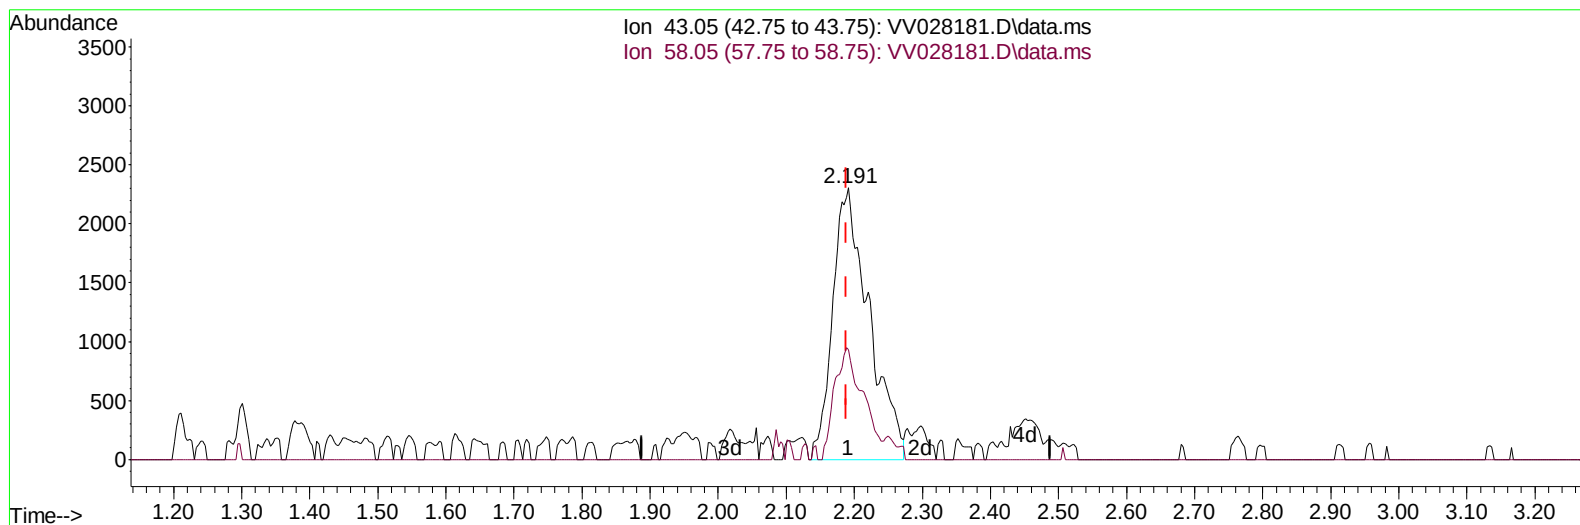

TIC: VV028181.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 4.14 ug/L m

response 8525

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	32.41
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028181.D
 Acq On : 29 Sep 2022 12:56
 Operator : SY/MD
 Sample : N4871-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H80

Manual IntegrationsAPPROVED

Quant Time: Oct 03 02:08:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.612	114		152729	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		140226	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		70009	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		47145	2.977	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	59.600%	
7) Chloroethane-d5	1.561	69		49370	3.922	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	78.400%	
11) 1,1-Dichloroethene-d2	2.101	63		67783	2.468	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	49.400%#	
20) 2-Butanone-d5	3.892	46		156669	58.608	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	117.220%	
24) Chloroform-d	4.342	84		119862	4.744	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	5.027	65		60702	5.049	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.043	84		213611	4.646	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.066	67		70435	4.914	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.313	98		155492	3.736	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.800%	
43) trans-1,3-Dichloroprop...	7.622	79		20244	3.910	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.200%	
46) 2-Hexanone-d5	8.085	63		118194	54.694	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	109.380%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		48001	4.899	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	11.619	152		68544	4.992	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%	
Target Compounds							
13) Acetone	2.191	43		8525m	4.140	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028181.D
Acq On : 29 Sep 2022 12:56
Operator : SY/MD
Sample : N4871-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H80

Manual IntegrationsAPPROVED

Quant Time: Oct 03 02:08:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
Supervised By :Mahesh Dadoda 10/05/2022

