




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028201.D
 Acq On : 29 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4870-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H79

Manual IntegrationsAPPROVED

Quant Time: Oct 03 05:06:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

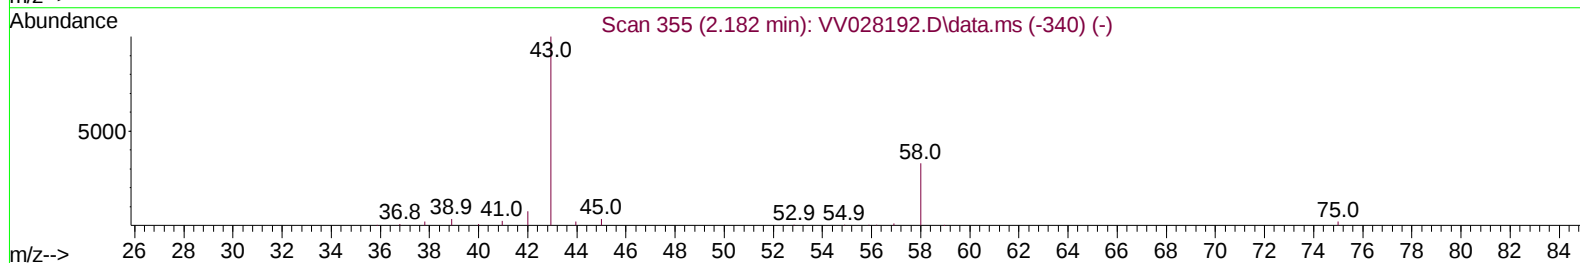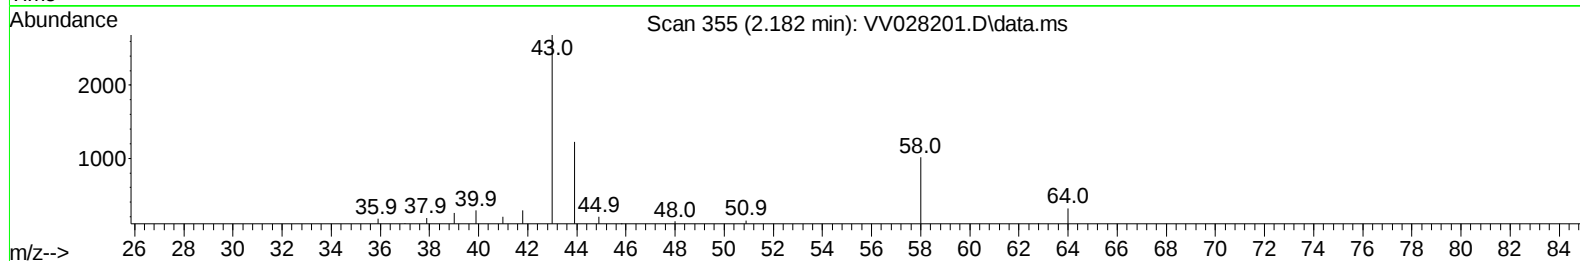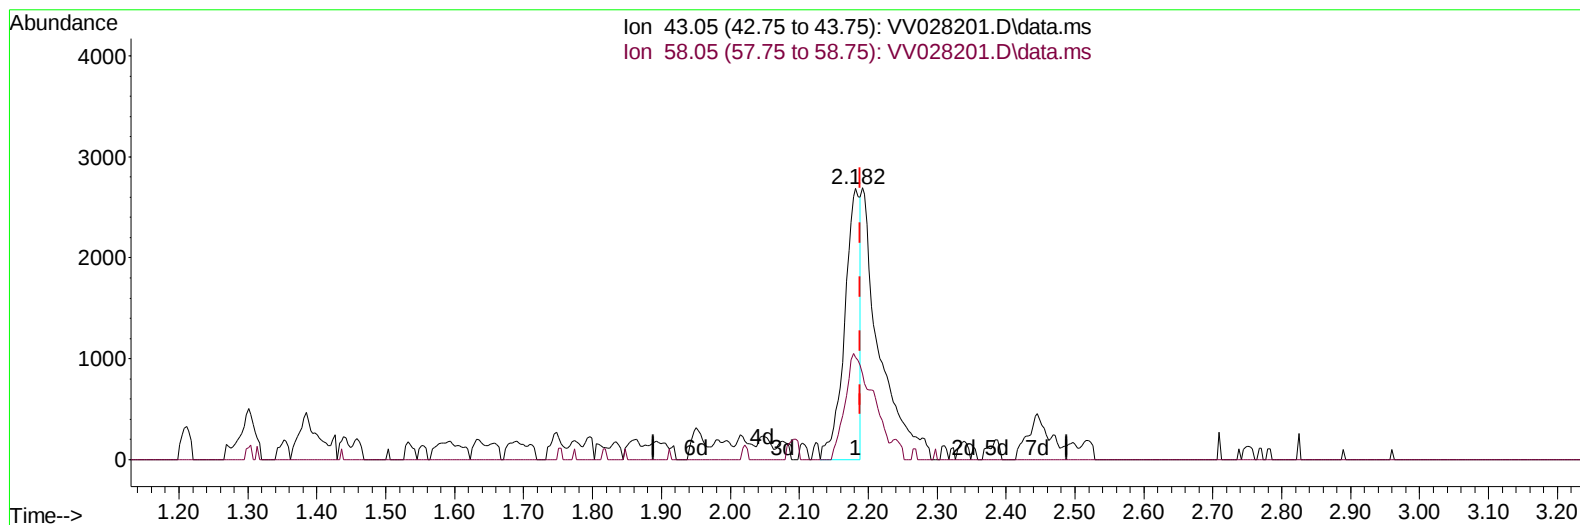

TIC: VV028201.D\data.ms

(13) Acetone (T)

2.182min (-0.006) 2.18 ug/L

response 4234

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	70.15#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028201.D
 Acq On : 29 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4870-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H79

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

Quant Time: Oct 03 05:06:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

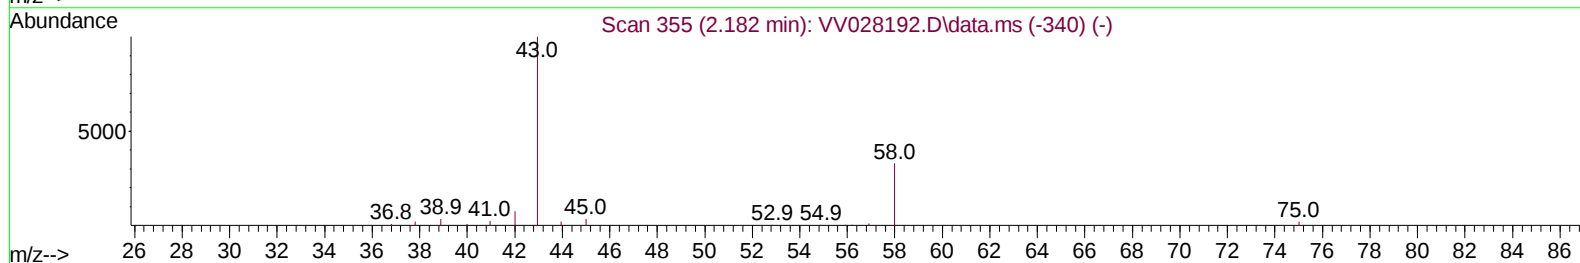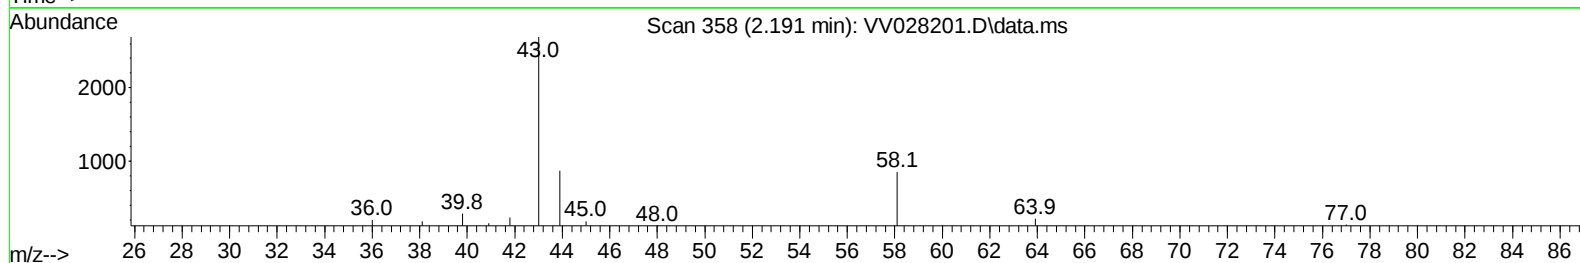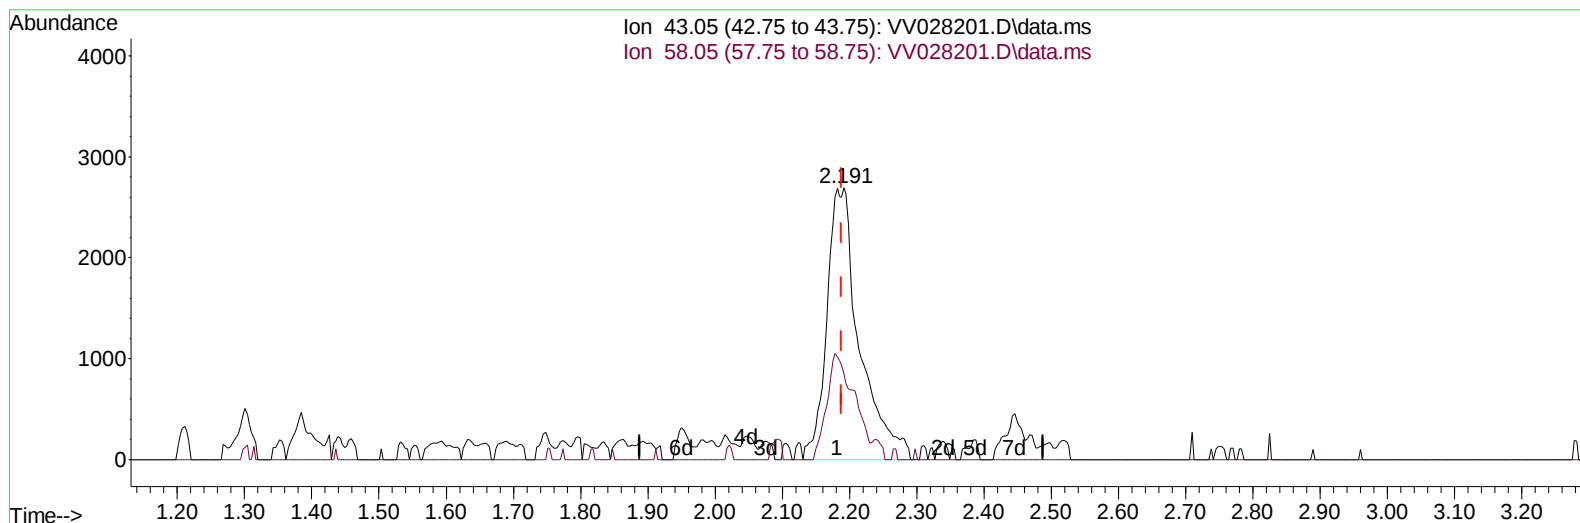

TIC: VV028201.D\data.ms

(13) Acetone (T)

2.191min (+ 0.003) 4.65 ug/L m

response 9035

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	32.80	32.87
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028201.D
 Acq On : 29 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4870-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H79

Manual IntegrationsAPPROVED

Quant Time: Oct 03 05:06:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.613	114		144132	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117		144240	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152		71981	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.301	65		66854	4.474	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.400%	
7) Chloroethane-d5	1.561	69		57577	4.846	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.000%	
11) 1,1-Dichloroethene-d2	2.101	63		96153	3.710	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.200%	
20) 2-Butanone-d5	3.892	46		108139	42.867	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.740%	
24) Chloroform-d	4.342	84		109138	4.577	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%	
26) 1,2-Dichloroethane-d4	5.027	65		49766	4.386	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%	
32) Benzene-d6	5.043	84		213138	4.507	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.200%	
36) 1,2-Dichloropropane-d6	6.066	67		57511	3.901	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	78.000%	
41) Toluene-d8	7.313	98		166274	3.884	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.600%	
43) trans-1,3-Dichloroprop...	7.619	79		20751	3.896	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.085	63		83536	37.580	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	75.160%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84		40423	4.011	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.200%	
66) 1,2-Dichlorobenzene-d4	11.622	152		70864	5.019	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.400%	
Target Compounds							
13) Acetone	2.191	43		9035m	4.650	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028201.D
Acq On : 29 Sep 2022 21:18
Operator : SY/MD
Sample : N4870-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 3

Instrument :
MSVOA_V
ClientSampleId :
F5H79

Manual IntegrationsAPPROVED

Quant Time: Oct 03 05:06:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 10/05/2022
Supervised By :Mahesh Dadoda 10/05/2022

