

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028176.D
 Acq On : 29 Sep 2022 10:57
 Operator : SY/MD
 Sample : VV0929WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK238

Quant Time: Sep 30 01:46:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	142885	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	131219	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	63678	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	74244	5.012	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	100.200%	
7) Chloroethane-d5	1.561	69	60537	5.140	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	102.800%	
11) 1,1-Dichloroethene-d2	2.098	63	101798	3.962	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	79.200%	
20) 2-Butanone-d5	3.895	46	111170	44.453	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	88.900%	
24) Chloroform-d	4.336	84	122691	5.190	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.800%	
26) 1,2-Dichloroethane-d4	5.024	65	57534	5.115	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	102.400%	
32) Benzene-d6	5.040	84	254867	5.924	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	118.400%	
36) 1,2-Dichloropropane-d6	6.063	67	69599	5.189	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	103.800%	
41) Toluene-d8	7.310	98	202629	5.203	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.000%	
43) trans-1,3-Dichloroprop...	7.619	79	23198	4.788	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.800%	
46) 2-Hexanone-d5	8.085	63	94564	46.763	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	93.520%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	44332	4.835	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.800%	
66) 1,2-Dichlorobenzene-d4	11.622	152	71649	5.736	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.497	84	2994	0.272	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028176.D
Acq On : 29 Sep 2022 10:57
Operator : SY/MD
Sample : VV0929WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK238

Quant Time: Sep 30 01:46:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

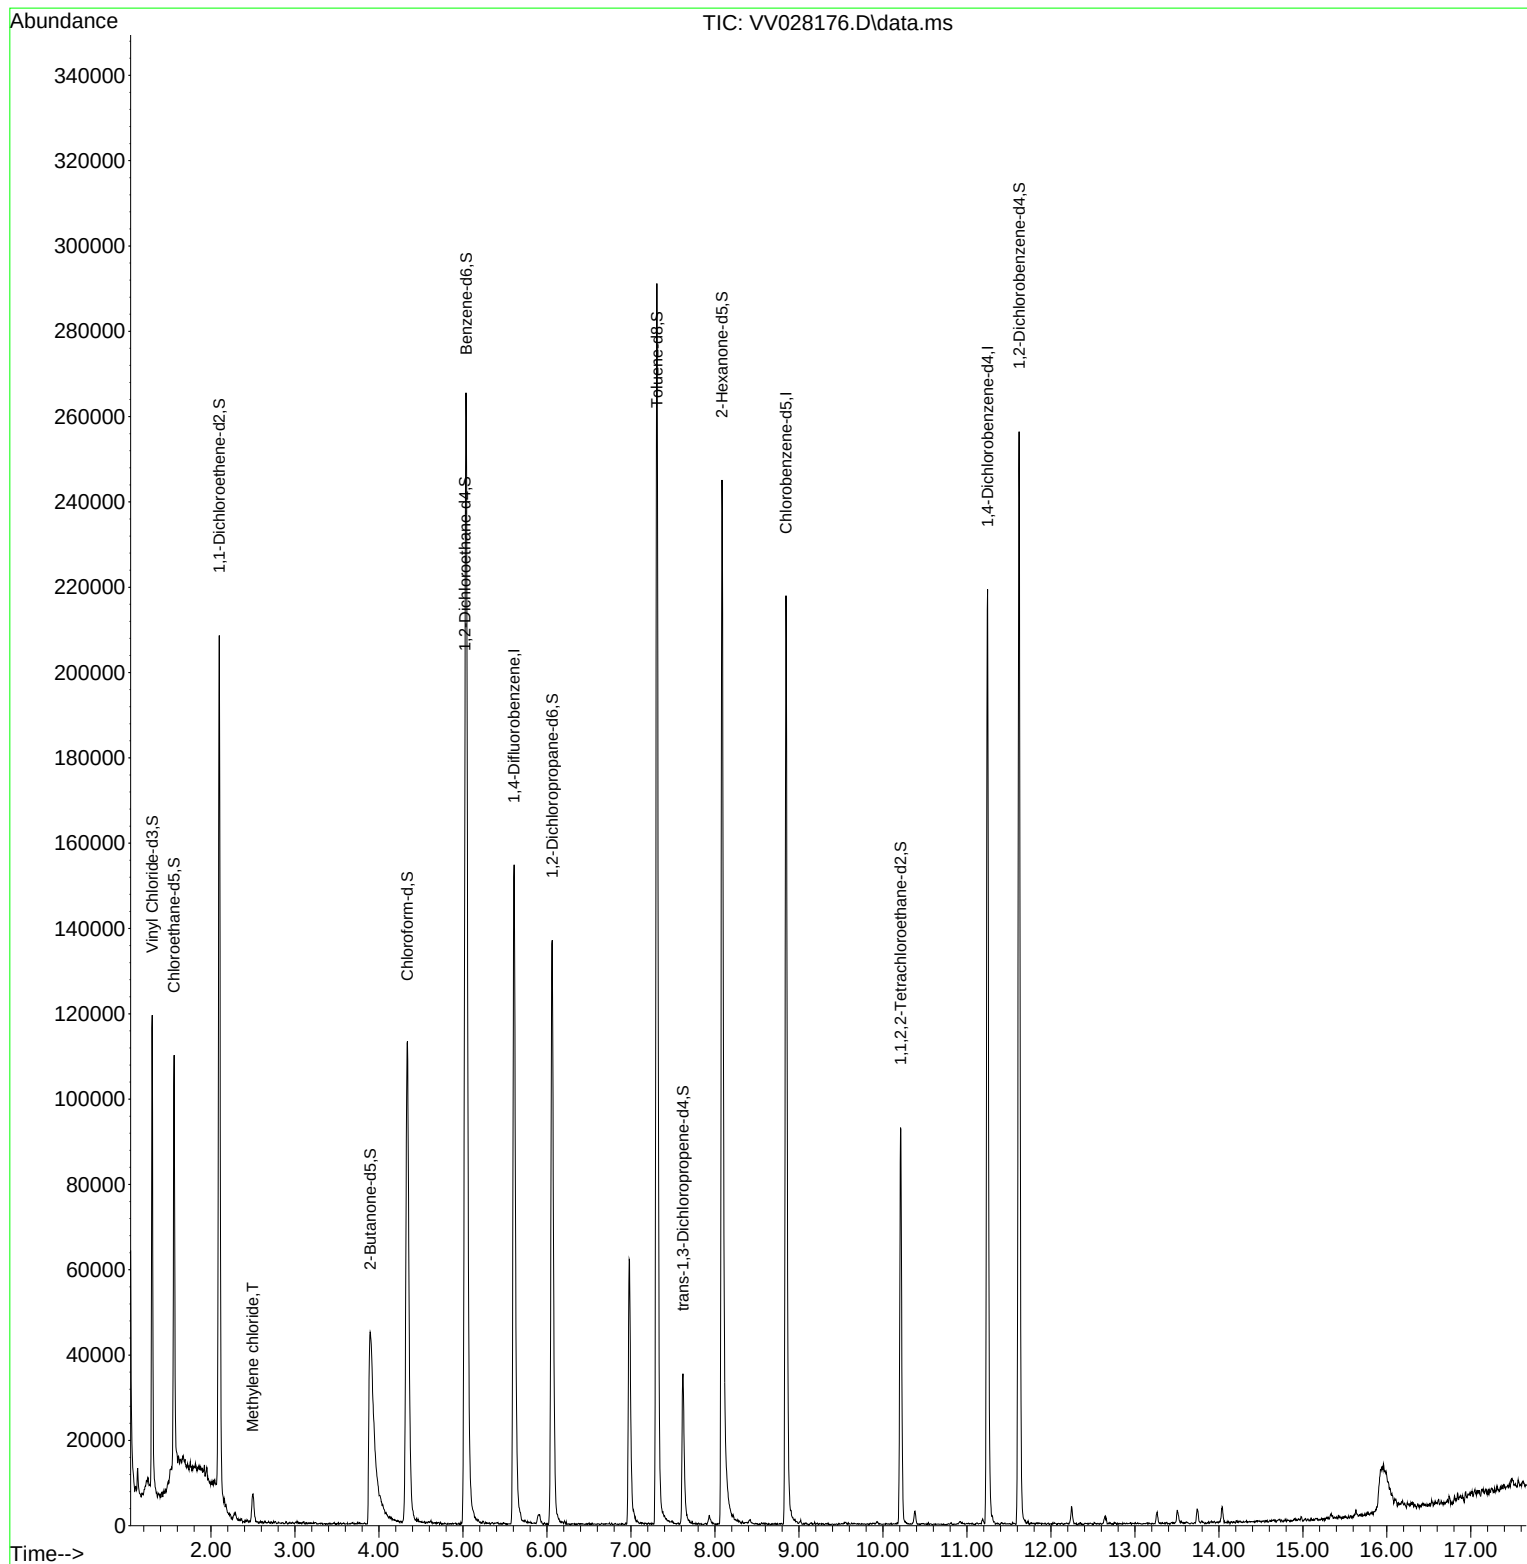

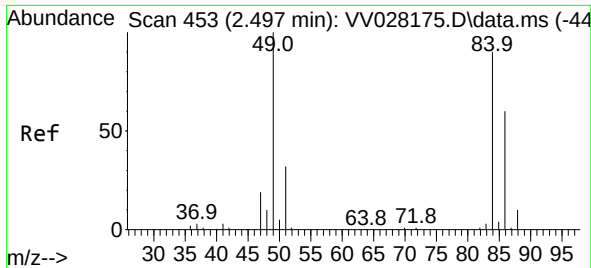

#16

Methylene chloride

Concen: 0.272 ug/L

RT: 2.497 min Scan# 4

Delta R.T. -0.000 min

Lab File: VV028176.D

Acq: 29 Sep 2022 10:57

Instrument :

MSVOA_V

ClientSampleId :

VBLK238

Tgt Ion: 84 Resp: 2994

Ion Ratio Lower Upper

84 100

86 70.8 46.8 86.8

49 98.3 87.5 162.5

