

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028177.D
 Acq On : 29 Sep 2022 11:21
 Operator : SY/MD
 Sample : N4856-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Sep 30 01:46:34 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	166665	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	159507	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	72663	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	79399	4.595	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.000%
7) Chloroethane-d5	1.561	69	63825	4.646	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.000%
11) 1,1-Dichloroethene-d2	2.101	63	107252	3.579	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	71.600%
20) 2-Butanone-d5	3.896	46	130541	44.751	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.500%
24) Chloroform-d	4.339	84	132154	4.793	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.800%
26) 1,2-Dichloroethane-d4	5.027	65	60327	4.598	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.000%
32) Benzene-d6	5.043	84	265951	5.085	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.800%
36) 1,2-Dichloropropane-d6	6.063	67	75827	4.651	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.000%
41) Toluene-d8	7.310	98	212449	4.488	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.800%
43) trans-1,3-Dichloroprop...	7.619	79	22726	3.859	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	77.200%
46) 2-Hexanone-d5	8.085	63	99357	40.419	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	80.840%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	44726	4.013	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	80.200%
66) 1,2-Dichlorobenzene-d4	11.622	152	73733	5.173	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.400%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.500	84	7657	0.596	ug/L	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028177.D
Acq On : 29 Sep 2022 11:21
Operator : SY/MD
Sample : N4856-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Sep 30 01:46:34 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

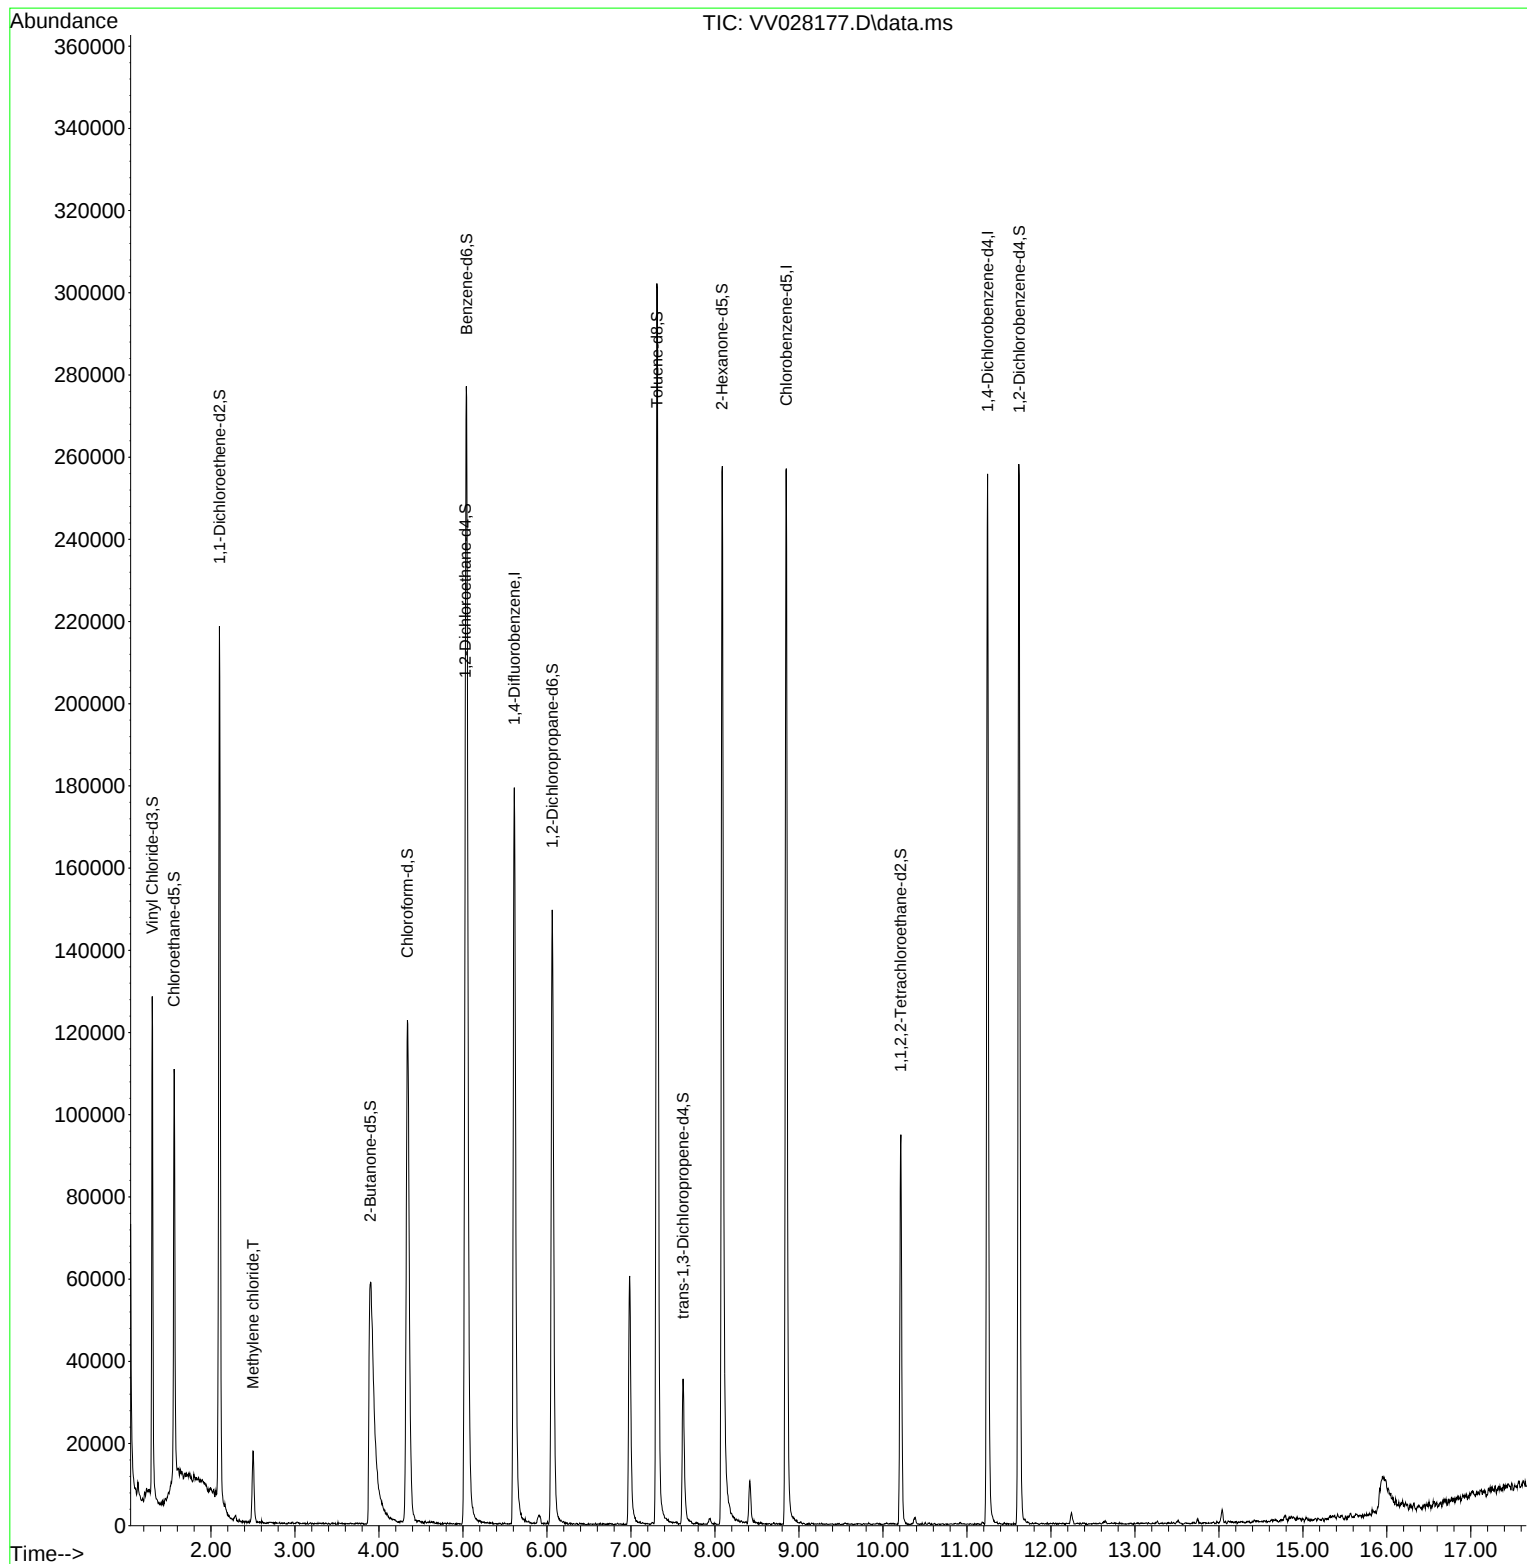

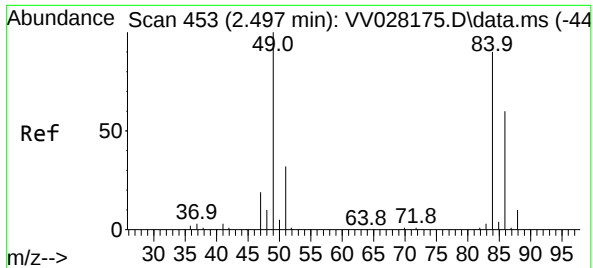

#16
Methylene chloride
Concen: 0.596 ug/L
RT: 2.500 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV028177.D
Acq: 29 Sep 2022 11:21

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 7657
Ion Ratio Lower Upper
84 100
86 56.6 46.8 86.8
49 100.2 87.5 162.5

