

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028181.D
 Acq On : 29 Sep 2022 12:56
 Operator : SY/MD
 Sample : N4871-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H80

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

Quant Time: Oct 03 02:08:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	152729	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	140226	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	70009	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	47145	2.977	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	59.600%	
7) Chloroethane-d5	1.561	69	49370	3.922	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	78.400%	
11) 1,1-Dichloroethene-d2	2.101	63	67783	2.468	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	49.400%#	
20) 2-Butanone-d5	3.892	46	156669	58.608	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	117.220%	
24) Chloroform-d	4.342	84	119862	4.744	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	94.800%	
26) 1,2-Dichloroethane-d4	5.027	65	60702	5.049	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.043	84	213611	4.646	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.000%	
36) 1,2-Dichloropropane-d6	6.066	67	70435	4.914	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	98.200%	
41) Toluene-d8	7.313	98	155492	3.736	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	74.800%	
43) trans-1,3-Dichloroprop...	7.622	79	20244	3.910	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.200%	
46) 2-Hexanone-d5	8.085	63	118194	54.694	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	109.380%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48001	4.899	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	11.619	152	68544	4.992	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	99.800%	
Target Compounds					Qvalue	
13) Acetone	2.191	43	8525m	4.140	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028181.D
Acq On : 29 Sep 2022 12:56
Operator : SY/MD
Sample : N4871-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
F5H80

Quant Time: Oct 03 02:08:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 10/05/2022
Supervised By :Mahesh Dadoda 10/05/2022

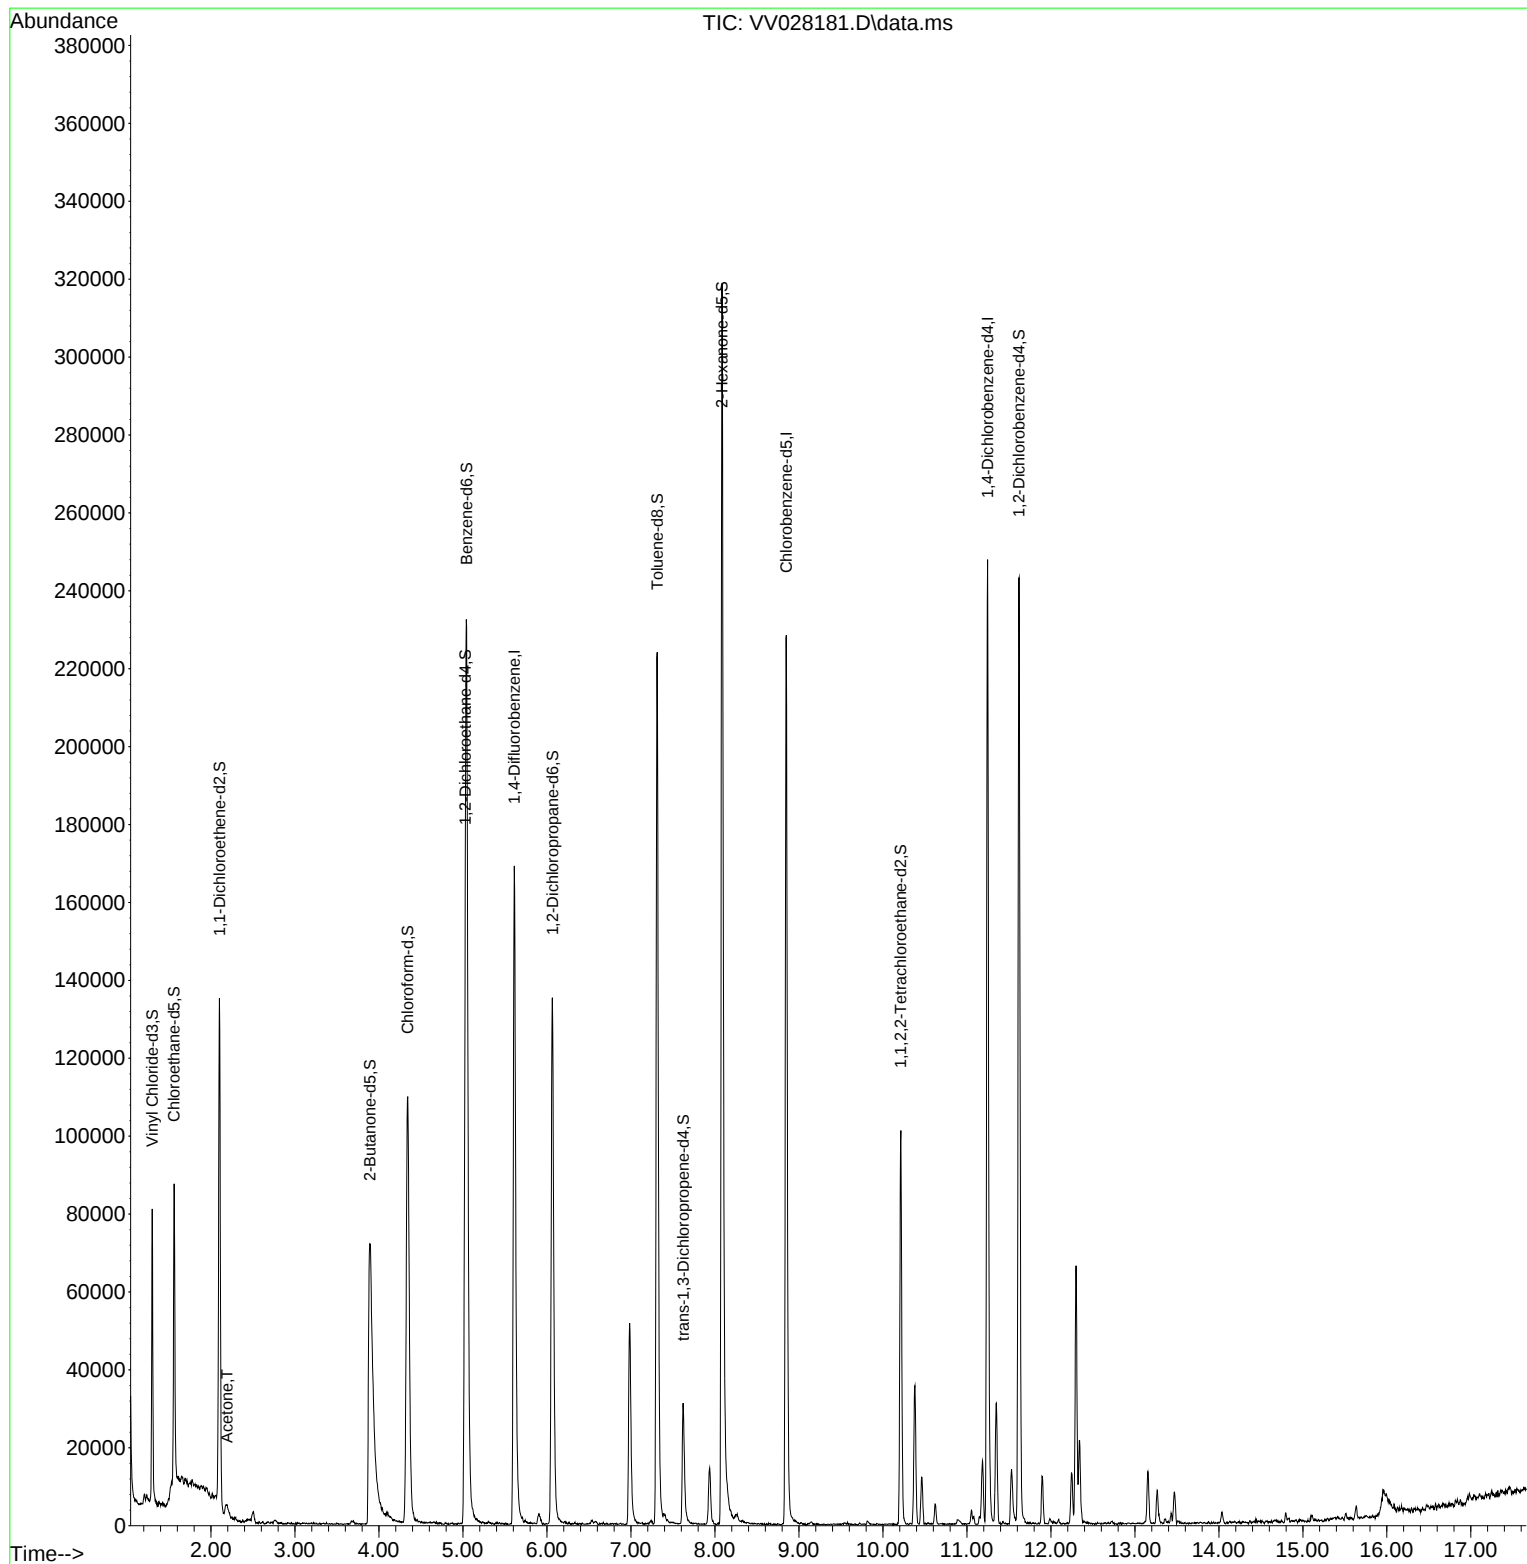

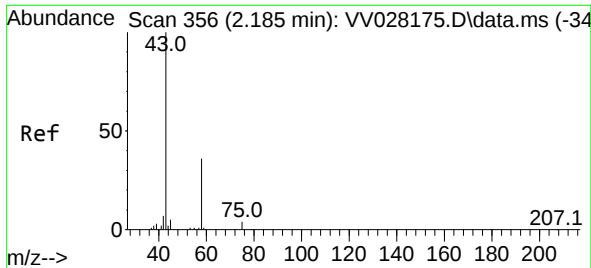

#13
 Acetone
 Concen: 4.140 ug/L m
 RT: 2.191 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV028181.D
 Acq: 29 Sep 2022 12:56

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H80

Tgt Ion: 43 Resp: 852
 Ion Ratio Lower Upper
 43 100
 58 32.4 0.0 65.6

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 10/05/2022
 Supervised By :Mahesh Dadoda 10/05/2022

