

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028193.D
 Acq On : 29 Sep 2022 18:04
 Operator : SY/MD
 Sample : VV0929WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK239

Quant Time: Sep 30 01:49:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 29 01:25:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	159337	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	156023	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	69972	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	72161	4.368	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.400%
7) Chloroethane-d5	1.561	69	59467	4.528	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	90.600%
11) 1,1-Dichloroethene-d2	2.101	63	97025	3.386	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.800%
20) 2-Butanone-d5	3.899	46	113428	40.673	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.340%
24) Chloroform-d	4.346	84	121036	4.592	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
26) 1,2-Dichloroethane-d4	5.034	65	57952	4.620	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.400%
32) Benzene-d6	5.047	84	242544	4.741	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
36) 1,2-Dichloropropane-d6	6.066	67	72686	4.557	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.200%
41) Toluene-d8	7.313	98	199170	4.301	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%
43) trans-1,3-Dichloroprop...	7.622	79	21295	3.696	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.000%
46) 2-Hexanone-d5	8.088	63	93542	38.903	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	77.800%
56) 1,1,2,2-Tetrachloroeth...	10.214	84	48009	4.404	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	11.622	152	69080	5.033	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%
Target Compounds						
					Qvalue	
16) Methylene chloride	2.503	84	7134	0.580	ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028193.D
Acq On : 29 Sep 2022 18:04
Operator : SY/MD
Sample : VV0929WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Quant Time: Sep 30 01:49:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 29 01:25:35 2022
Response via : Initial Calibration

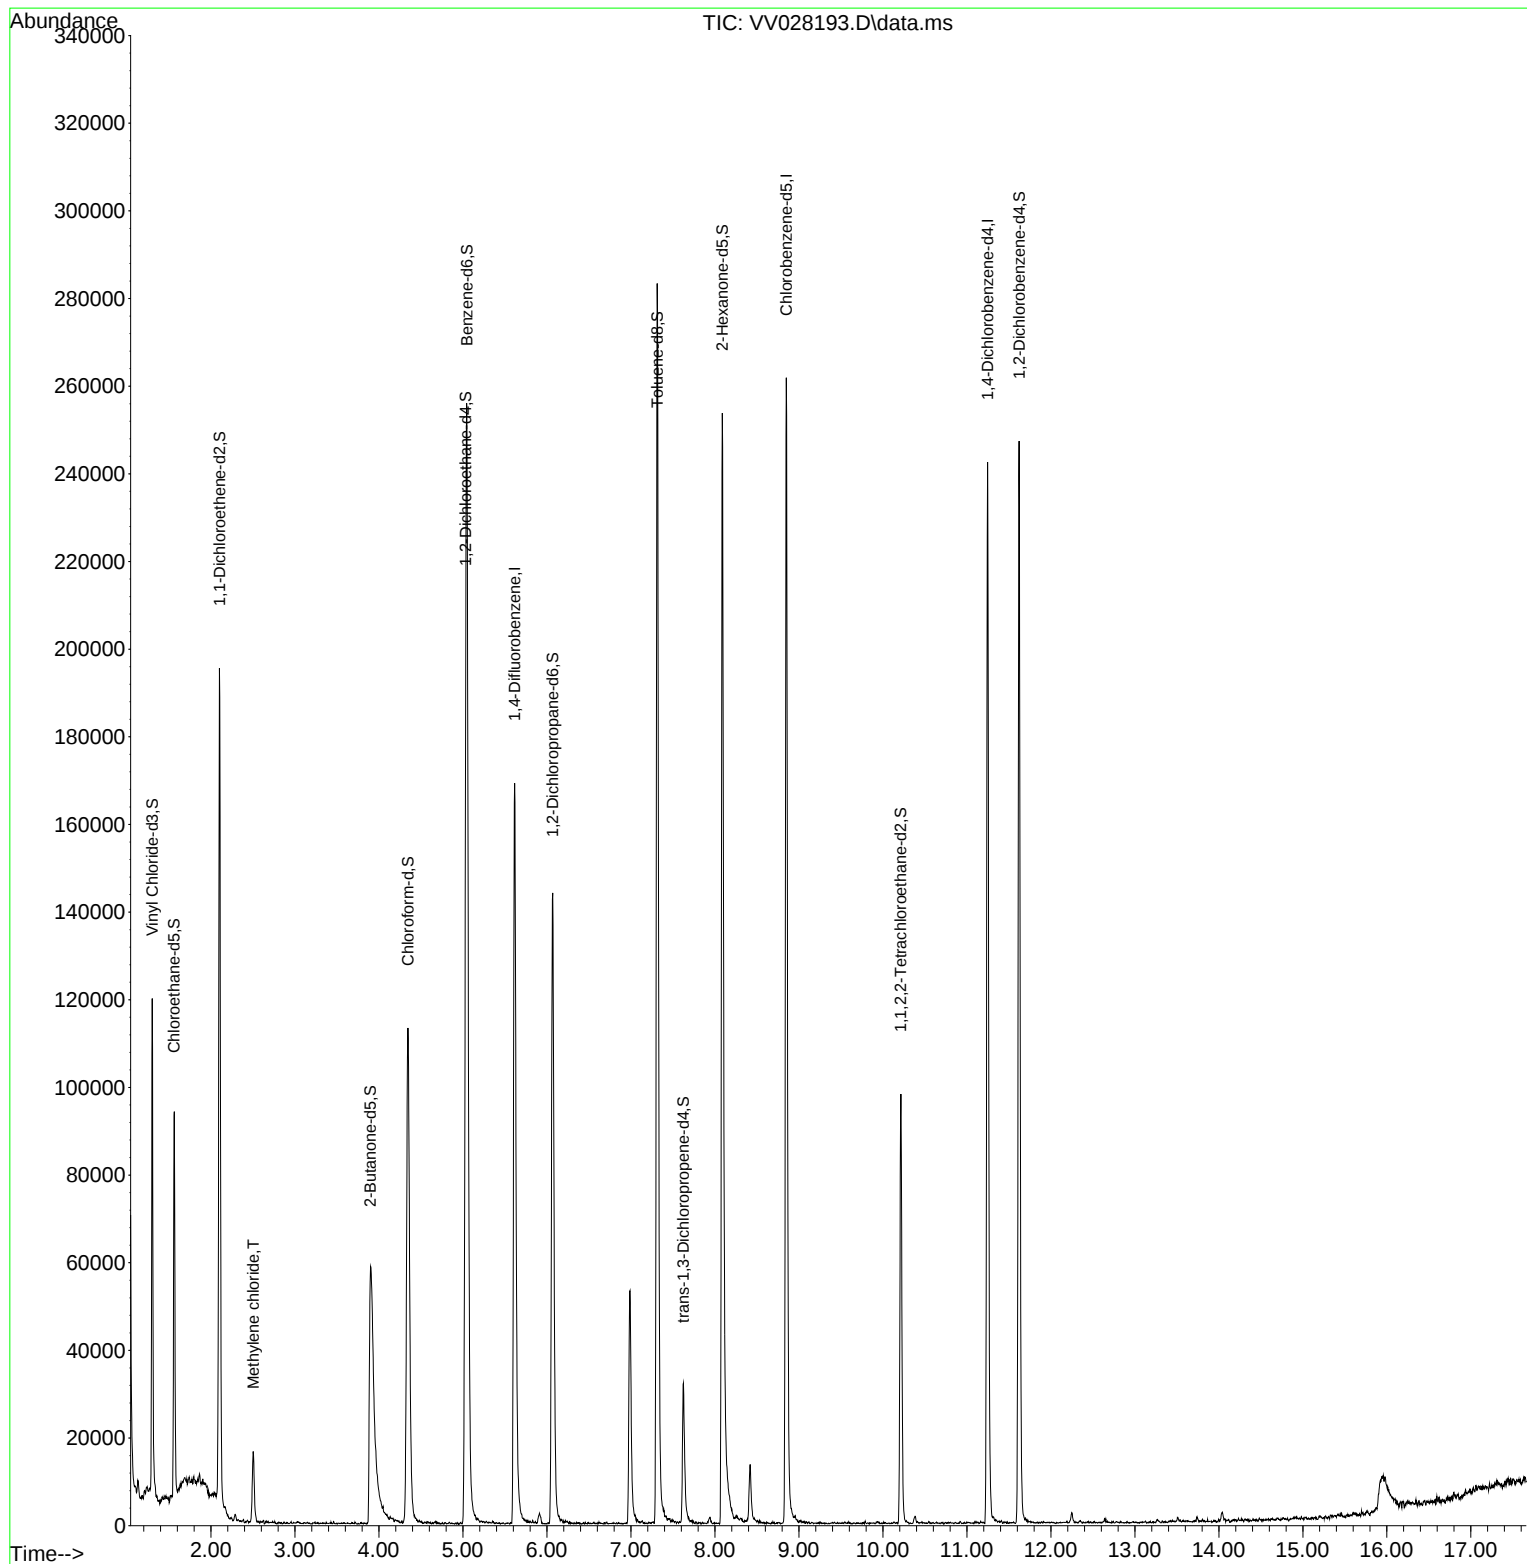

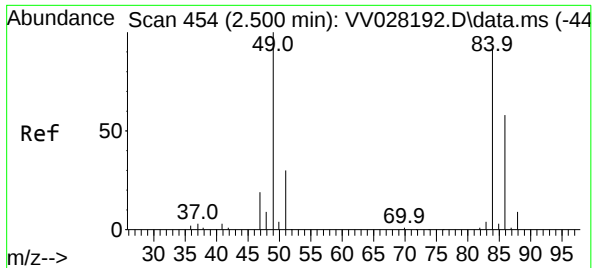

#16
Methylene chloride
Concen: 0.580 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.006 min
Lab File: VV028193.D
Acq: 29 Sep 2022 18:04

Instrument :
MSVOA_V
ClientSampleId :
VBLK239

Tgt Ion:	84	Resp:	7134
Ion	Ratio	Lower	Upper
84	100		
86	66.7	46.8	86.8
49	97.2	87.5	162.5

