

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028178.D
 Acq On : 29 Sep 2022 11:45
 Operator : SY/MD
 Sample : N4871-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H64

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028178.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	73011	74530	13.28%	1.619%
2	1.413	110	116	119	rBV2	6555	8533	1.52%	0.185%
3	1.561	156	162	178	rVB	77017	93541	16.66%	2.032%
4	2.101	321	330	344	rVB	140682	204566	36.44%	4.445%
5	3.896	876	888	933	rBV2	67662	280565	49.98%	6.096%
6	4.343	1009	1027	1062	rBV2	99396	261319	46.55%	5.678%
7	5.040	1228	1244	1269	rBV2	208606	523992	93.35%	11.385%
8	5.613	1409	1422	1440	rBV	168046	333594	59.43%	7.248%
9	6.066	1548	1563	1585	rBV	121300	252432	44.97%	5.485%
10	6.986	1839	1849	1873	rBV2	50824	98210	17.50%	2.134%
11	7.314	1939	1951	1973	rBV	208155	372546	66.37%	8.095%
12	7.622	2035	2047	2067	rBV2	30048	56364	10.04%	1.225%
13	7.937	2132	2145	2156	rBV	12359	22498	4.01%	0.489%
14	8.085	2179	2191	2220	rBV	305923	561321	100.00%	12.196%
15	8.847	2417	2428	2452	rBV	247748	418609	74.58%	9.095%
16	10.214	2842	2853	2870	rBV	104136	166629	29.69%	3.620%
17	10.381	2893	2905	2918	rBV	43277	71706	12.77%	1.558%
18	11.246	3161	3174	3193	rBV	254323	400197	71.30%	8.695%
19	11.619	3279	3290	3309	rBV	232325	378090	67.36%	8.215%
20	12.249	3475	3486	3495	rVB3	7944	13140	2.34%	0.285%
21	15.924	4617	4629	4630	rBV9	6782	10074	1.79%	0.219%




Sum of corrected areas: 4602456

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028178.D
Acq On : 29 Sep 2022 11:45
Operator : SY/MD
Sample : N4871-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

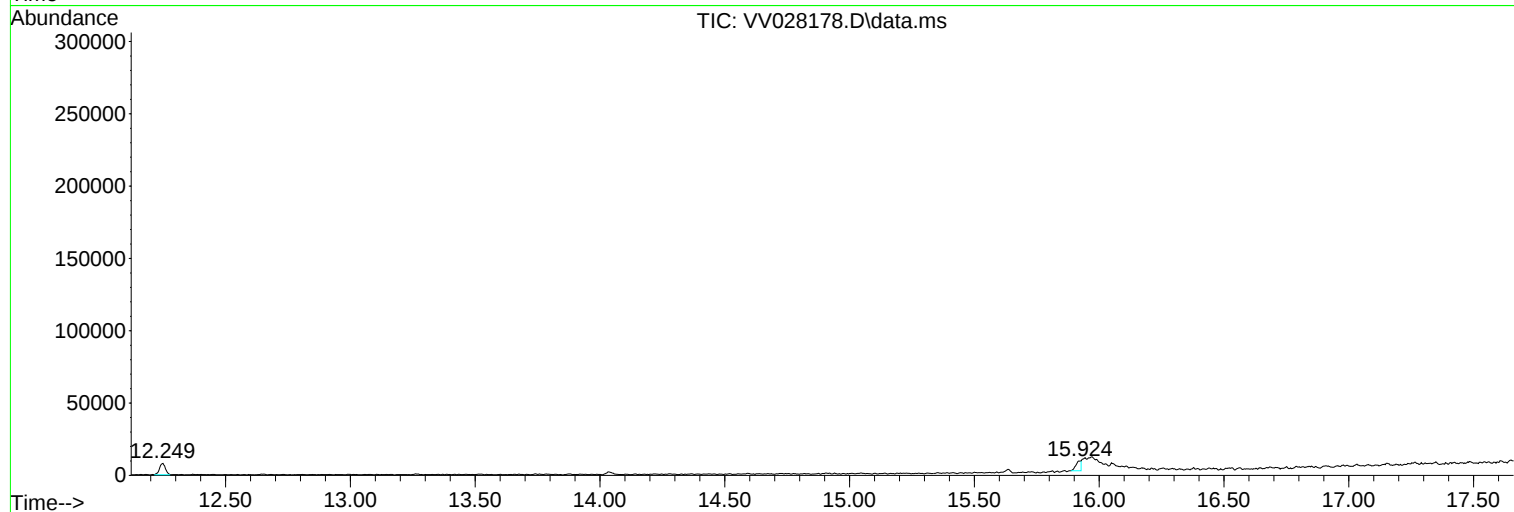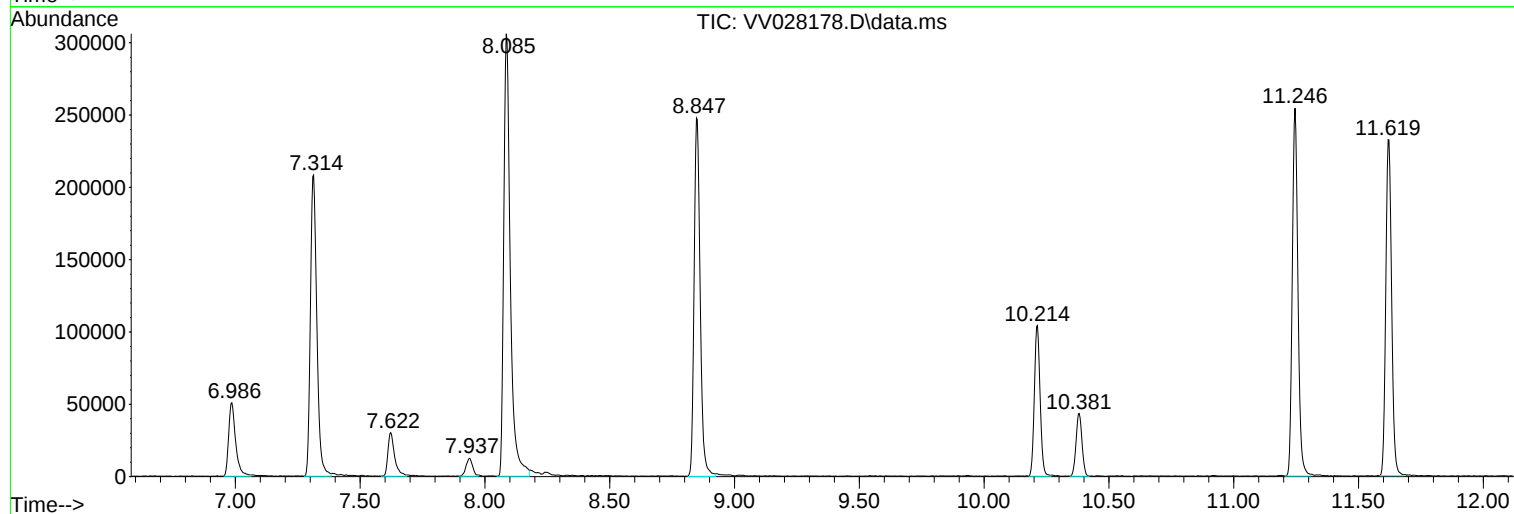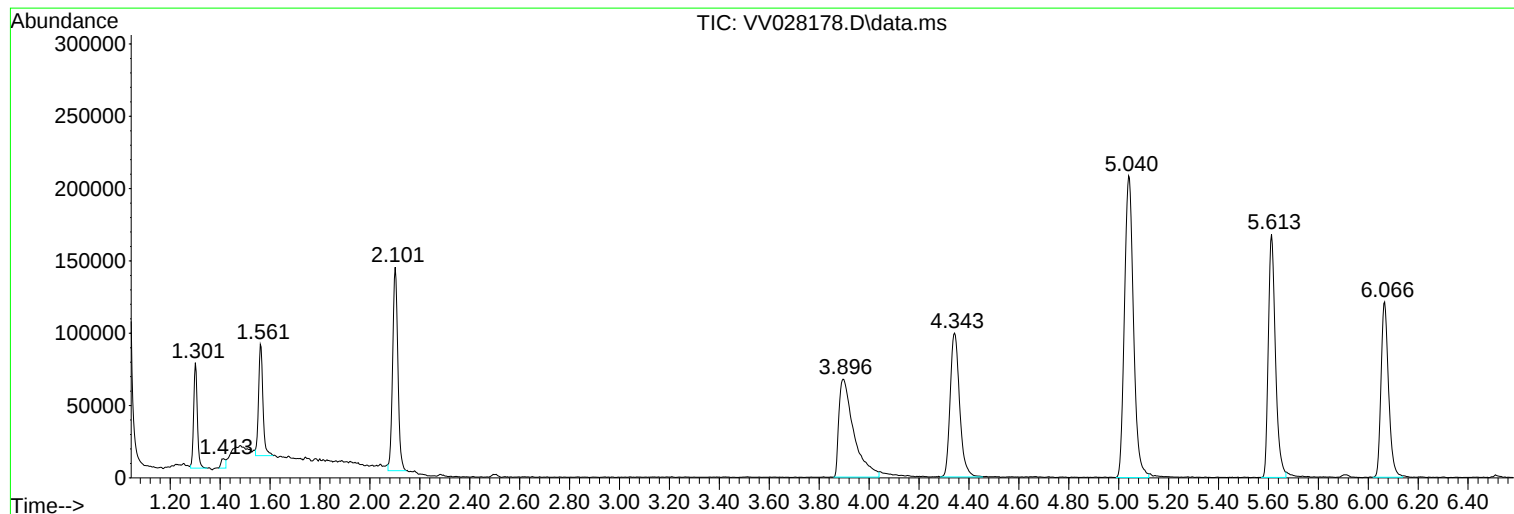

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028178.D
Acq On : 29 Sep 2022 11:45
Operator : SY/MD
Sample : N4871-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028178.D
Acq On : 29 Sep 2022 11:45
Operator : SY/MD
Sample : N4871-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H64

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc