

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028180.D
 Acq On : 29 Sep 2022 12:32
 Operator : SY/MD
 Sample : N4871-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5H71

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV028180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	94	rVB	74337	73138	13.26%	1.475%
2	1.413	110	116	122	rBV2	5800	7224	1.31%	0.146%
3	1.561	155	162	174	rVB	74976	84357	15.30%	1.701%
4	2.101	321	330	353	rVB	134886	201196	36.49%	4.056%
5	3.895	874	888	944	rBV3	72039	294071	53.33%	5.929%
6	4.342	1010	1027	1057	rBV	105044	265787	48.20%	5.359%
7	5.040	1228	1244	1276	rBV2	209764	528469	95.84%	10.654%
8	5.612	1408	1422	1446	rBV	148903	303616	55.06%	6.121%
9	6.066	1550	1563	1593	rBV	123020	251030	45.52%	5.061%
10	6.985	1838	1849	1868	rBV	48016	89359	16.21%	1.802%
11	7.313	1940	1951	1974	rBV	200487	353081	64.03%	7.118%
12	7.622	2036	2047	2066	rBV3	27407	51484	9.34%	1.038%
13	7.972	2132	2156	2175	rBV2	309160	551415	100.00%	11.117%
14	8.085	2181	2191	2208	rBV	298435	522359	94.73%	10.531%
15	8.850	2415	2429	2446	rBV	234089	378479	68.64%	7.631%
16	10.214	2842	2853	2867	rBV	102161	165922	30.09%	3.345%
17	10.381	2892	2905	2918	rBV	45368	76380	13.85%	1.540%
18	11.246	3162	3174	3192	rBV	238237	372475	67.55%	7.509%
19	11.622	3280	3291	3314	rBV	228141	371289	67.33%	7.486%
20	12.246	3475	3485	3496	rVB2	12066	18931	3.43%	0.382%




Sum of corrected areas: 4960062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028180.D
Acq On : 29 Sep 2022 12:32
Operator : SY/MD
Sample : N4871-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

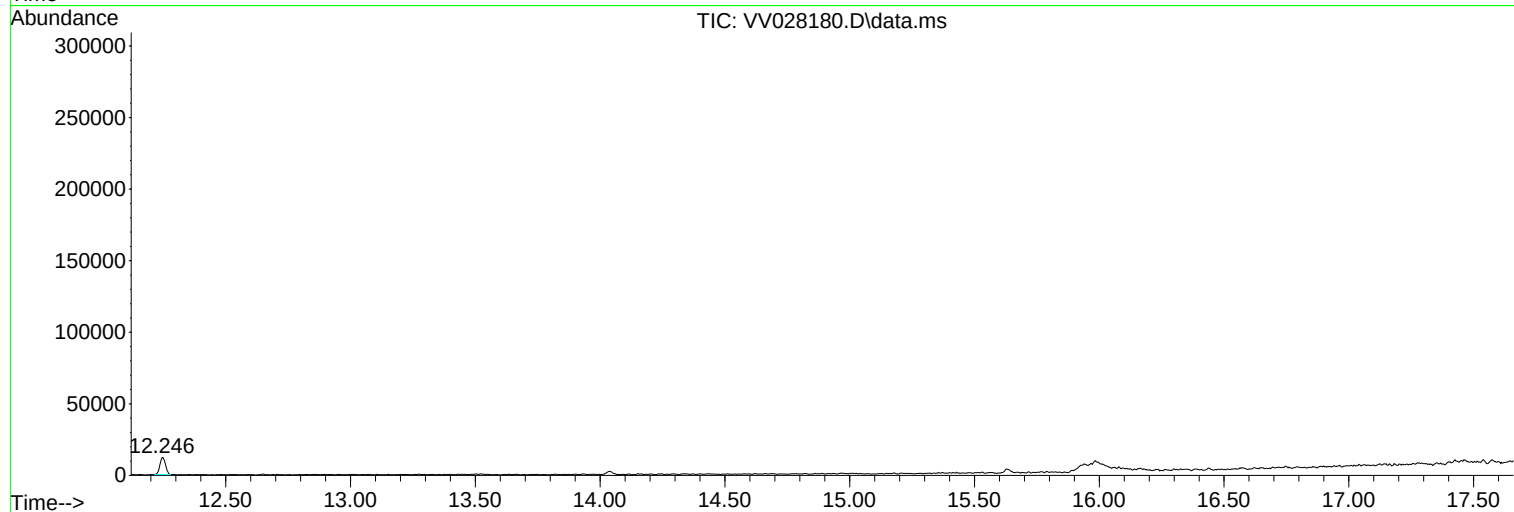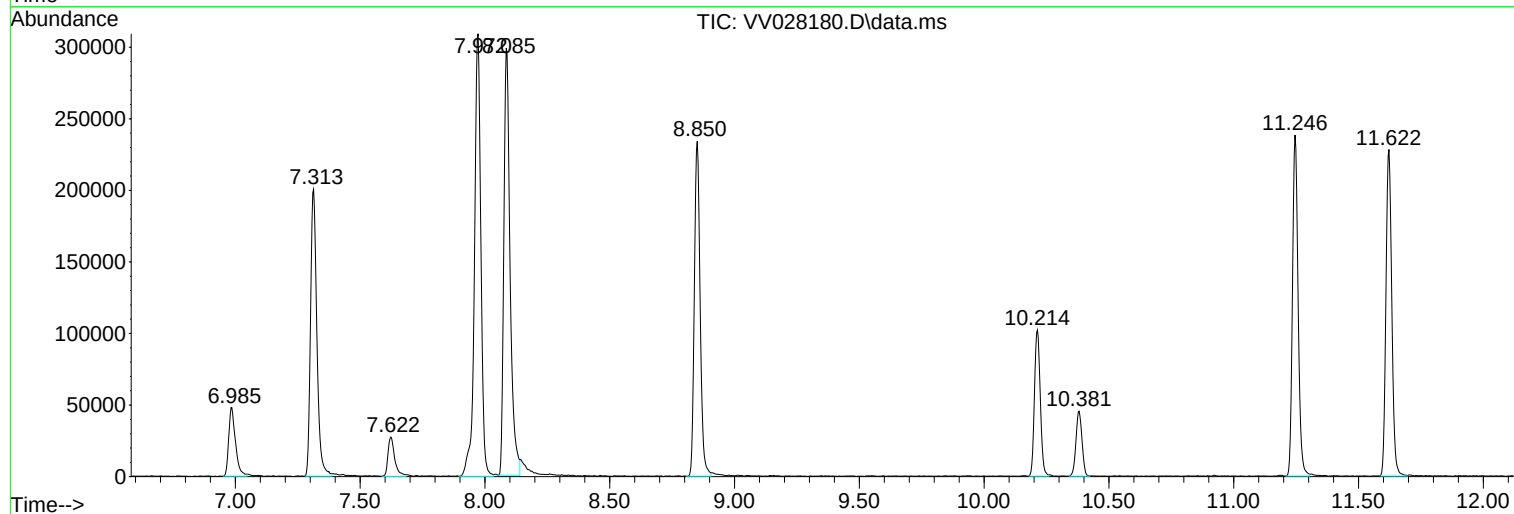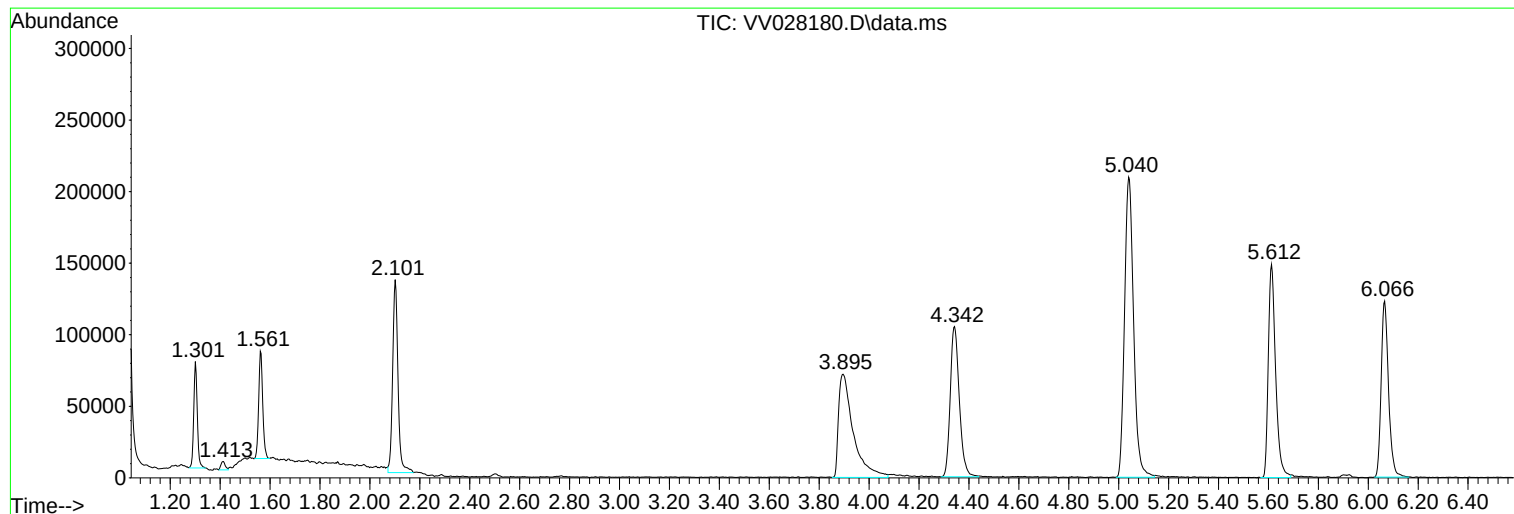

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028180.D
Acq On : 29 Sep 2022 12:32
Operator : SY/MD
Sample : N4871-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028180.D
Acq On : 29 Sep 2022 12:32
Operator : SY/MD
Sample : N4871-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5H71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
