

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028197.D
 Acq On : 29 Sep 2022 19:41
 Operator : SY/MD
 Sample : N4865-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW844

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028197.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	109044	118107	3.62%	1.491%
2	1.561	154	162	172	rBV	85798	103847	3.19%	1.311%
3	2.101	319	330	348	rVB	188159	276101	8.47%	3.486%
4	2.500	439	454	471	rBV	24000	40929	1.26%	0.517%
5	2.757	520	534	551	rBV2	32674	59277	1.82%	0.748%
6	3.899	876	889	922	rBV2	63854	226164	6.94%	2.855%
7	4.342	1010	1027	1057	rBV3	95502	244988	7.52%	3.093%
8	5.040	1227	1244	1271	rBV2	215596	541274	16.61%	6.833%
9	5.612	1409	1422	1450	rBV2	157627	322589	9.90%	4.072%
10	5.911	1505	1515	1539	rBV2	33722	71067	2.18%	0.897%
11	6.066	1550	1563	1597	rBV	120499	251662	7.72%	3.177%
12	6.985	1838	1849	1864	rBV2	52736	98875	3.03%	1.248%
13	7.313	1938	1951	1972	rBV	242928	441027	13.53%	5.568%
14	7.622	2038	2047	2065	rBV2	31750	57116	1.75%	0.721%
15	7.969	2131	2155	2175	rBV	1938462	3259122	100.00%	41.143%
16	8.085	2182	2191	2221	rVB	242190	440294	13.51%	5.558%
17	8.850	2417	2429	2448	rBV	254780	420830	12.91%	5.313%
18	10.214	2842	2853	2869	rBV	87262	137668	4.22%	1.738%
19	10.381	2893	2905	2918	rBV2	23956	40716	1.25%	0.514%
20	11.246	3163	3174	3194	rBV	253809	395021	12.12%	4.987%
21	11.622	3277	3291	3312	rBV	234060	374712	11.50%	4.730%




Sum of corrected areas: 7921386

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028197.D
Acq On : 29 Sep 2022 19:41
Operator : SY/MD
Sample : N4865-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW844

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

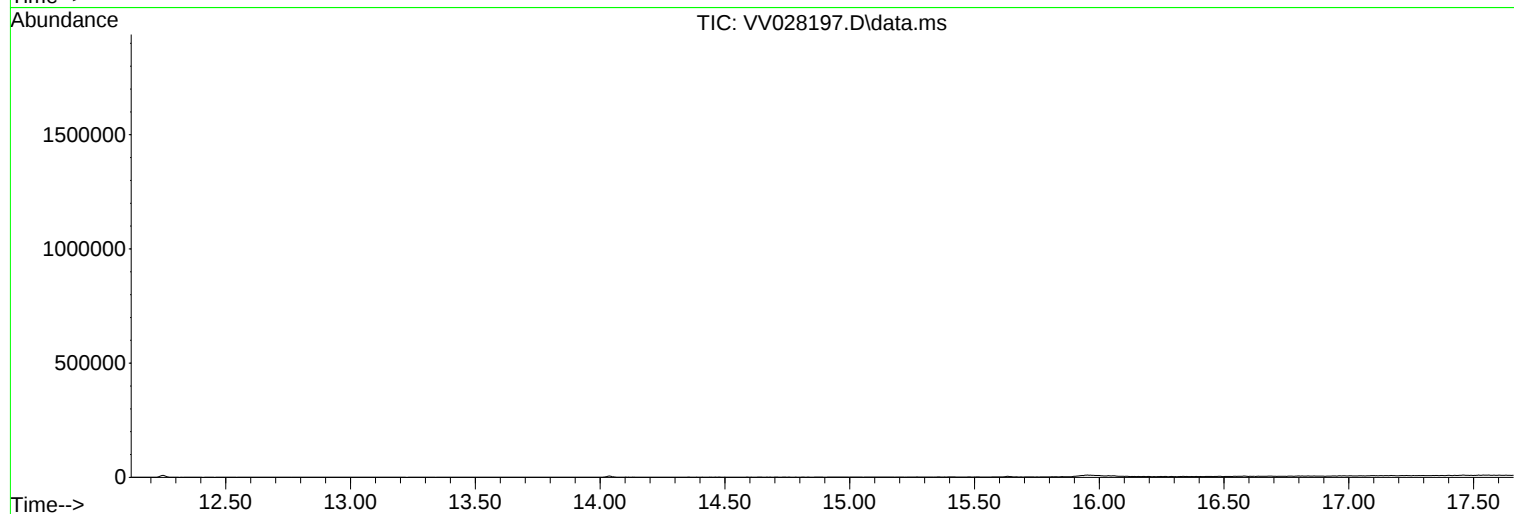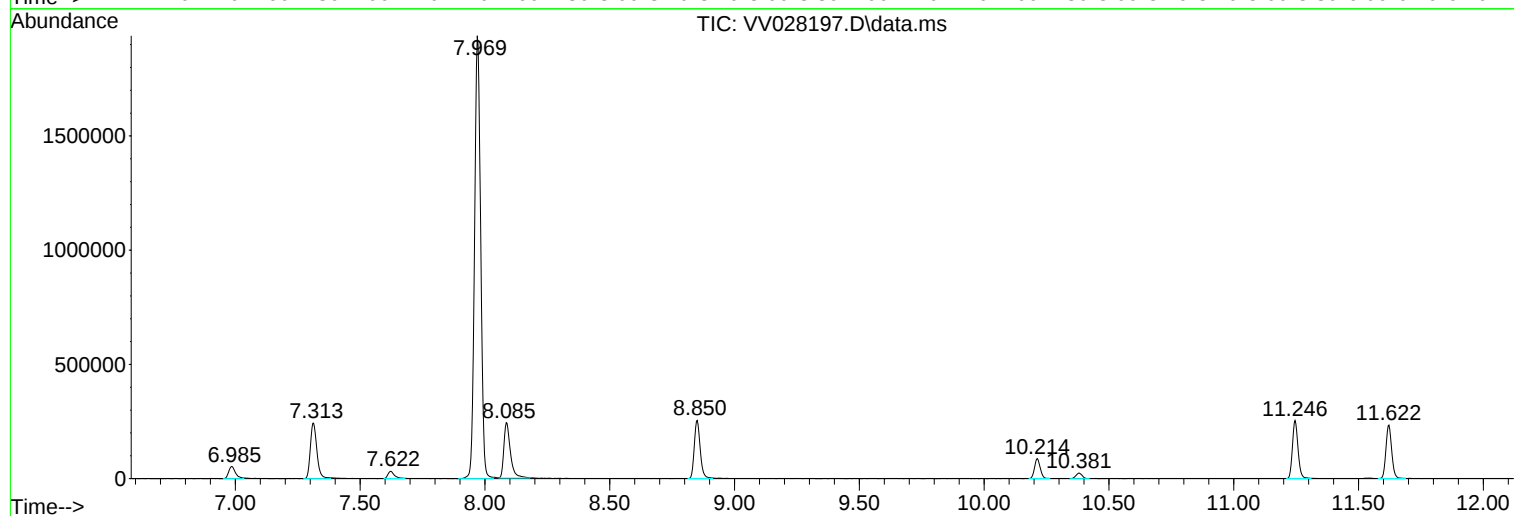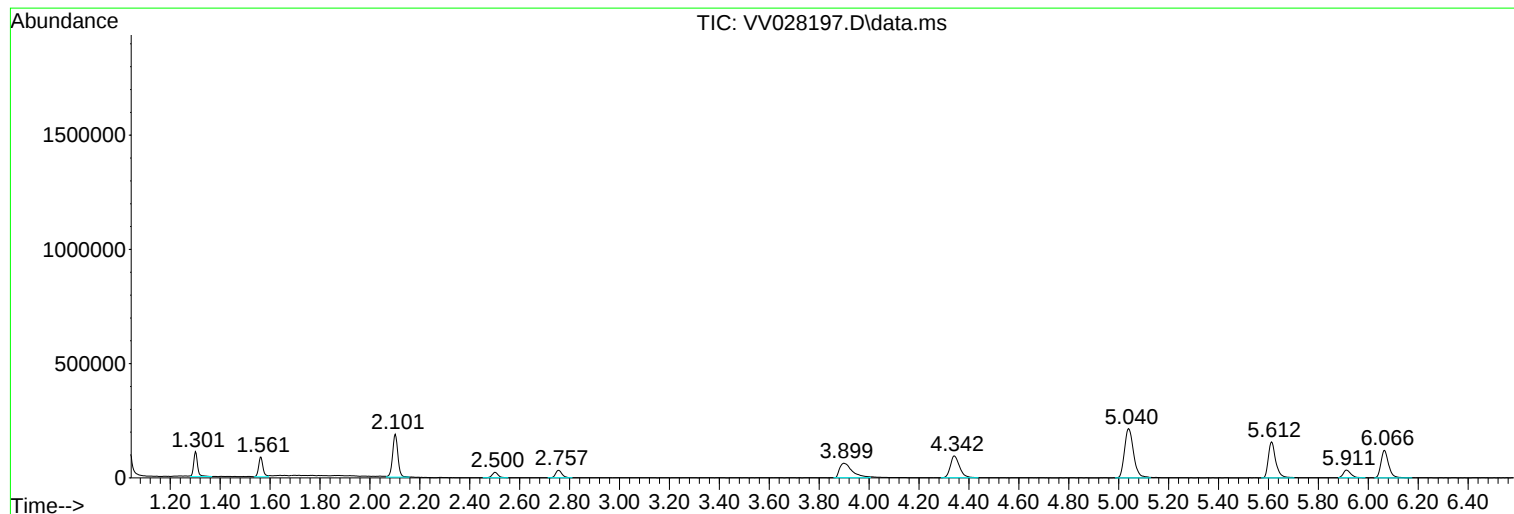

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028197.D
Acq On : 29 Sep 2022 19:41
Operator : SY/MD
Sample : N4865-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW844

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028197.D
Acq On : 29 Sep 2022 19:41
Operator : SY/MD
Sample : N4865-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW844

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc