

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028198.D
 Acq On : 29 Sep 2022 20:05
 Operator : SY/MD
 Sample : N4865-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW845

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028198.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	74	81	99	rVB	116354	122073	3.44%	1.363%
2	1.561	154	162	173	rBV	90877	110580	3.12%	1.235%
3	2.101	320	330	355	rVB	208736	308215	8.68%	3.442%
4	2.500	441	454	473	rBV	24330	42125	1.19%	0.470%
5	2.757	522	534	557	rBV2	32987	60125	1.69%	0.671%
6	3.902	878	890	926	rBV4	69264	254434	7.17%	2.841%
7	4.342	1010	1027	1061	rVB	114608	294925	8.31%	3.293%
8	5.040	1227	1244	1273	rBV2	262674	654559	18.44%	7.309%
9	5.612	1410	1422	1452	rBV	172979	360118	10.15%	4.021%
10	5.915	1504	1516	1535	rBV4	39573	83983	2.37%	0.938%
11	6.066	1547	1563	1591	rBV2	147150	306329	8.63%	3.421%
12	6.985	1838	1849	1877	rBV2	64874	124997	3.52%	1.396%
13	7.313	1939	1951	1972	rBV	293536	521441	14.69%	5.823%
14	7.622	2033	2047	2066	rBV	38270	71810	2.02%	0.802%
15	7.969	2133	2155	2181	rBV	2072889	3549176	100.00%	39.633%
16	8.088	2182	2192	2226	rVB	301835	555262	15.64%	6.200%
17	8.850	2417	2429	2451	rBV	268183	455313	12.83%	5.084%
18	10.213	2841	2853	2873	rBV	105385	167810	4.73%	1.874%
19	10.377	2894	2904	2916	rBV3	30197	48345	1.36%	0.540%
20	11.246	3163	3174	3200	rBV	273841	422938	11.92%	4.723%
21	11.622	3278	3291	3310	rBV	280936	440631	12.42%	4.920%




Sum of corrected areas: 8955189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028198.D
Acq On : 29 Sep 2022 20:05
Operator : SY/MD
Sample : N4865-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW845

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

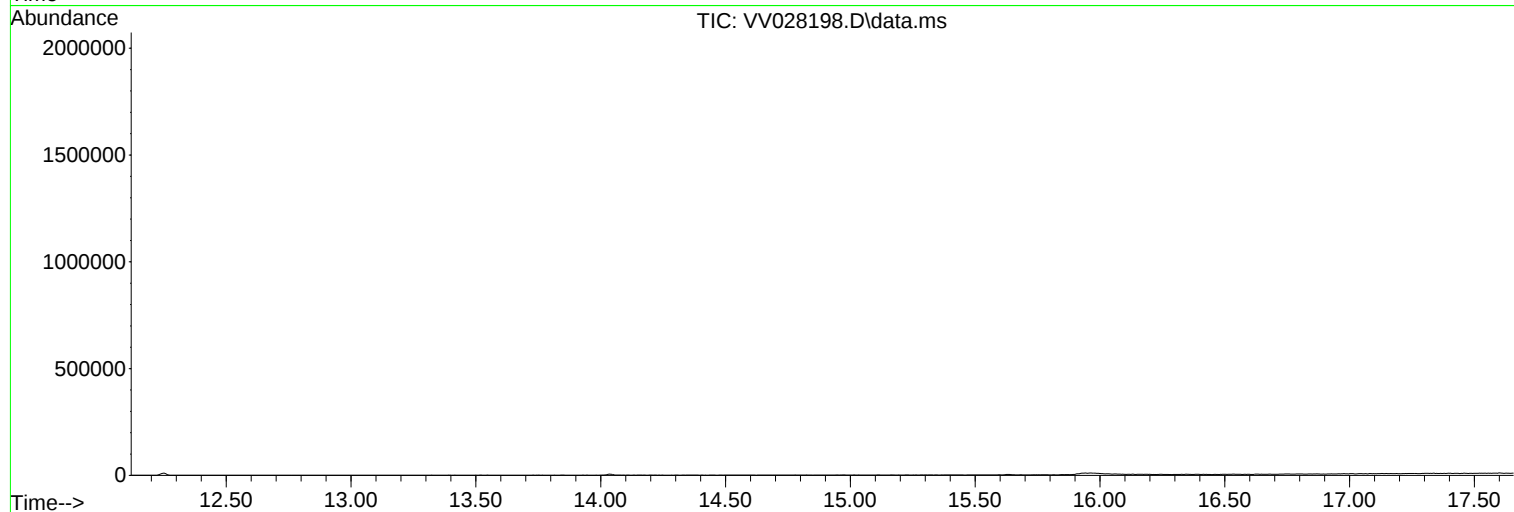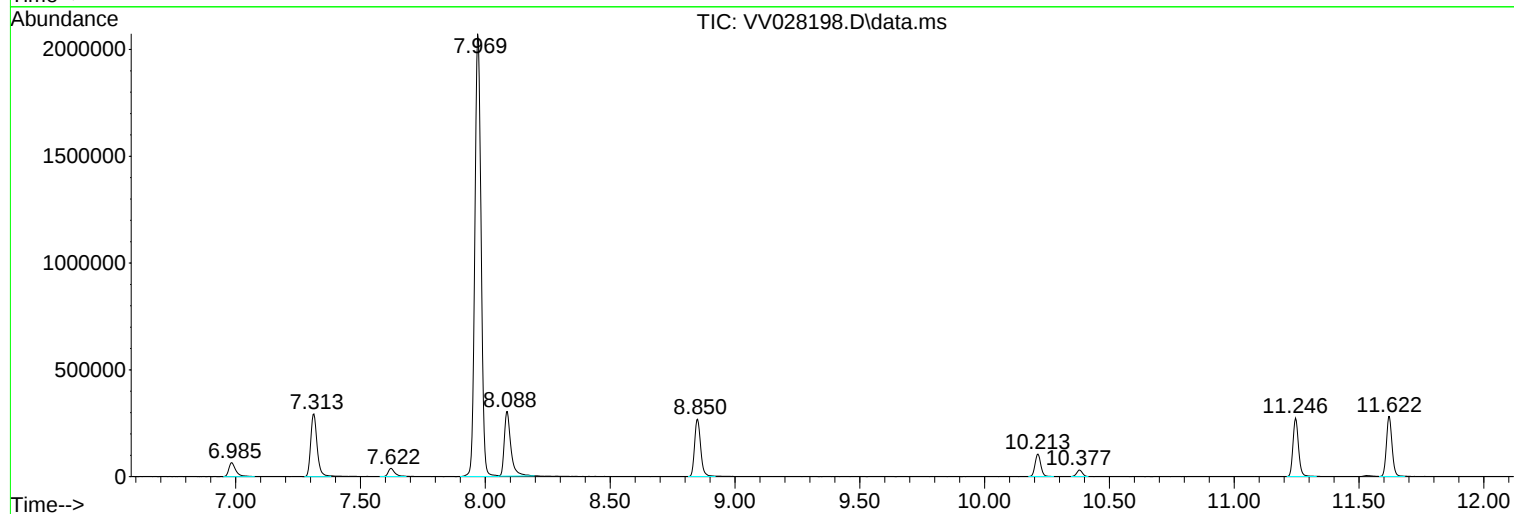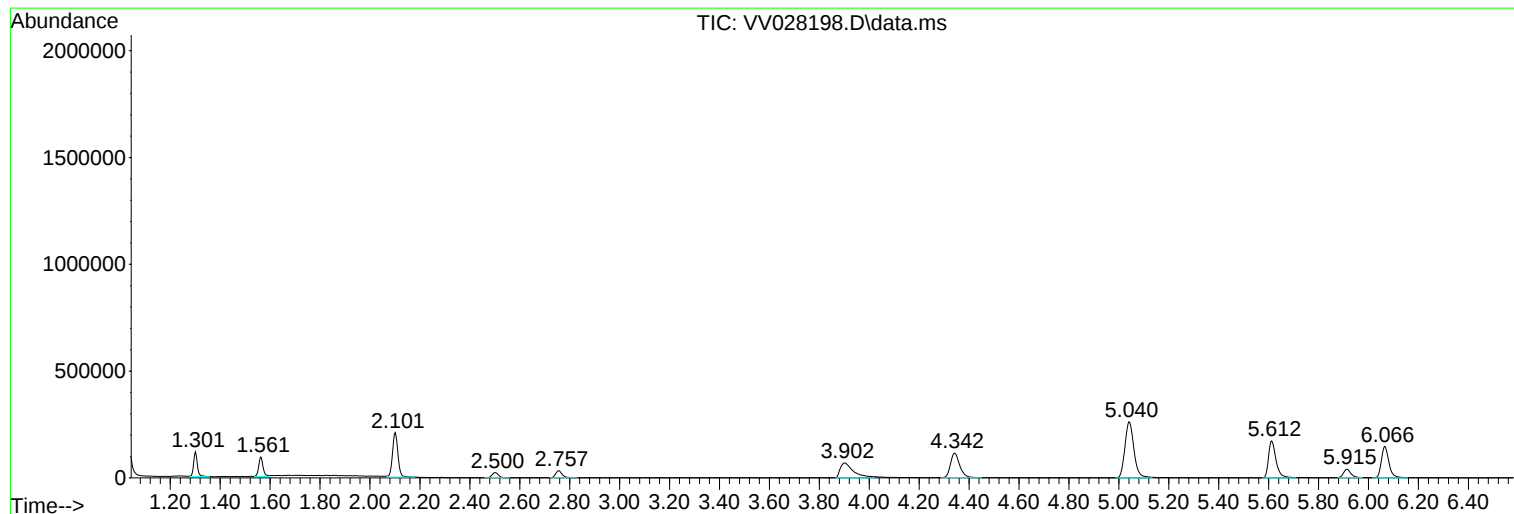

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028198.D
Acq On : 29 Sep 2022 20:05
Operator : SY/MD
Sample : N4865-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW845

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
Data File : VV028198.D
Acq On : 29 Sep 2022 20:05
Operator : SY/MD
Sample : N4865-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW845

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc