


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092922\
 Data File : VV028174.D
 Acq On : 29 Sep 2022 09:10
 Operator : SY/MD
 Sample : BFB379
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB379

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092222WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Sep 29 01:25:35 2022

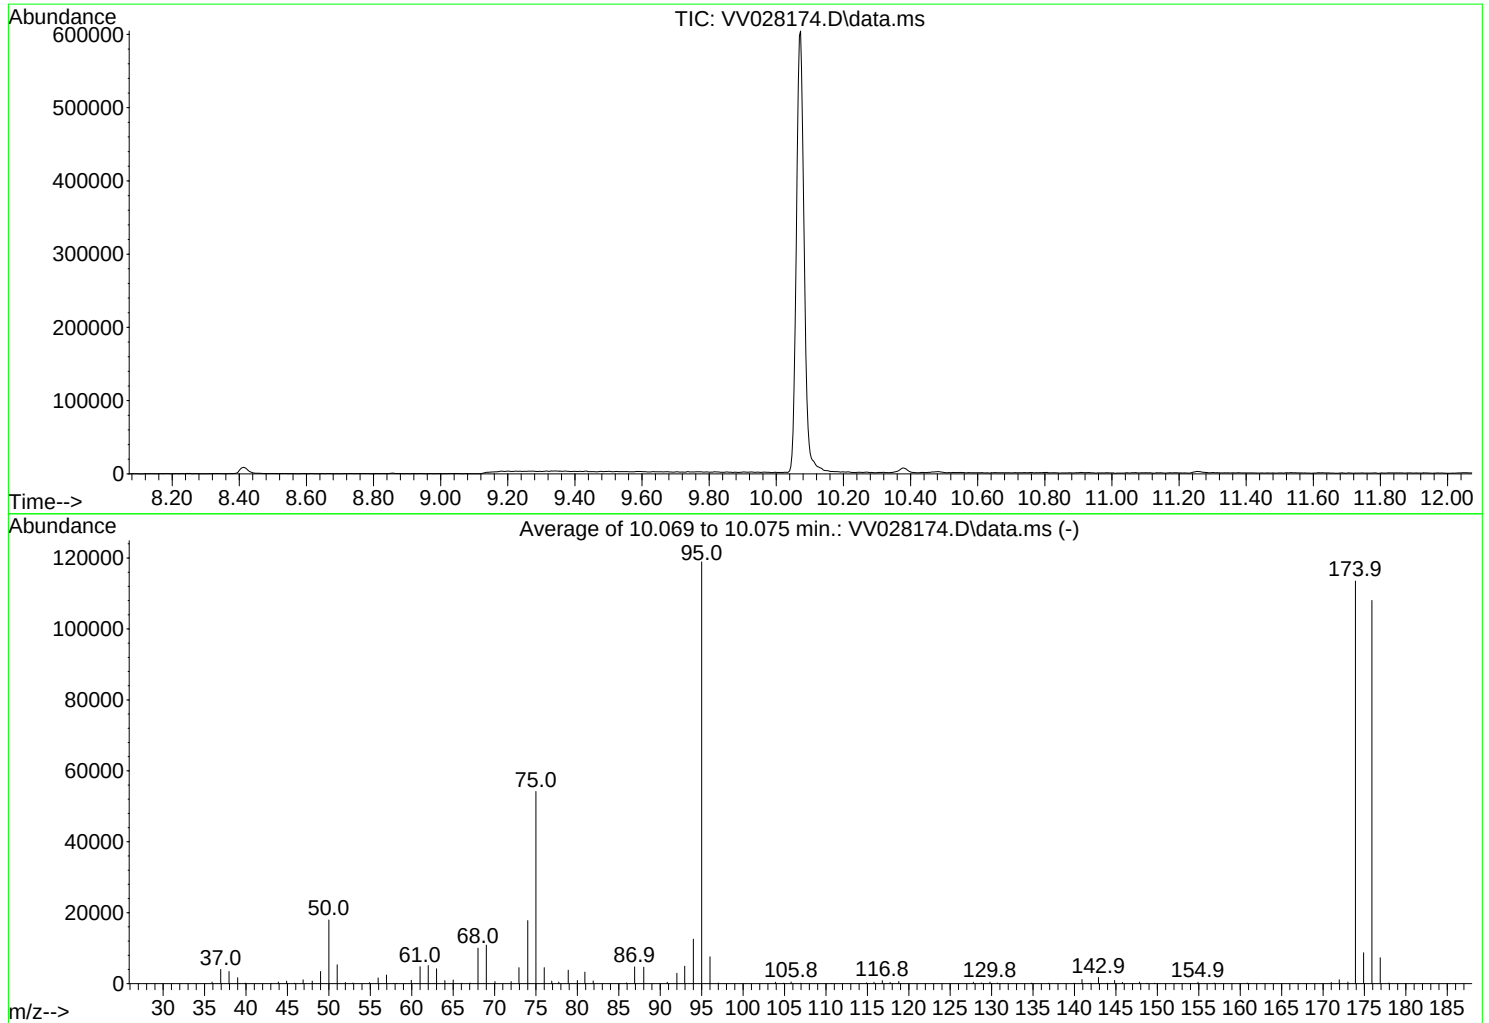

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.1	17971	PASS
75	95	30	80	45.6	54189	PASS
95	95	100	100	100.0	118928	PASS
96	95	5	9	6.4	7579	PASS
173	174	0.00	2	0.4	437	PASS
174	95	50	120	95.5	113517	PASS
175	174	5	9	7.7	8721	PASS
176	174	95	105	95.2	108069	PASS
177	176	5	10	6.7	7288	PASS

m/z	Abundance
35.90	1309.0
36.90	168.0
37.90	463.0
39.90	107.0
43.80	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
36.00	1751.0
37.00	4291.0
38.00	3920.0
39.00	1867.0
39.90	324.0
43.00	132.0
44.00	668.0
44.90	761.0
45.90	171.0
46.90	1163.0
48.00	717.0
49.00	3538.0
50.00	18704.0
51.00	5723.0
52.00	282.0
53.00	163.0
54.90	322.0
55.90	1679.0
57.00	2588.0
57.80	148.0
59.90	1013.0
61.00	4929.0
62.00	5177.0
63.00	4282.0
64.00	891.0
65.00	1082.0
66.00	110.0
68.00	10494.0
69.00	11484.0
70.10	608.0
72.00	492.0
73.00	4626.0
74.00	18336.0
75.00	57080.0
76.00	4545.0
76.90	780.0
77.80	474.0
78.90	3950.0
80.00	931.0
80.90	3436.0
81.90	756.0
85.90	209.0
86.90	4940.0
88.00	4987.0
90.90	418.0
92.00	2989.0
92.90	5109.0
94.00	12958.0
95.00	121664.0
96.00	7871.0
97.00	199.0
103.90	434.0
104.80	161.0
105.80	516.0
106.90	133.0
110.70	119.0
114.90	188.0
115.80	468.0
116.80	843.0
117.80	323.0
118.90	699.0
127.80	404.0
128.80	227.0
129.80	438.0
130.70	158.0
134.90	228.0
137.00	169.0
140.00	150.0
140.90	1093.0
141.70	189.0
142.90	1691.0
144.00	133.0
144.90	985.0
145.80	325.0
147.90	440.0
148.70	125.0
149.70	110.0
154.90	347.0
156.80	141.0
160.90	161.0
171.00	282.0
172.00	1102.0
173.90	114664.0
174.90	9006.0
175.90	108240.0
176.90	7659.0
178.00	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
36.00	1827.0
37.00	4324.0
38.00	3923.0
39.00	1708.0
39.90	271.0
43.10	107.0
44.00	645.0
44.90	725.0
45.90	162.0
46.90	1118.0
48.00	767.0
49.00	3513.0
50.00	18712.0
51.00	5593.0
52.00	315.0
52.90	175.0
54.90	312.0
55.90	1654.0
57.00	2471.0
57.80	133.0
58.20	114.0
60.00	965.0
61.00	4975.0
62.00	5323.0
63.00	4320.0
64.00	878.0
65.00	1050.0
66.10	161.0
67.10	271.0
68.00	10381.0
69.00	11287.0
70.10	606.0
72.00	599.0
73.00	4641.0
74.00	18336.0
75.00	55888.0
76.00	4636.0
76.90	728.0
77.70	465.0
78.90	3907.0
80.00	932.0
80.90	3334.0
81.90	788.0
86.00	235.0
86.90	4892.0
88.00	4839.0
90.80	407.0
92.00	2988.0
93.00	5058.0
94.00	12935.0
95.00	123200.0
96.00	7770.0
97.00	219.0
103.90	411.0
104.80	151.0
105.80	551.0
107.00	149.0
114.90	222.0
115.80	434.0
116.80	871.0
117.80	386.0
118.80	624.0
127.80	437.0
128.70	248.0
129.80	496.0
130.70	176.0
134.90	202.0
136.80	166.0
139.90	132.0
140.90	1190.0
141.90	185.0
142.90	1814.0
144.00	163.0
144.90	973.0
145.80	370.0
147.80	491.0
148.70	122.0
149.70	140.0
154.90	443.0
156.90	168.0
160.90	134.0
171.00	327.0
171.90	1166.0
173.90	117408.0
174.90	8965.0
175.90	111624.0
176.90	7510.0
177.90	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379

m/z	Abundance
36.00	1773.0
37.00	3906.0
38.00	3789.0
39.00	1433.0
39.90	216.0
43.90	668.0
44.90	631.0
45.80	128.0
46.90	1002.0
48.00	709.0
49.00	3190.0
50.00	16496.0
51.00	4656.0
52.00	322.0
52.80	175.0
54.90	241.0
56.00	1530.0
56.90	2211.0
58.20	123.0
60.00	872.0
61.00	4493.0
62.00	4790.0
63.00	3935.0
64.00	738.0
65.00	970.0
66.10	169.0
67.00	230.0
68.00	9201.0
69.00	9866.0
70.00	599.0
72.00	614.0
72.90	4320.0
74.00	16720.0
75.00	49600.0
76.00	4317.0
76.90	619.0
77.70	462.0
78.90	3504.0
80.00	802.0
80.90	3036.0
81.90	789.0
86.00	204.0
86.90	4351.0
88.00	4109.0
90.80	366.0
92.00	2784.0
93.00	4542.0
94.00	11712.0
95.00	111920.0
96.00	7095.0
97.00	192.0
103.90	376.0
104.90	131.0
105.80	447.0
107.00	135.0
114.90	218.0
115.80	378.0
116.80	806.0
117.70	416.0
118.70	569.0
127.80	444.0
128.80	223.0
129.80	462.0
130.70	192.0
134.80	178.0
136.80	126.0
139.90	104.0
140.90	1202.0
142.00	166.0
142.90	1704.0
143.90	168.0
144.80	815.0
145.80	327.0
147.80	397.0
148.80	105.0
149.70	163.0
154.90	461.0
156.90	184.0
160.70	102.0
160.80	104.0
171.00	326.0
171.90	1044.0
173.00	1311.0
173.90	108480.0
174.90	8192.0
175.90	104344.0
176.90	6695.0
177.90	205.0

Instrument :
MSVOA_V
ClientSampleId :
BFB379