

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV093024\  
 Data File : VV037644.D  
 Acq On : 30 Sep 2024 11:03  
 Operator : SY/MD  
 Sample : VV0930WBLO1  
 Misc : 5mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :

Quant Time: Oct 01 02:05:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Oct 01 02:04:27 2024  
 Response via : Initial Calibration


Compound	R. T.	QI on	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	693226	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	666173	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	316829	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	271447	44.606	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	89.220%		
7) Chloroethane-d5	1.532	69	212164	44.916	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	89.840%		
11) 1,1-Dichloroethene-d2	2.060	65	116288	45.739	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	91.480%		
21) 2-Butanone-d5	3.793	46	173608	80.096	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	80.100%		
24) Chloroform-d	4.243	84	471914	43.588	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	87.180%		
26) 1,2-Dichloroethane-d4	4.937	65	291091	45.934	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	91.860%		
32) Benzene-d6	4.953	84	960805	46.091	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	92.180%		
36) 1,2-Dichloropropane-d6	5.986	67	296959	44.737	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	89.480%		
41) Toluene-d8	7.236	98	861108	45.555	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	91.120%		
43) trans-1,3-Dichloropropene	7.548	79	131750	42.726	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	85.460%		
47) 2-Hexanone-d5	8.024	63	105476	75.251	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery =	75.250%		
56) 1,1,2,2-Tetrachloroethene	10.146	84	320169	41.511	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	83.020%		
66) 1,2-Dichlorobenzene-d4	11.554	152	325991	48.829	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	97.660%		
Target Compounds						
39) cis-1,3-Dichloropropene	6.905	75	8657	1.045	ug/L	Qvalue # 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV093024\  
 Data File : VV037644.D  
 Acq On : 30 Sep 2024 11:03  
 Operator : SY/MD  
 Sample : VV0930WBL01  
 Misc : 5mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

**Instrument :**  
 MSVOA\_V  
**ClientSampleId :**

Quant Time: Oct 01 02:05:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVLM092624WMA.M  
 Quant Title : VOC Analysis  
 QLast Update : Tue Oct 01 02:04:27 2024  
 Response via : Initial Calibration

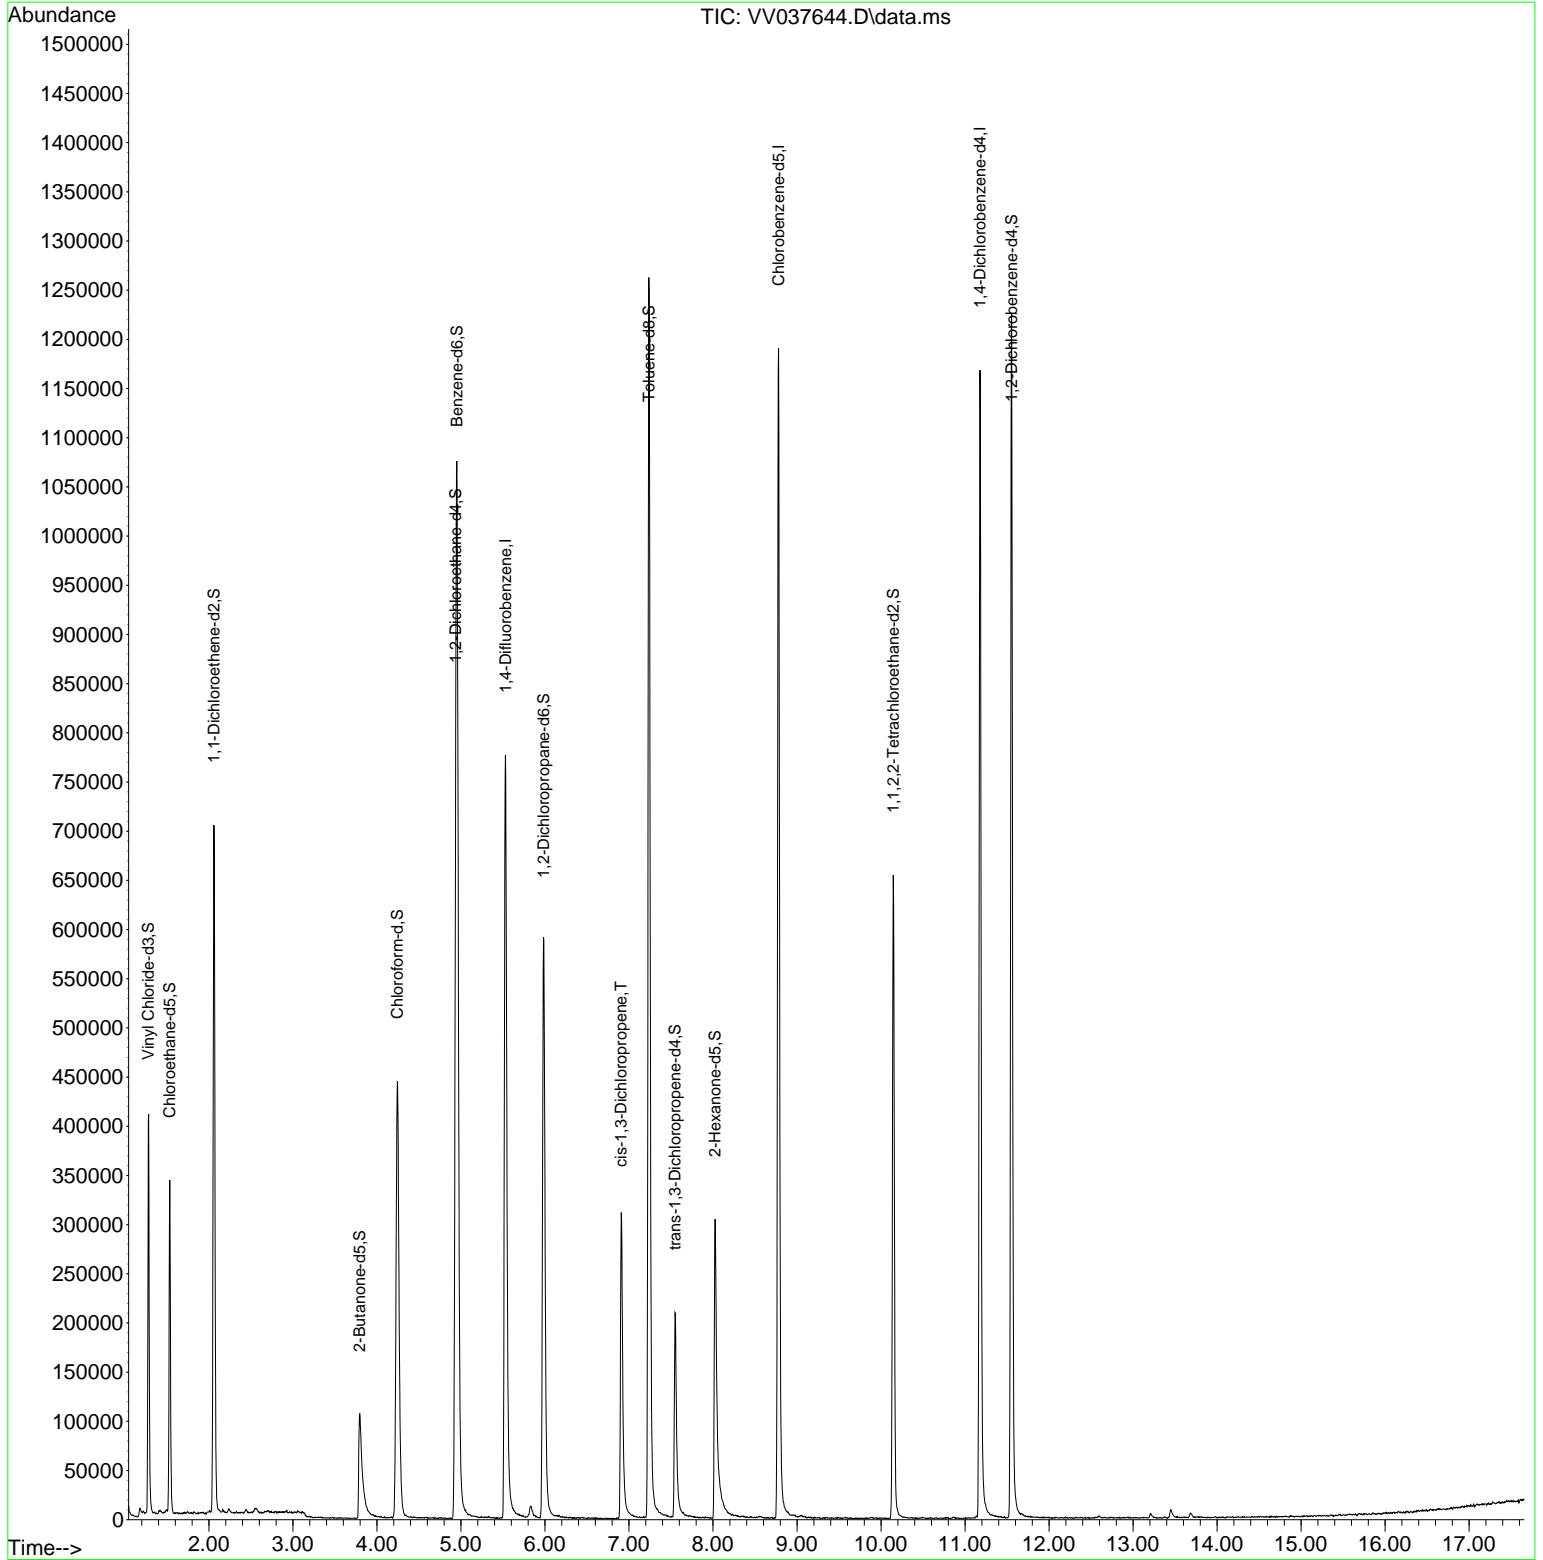

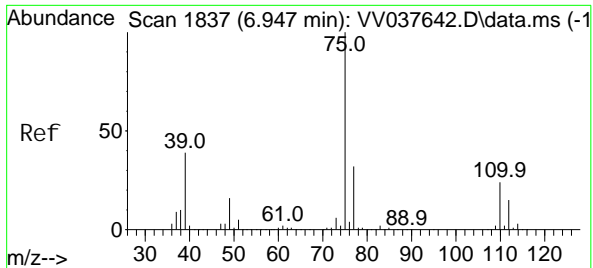

#39  
 ci s-1, 3-Di chl oropropene  
 Concen: 1.045 ug/L  
 RT: 6.905 min Scan# 18  
 Delta R.T. -0.042 min  
 Lab File: VV037644.D  
 Acq: 30 Sep 2024 11:03

Instrument : MSVOA\_V  
 ClientSampleId :

Tgt Ion: 75 Resp: 8657  
 Ion Ratio Lower Upper  
 75 100  
 77 44.0 21.8 40.4#

