

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037667.D
 Acq On : 30 Sep 2024 19:34
 Operator : SY/MD
 Sample : P4162-14
 Misc : 5.20g/5mL/100ul/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 01 02:11:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 01 02:04:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	711015	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	689865	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	341774	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	155688	24.944	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	49.880%#
7) Chloroethane-d5	1.510	69	87171	17.993	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	35.980%#
11) 1,1-Dichloroethene-d2	2.044	65	75684	29.024	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	58.040%#
21) 2-Butanone-d5	3.802	46	120208	54.071	ug/L	0.02
Spiked Amount	100.000	Range	40 - 130	Recovery	=	54.070%
24) Chloroform-d	4.240	84	389002	35.031	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	70.060%
26) 1,2-Dichloroethane-d4	4.934	65	246204	37.879	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.760%
32) Benzene-d6	4.950	84	756045	35.023	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	70.040%
36) 1,2-Dichloropropane-d6	5.982	67	248161	36.101	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	72.200%
41) Toluene-d8	7.236	98	673512	34.407	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	68.820%#
43) trans-1,3-Dichloroprop...	7.551	79	112974	35.379	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	70.760%
47) 2-Hexanone-d5	8.034	63	119613	82.406	ug/L	0.01
Spiked Amount	100.000	Range	45 - 130	Recovery	=	82.410%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	304641	38.142	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.280%
66) 1,2-Dichlorobenzene-d4	11.554	152	293755	40.789	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.580%
Target Compounds						
					Qvalue	
15) Methyl Acetate	2.375	43	11754	3.091	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037667.D
Acq On : 30 Sep 2024 19:34
Operator : SY/MD
Sample : P4162-14
Misc : 5.20g/5mL/100ul/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 01 02:11:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 01 02:04:27 2024
Response via : Initial Calibration

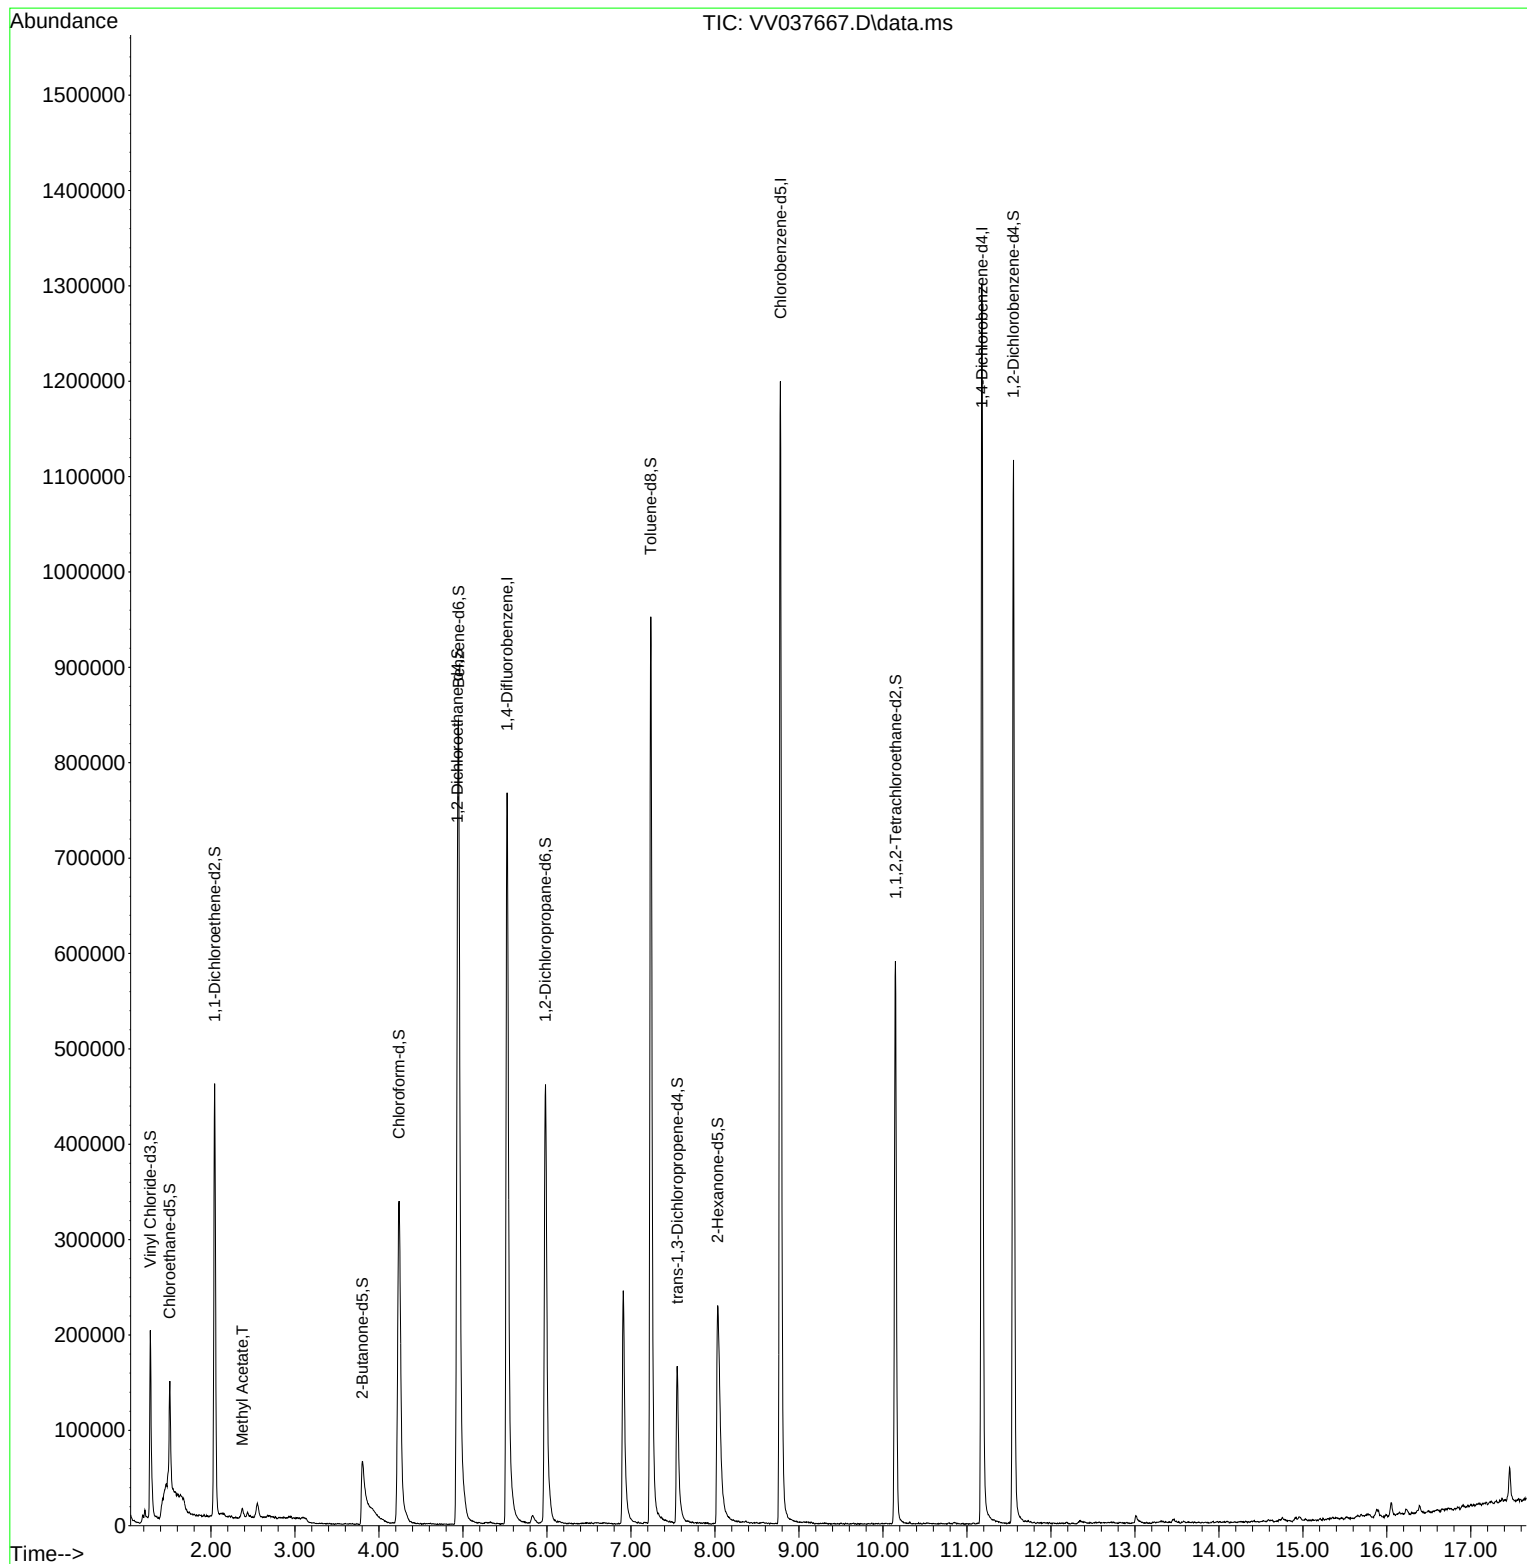

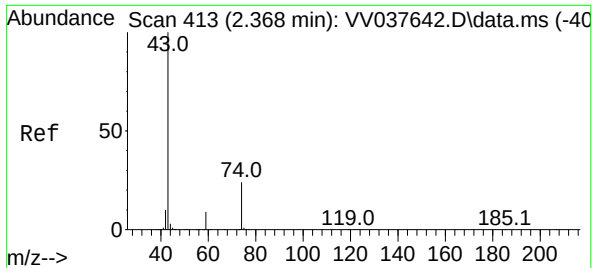

#15
Methyl Acetate
Concen: 3.091 ug/L
RT: 2.375 min Scan# 41
Delta R.T. 0.007 min
Lab File: VV037667.D
Acq: 30 Sep 2024 19:34

Instrument :
MSVOA_V
ClientSampleId :

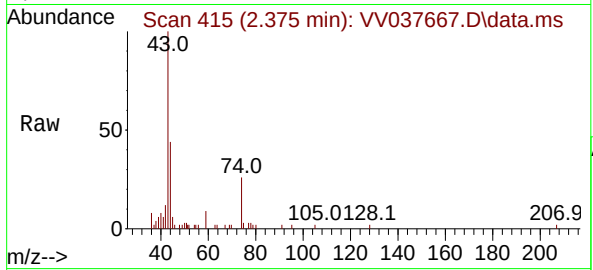

Tgt Ion: 43 Resp: 11754
Ion Ratio Lower Upper
43 100
74 22.5 19.4 29.0

