

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037652.D
 Acq On : 30 Sep 2024 14:10
 Operator : SY/MD
 Sample : VIBLK393
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	50	rBV	7659	13260	0.52%	0.072%
2	1.278	67	74	92	rBV	333638	363418	14.19%	1.960%
3	1.532	145	153	168	rVB	290278	343446	13.41%	1.852%
4	2.060	307	317	337	rBV	583624	837916	32.72%	4.519%
5	3.372	722	725	726	rBV	780	435	0.02%	0.002%
6	3.384	726	729	736	rVB5	830	866	0.03%	0.005%
7	3.468	752	755	757	rVV3	722	476	0.02%	0.003%
8	3.796	848	857	896	rBV2	111117	359315	14.03%	1.938%
9	4.143	963	965	969	rVB4	1119	632	0.02%	0.003%
10	4.243	979	996	1027	rBV	414300	1052928	41.12%	5.679%
11	4.481	1066	1070	1073	rVB5	872	603	0.02%	0.003%
12	4.516	1077	1081	1083	rBV4	889	682	0.03%	0.004%
13	4.558	1090	1094	1095	rBV4	1391	1028	0.04%	0.006%
14	4.622	1112	1114	1118	rVB4	1016	671	0.03%	0.004%
15	4.642	1118	1120	1123	rBV4	843	627	0.02%	0.003%
16	4.661	1123	1126	1128	rVV2	878	512	0.02%	0.003%
17	4.690	1131	1135	1138	rVB3	754	544	0.02%	0.003%
18	4.712	1138	1142	1144	rBV3	1179	760	0.03%	0.004%
19	4.876	1190	1193	1199	rVB6	1084	1134	0.04%	0.006%
20	4.950	1199	1216	1247	rBV2	1010045	2560809	100.00%	13.812%
21	5.162	1280	1282	1288	rBV6	1081	978	0.04%	0.005%
22	5.201	1292	1294	1300	rVB5	841	722	0.03%	0.004%
23	5.227	1300	1302	1307	rVB4	1080	865	0.03%	0.005%
24	5.449	1367	1371	1375	rBV4	762	687	0.03%	0.004%
25	5.529	1385	1396	1427	rBV	690194	1431754	55.91%	7.722%
26	5.834	1483	1491	1503	rBV10	6864	14730	0.58%	0.079%
27	5.928	1516	1520	1521	rBV2	893	557	0.02%	0.003%
28	5.982	1524	1537	1569	rBV	568277	1212562	47.35%	6.540%
29	6.908	1815	1825	1855	rBV	315167	598021	23.35%	3.226%
30	7.240	1917	1928	1960	rBV	1111170	1969598	76.91%	10.623%
31	7.548	2015	2024	2058	rBV2	208967	389859	15.22%	2.103%
32	7.905	2129	2135	2145	rVB8	4212	6117	0.24%	0.033%
33	8.024	2163	2172	2211	rBV	361420	739975	28.90%	3.991%
34	8.352	2269	2274	2275	rBV4	1984	1679	0.07%	0.009%
35	8.481	2311	2314	2316	rBV3	1062	484	0.02%	0.003%
36	8.619	2354	2357	2359	rBV3	738	432	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037652.D
 Acq On : 30 Sep 2024 14:10
 Operator : SY/MD
 Sample : VIBLK393
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.780	2395	2407	2435	rBV	1070990	1784773	69.70%	9.626%
38	9.082	2497	2501	2509	rBV9	2416	3396	0.13%	0.018%
39	9.301	2567	2569	2571	rBV2	896	502	0.02%	0.003%
40	9.381	2591	2594	2602	rVB7	1125	1380	0.05%	0.007%
41	9.490	2619	2628	2632	rBV7	3616	5924	0.23%	0.032%
42	9.577	2653	2655	2663	rVB6	1075	927	0.04%	0.005%
43	9.876	2737	2748	2756	rBV5	4841	8491	0.33%	0.046%
44	9.989	2781	2783	2786	rBV3	952	587	0.02%	0.003%
45	10.043	2797	2800	2803	rBV3	608	444	0.02%	0.002%
46	10.088	2811	2814	2818	rBV6	800	499	0.02%	0.003%
47	10.146	2818	2832	2851	rBV	664352	1060718	41.42%	5.721%
48	10.355	2895	2897	2901	rVB4	574	427	0.02%	0.002%
49	10.391	2905	2908	2909	rBV4	770	427	0.02%	0.002%
50	10.445	2921	2925	2928	rBV3	1267	980	0.04%	0.005%
51	10.481	2928	2936	2942	rBV2	5273	7838	0.31%	0.042%
52	10.702	3002	3005	3009	rVB4	1011	615	0.02%	0.003%
53	10.728	3009	3013	3016	rBV5	971	890	0.03%	0.005%
54	10.786	3027	3031	3033	rBV4	949	632	0.02%	0.003%
55	10.860	3045	3054	3066	rVV7	5630	10846	0.42%	0.058%
56	10.931	3073	3076	3079	rBV5	766	536	0.02%	0.003%
57	11.024	3103	3105	3110	rVB2	1016	865	0.03%	0.005%
58	11.050	3110	3113	3115	rBV3	883	672	0.03%	0.004%
59	11.088	3121	3125	3128	rBV4	982	818	0.03%	0.004%
60	11.127	3128	3137	3143	rBV3	10807	17619	0.69%	0.095%
61	11.178	3143	3153	3189	rVB	1040530	1663299	64.95%	8.971%
62	11.390	3217	3219	3224	rBV3	924	788	0.03%	0.004%
63	11.554	3256	3270	3302	rBV	1103845	1779826	69.50%	9.600%
64	11.821	3350	3353	3355	rBV4	821	596	0.02%	0.003%
65	11.902	3376	3378	3381	rVB4	1064	609	0.02%	0.003%
66	11.918	3381	3383	3388	rVB3	741	482	0.02%	0.003%
67	12.088	3431	3436	3443	rBV5	793	997	0.04%	0.005%
68	12.120	3443	3446	3449	rBV3	598	466	0.02%	0.003%
69	12.185	3461	3466	3468	rBV5	1021	975	0.04%	0.005%
70	12.223	3475	3478	3481	rBV3	715	486	0.02%	0.003%
71	12.313	3503	3506	3509	rVB4	917	563	0.02%	0.003%
72	12.368	3512	3523	3524	rBV6	2811	2887	0.11%	0.016%
73	12.448	3546	3548	3553	rVB5	1182	658	0.03%	0.004%
74	12.493	3558	3562	3564	rBV4	805	598	0.02%	0.003%
75	12.583	3581	3590	3602	rBV5	15270	27580	1.08%	0.149%
76	12.722	3630	3633	3636	rBV4	1030	588	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037652.D
 Acq On : 30 Sep 2024 14:10
 Operator : SY/MD
 Sample : VIBLK393
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK393

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.744	3636	3640	3643	rBV4	1019	966	0.04%	0.005%
78	12.905	3686	3690	3691	rBV2	938	562	0.02%	0.003%
79	12.988	3714	3716	3719	rVB3	1452	686	0.03%	0.004%
80	13.005	3719	3721	3723	rBV3	721	482	0.02%	0.003%
81	13.066	3734	3740	3742	rBV5	1008	919	0.04%	0.005%
82	13.124	3755	3758	3763	rVB5	830	573	0.02%	0.003%
83	13.201	3773	3782	3800	rBV2	25280	46390	1.81%	0.250%
84	13.439	3847	3856	3871	rBV	59829	111012	4.34%	0.599%
85	13.677	3920	3930	3945	rBV2	38829	65700	2.57%	0.354%
86	13.850	3978	3984	3986	rBV4	1456	1547	0.06%	0.008%
87	13.892	3994	3997	4001	rBV2	1141	1014	0.04%	0.005%
88	13.918	4001	4005	4007	rBV4	781	651	0.03%	0.004%
89	13.953	4013	4016	4018	rBV4	1049	774	0.03%	0.004%
90	14.027	4037	4039	4041	rBV2	742	455	0.02%	0.002%
91	14.040	4041	4043	4047	rVB5	967	573	0.02%	0.003%
92	14.117	4063	4067	4071	rBV5	1129	957	0.04%	0.005%
93	14.175	4082	4085	4088	rBV3	1365	673	0.03%	0.004%
94	14.214	4094	4097	4101	rBV4	947	808	0.03%	0.004%
95	14.416	4157	4160	4162	rBV4	1082	827	0.03%	0.004%
96	14.477	4175	4179	4180	rBV2	781	549	0.02%	0.003%
97	14.963	4327	4330	4333	rBV4	965	708	0.03%	0.004%
98	15.001	4340	4342	4344	rBV4	948	568	0.02%	0.003%
99	15.146	4385	4387	4392	rVB4	1274	859	0.03%	0.005%
100	15.419	4470	4472	4475	rBV4	1285	802	0.03%	0.004%




Sum of corrected areas: 18540341

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037652.D
Acq On : 30 Sep 2024 14:10
Operator : SY/MD
Sample : VIBLK393
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK393

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

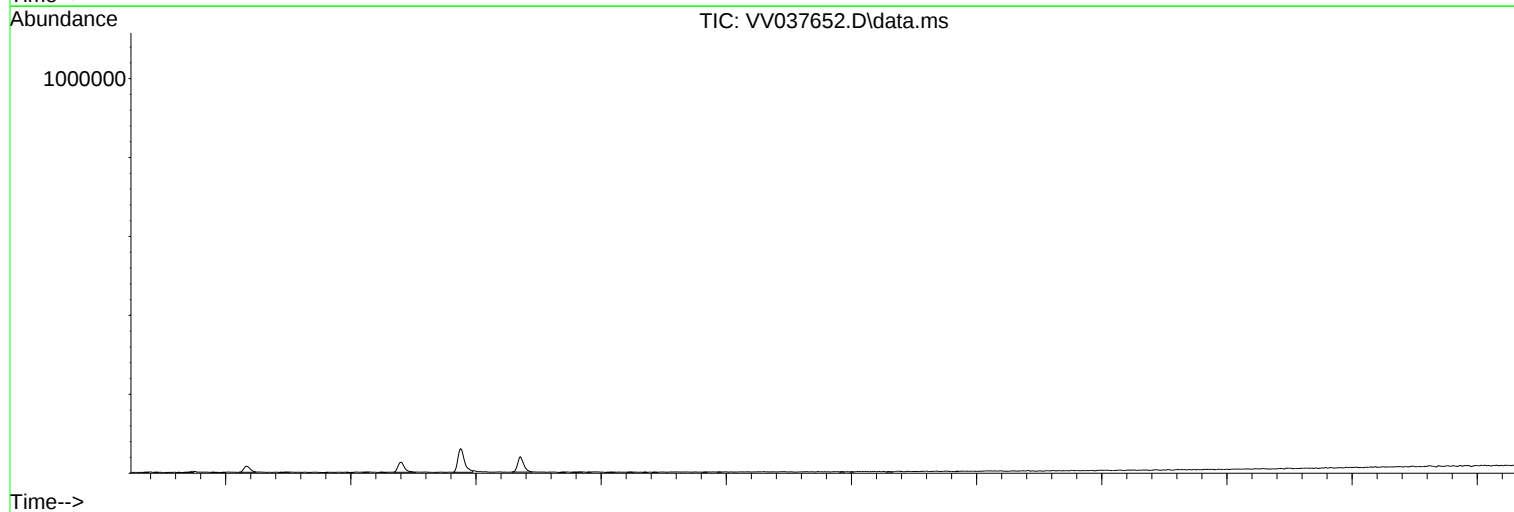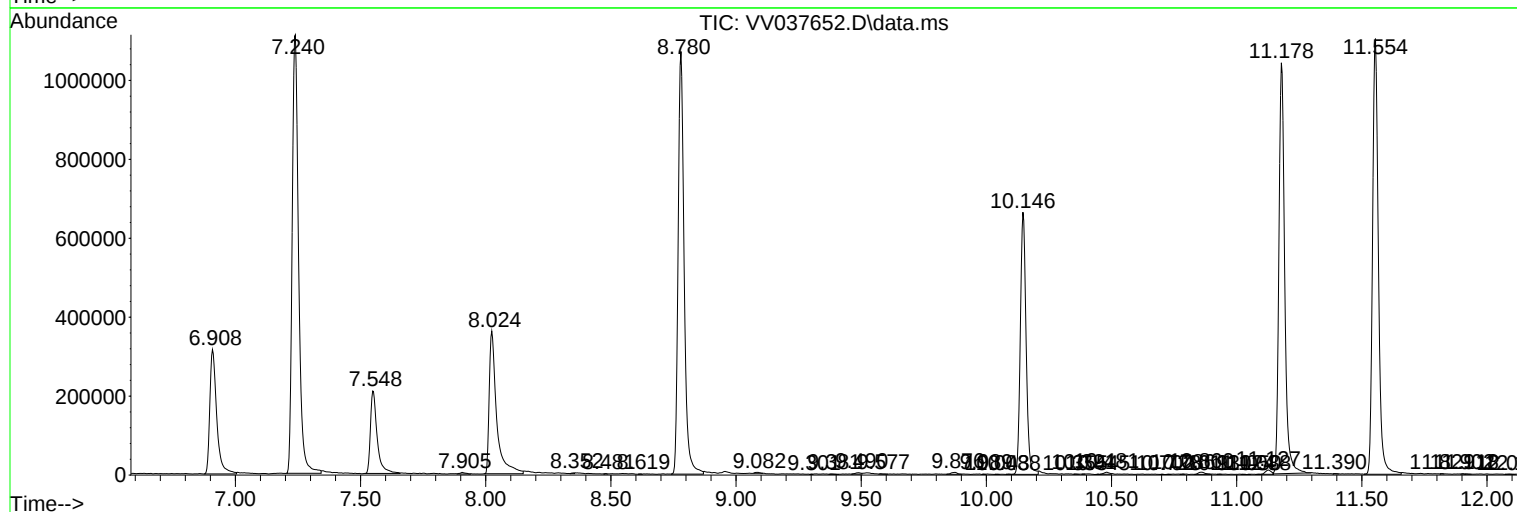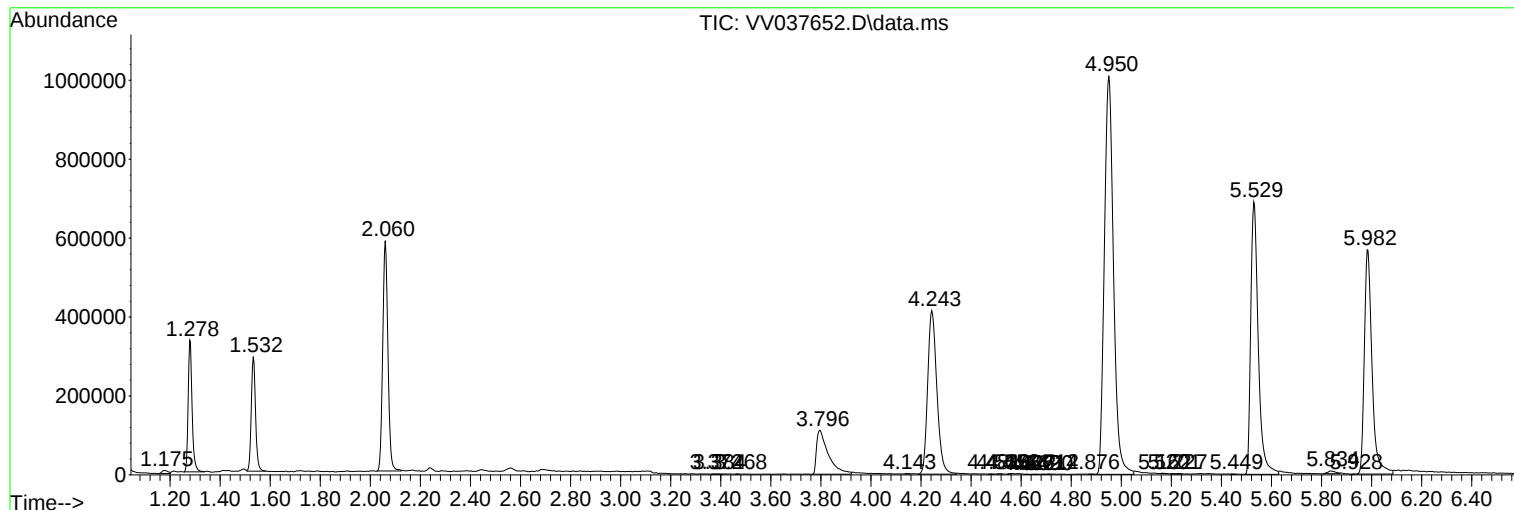

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037652.D
Acq On : 30 Sep 2024 14:10
Operator : SY/MD
Sample : VIBLK393
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK393

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037652.D
Acq On : 30 Sep 2024 14:10
Operator : SY/MD
Sample : VIBLK393
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK393

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
