

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037670.D
 Acq On : 30 Sep 2024 21:00
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	400030	426303	15.59%	2.171%
2	1.532	146	153	167	rVB	323504	375139	13.72%	1.910%
3	2.060	308	317	335	rVB	679970	980586	35.85%	4.994%
4	3.545	777	779	783	rVB3	756	423	0.02%	0.002%
5	3.564	783	785	789	rBV3	770	518	0.02%	0.003%
6	3.677	819	820	821	rBV	220	52	0.00%	0.000%
7	3.690	821	824	826	rVV	462	235	0.01%	0.001%
8	3.735	836	838	839	rBV2	476	191	0.01%	0.001%
9	3.757	843	845	846	rBV3	385	157	0.01%	0.001%
10	3.793	848	856	896	rBV2	111316	336050	12.29%	1.711%
11	4.243	981	996	1026	rBV	437023	1098907	40.18%	5.596%
12	4.616	1110	1112	1115	rBV2	503	255	0.01%	0.001%
13	4.642	1118	1120	1123	rBV2	343	168	0.01%	0.001%
14	4.670	1126	1129	1133	rVB3	472	345	0.01%	0.002%
15	4.706	1138	1140	1142	rBV	494	303	0.01%	0.002%
16	4.777	1160	1162	1163	rBV	214	55	0.00%	0.000%
17	4.789	1164	1166	1168	rBV2	659	271	0.01%	0.001%
18	4.860	1186	1188	1189	rBV	310	93	0.00%	0.000%
19	4.870	1189	1191	1195	rBV5	805	638	0.02%	0.003%
20	4.950	1200	1216	1246	rBV2	1084598	2734927	100.00%	13.928%
21	5.378	1346	1349	1350	rBV3	503	254	0.01%	0.001%
22	5.439	1366	1368	1373	rVB5	1133	661	0.02%	0.003%
23	5.529	1384	1396	1431	rBV	767955	1593245	58.26%	8.114%
24	5.986	1525	1538	1580	rBV	589736	1226170	44.83%	6.244%
25	6.320	1639	1642	1643	rBV3	699	433	0.02%	0.002%
26	6.358	1650	1654	1657	rVB4	878	719	0.03%	0.004%
27	6.378	1657	1660	1663	rBV2	582	382	0.01%	0.002%
28	6.404	1664	1668	1670	rBV2	643	453	0.02%	0.002%
29	6.516	1701	1703	1706	rBV3	549	256	0.01%	0.001%
30	6.551	1712	1714	1715	rVB	333	106	0.00%	0.001%
31	6.561	1715	1717	1720	rVB3	534	238	0.01%	0.001%
32	6.574	1720	1721	1723	rBV2	346	96	0.00%	0.000%
33	6.587	1723	1725	1727	rBV	553	235	0.01%	0.001%
34	6.600	1727	1729	1732	rBV2	781	494	0.02%	0.003%
35	6.648	1742	1744	1749	rVB4	638	427	0.02%	0.002%
36	6.674	1749	1752	1754	rBV2	756	437	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037670.D
 Acq On : 30 Sep 2024 21:00
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.690	1754	1757	1760	rVB2	770	493	0.02%	0.003%
38	6.712	1760	1764	1768	rBV3	941	1023	0.04%	0.005%
39	6.773	1778	1783	1785	rBV4	485	445	0.02%	0.002%
40	6.786	1785	1787	1791	rVB4	654	273	0.01%	0.001%
41	6.802	1791	1792	1795	rVB	248	130	0.00%	0.001%
42	6.822	1795	1798	1800	rBV3	550	269	0.01%	0.001%
43	6.908	1813	1825	1855	rBV	309719	594293	21.73%	3.026%
44	7.236	1916	1927	1953	rBV	1260393	2219981	81.17%	11.305%
45	7.548	2016	2024	2051	rBV	204981	377220	13.79%	1.921%
46	7.902	2131	2134	2136	rBV3	2059	1340	0.05%	0.007%
47	7.973	2153	2156	2162	rBV5	1028	735	0.03%	0.004%
48	8.024	2163	2172	2214	rBV	335915	722960	26.43%	3.682%
49	8.657	2367	2369	2371	rBV3	512	191	0.01%	0.001%
50	8.699	2380	2382	2385	rBV3	737	525	0.02%	0.003%
51	8.780	2396	2407	2440	rBV	1188491	1970992	72.07%	10.037%
52	9.358	2585	2587	2589	rBV2	499	243	0.01%	0.001%
53	9.410	2602	2603	2607	rBV3	529	347	0.01%	0.002%
54	9.448	2614	2615	2616	rVB3	385	74	0.00%	0.000%
55	9.587	2656	2658	2661	rBV4	632	423	0.02%	0.002%
56	9.635	2670	2673	2676	rBV3	524	376	0.01%	0.002%
57	9.834	2733	2735	2738	rVB	509	265	0.01%	0.001%
58	9.866	2741	2745	2746	rBV2	913	645	0.02%	0.003%
59	9.944	2768	2769	2774	rVB3	462	175	0.01%	0.001%
60	10.005	2786	2788	2789	rBV3	132	47	0.00%	0.000%
61	10.021	2789	2793	2795	rBV4	477	389	0.01%	0.002%
62	10.056	2800	2804	2805	rBV3	505	319	0.01%	0.002%
63	10.146	2818	2832	2858	rBV	660700	1042600	38.12%	5.309%
64	10.407	2911	2913	2916	rBV3	813	480	0.02%	0.002%
65	10.426	2916	2919	2920	rBV2	588	351	0.01%	0.002%
66	10.548	2954	2957	2961	rBV5	918	677	0.02%	0.003%
67	10.567	2961	2963	2964	rBV2	595	323	0.01%	0.002%
68	10.616	2975	2978	2979	rBV	555	278	0.01%	0.001%
69	10.664	2990	2993	2996	rVB4	746	489	0.02%	0.002%
70	10.690	2996	3001	3005	rBV3	402	427	0.02%	0.002%
71	10.709	3005	3007	3009	rBV	418	197	0.01%	0.001%
72	10.735	3012	3015	3017	rBV4	882	508	0.02%	0.003%
73	10.786	3027	3031	3036	rVB5	1554	1570	0.06%	0.008%
74	10.812	3036	3039	3042	rBV4	682	583	0.02%	0.003%
75	10.834	3045	3046	3048	rBV2	537	260	0.01%	0.001%
76	10.915	3069	3071	3076	rBV4	485	473	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037670.D
 Acq On : 30 Sep 2024 21:00
 Operator : SY/MD
 Sample : VV0930WBL02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK223

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.947	3076	3081	3083	rBV3	506	530	0.02%	0.003%
78	10.989	3091	3094	3095	rBV	529	284	0.01%	0.001%
79	11.017	3100	3103	3105	rBV2	785	419	0.02%	0.002%
80	11.050	3111	3113	3117	rVB4	649	356	0.01%	0.002%
81	11.127	3133	3137	3142	rBV5	2906	3865	0.14%	0.020%
82	11.178	3142	3153	3179	rVV	1181480	1887677	69.02%	9.613%
83	11.429	3229	3231	3233	rBV2	964	573	0.02%	0.003%
84	11.554	3258	3270	3304	rBV	1212194	1970548	72.05%	10.035%
85	11.940	3388	3390	3395	rVB5	1321	1141	0.04%	0.006%
86	11.979	3396	3402	3408	rVB9	1454	1757	0.06%	0.009%
87	12.104	3439	3441	3444	rBB3	504	163	0.01%	0.001%
88	12.124	3445	3447	3450	rVB2	805	304	0.01%	0.002%
89	12.140	3450	3452	3455	rBV2	662	426	0.02%	0.002%
90	12.188	3464	3467	3474	rBV7	1218	1122	0.04%	0.006%
91	12.316	3504	3507	3512	rBV4	648	686	0.03%	0.003%
92	12.339	3512	3514	3516	rVV3	519	277	0.01%	0.001%
93	12.358	3518	3520	3523	rBV3	470	300	0.01%	0.002%
94	12.516	3567	3569	3578	rVB8	1137	793	0.03%	0.004%
95	12.590	3586	3592	3594	rBV5	3078	3611	0.13%	0.018%
96	13.014	3720	3724	3727	rBV3	1020	927	0.03%	0.005%
97	13.201	3779	3782	3783	rBV3	3328	2027	0.07%	0.010%
98	13.262	3798	3801	3802	rBV2	1093	653	0.02%	0.003%
99	13.448	3851	3859	3877	rBV2	12093	23852	0.87%	0.121%
100	13.683	3925	3932	3941	rBV7	6821	10661	0.39%	0.054%

Sum of corrected areas: 19636563




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037670.D
Acq On : 30 Sep 2024 21:00
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

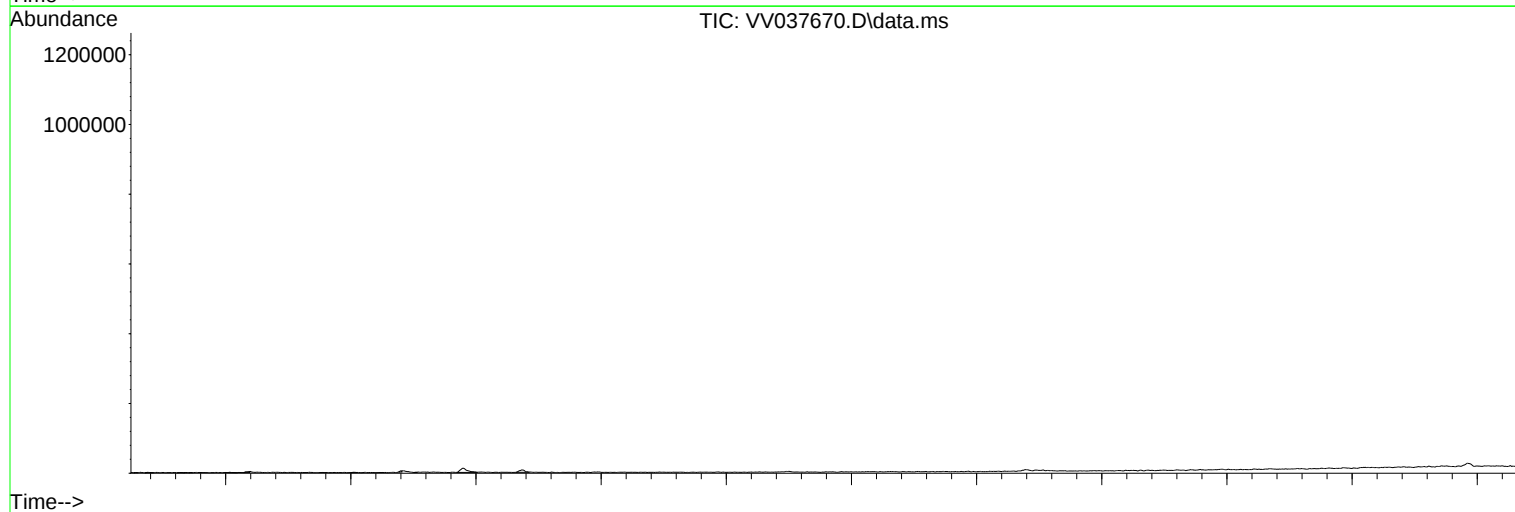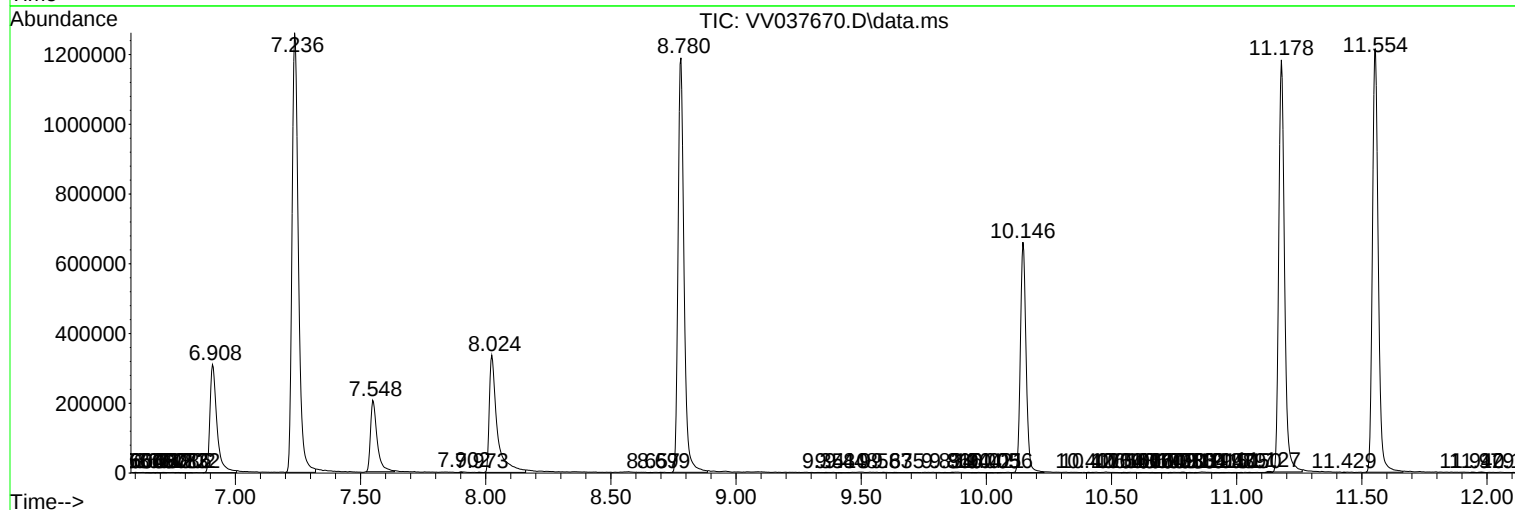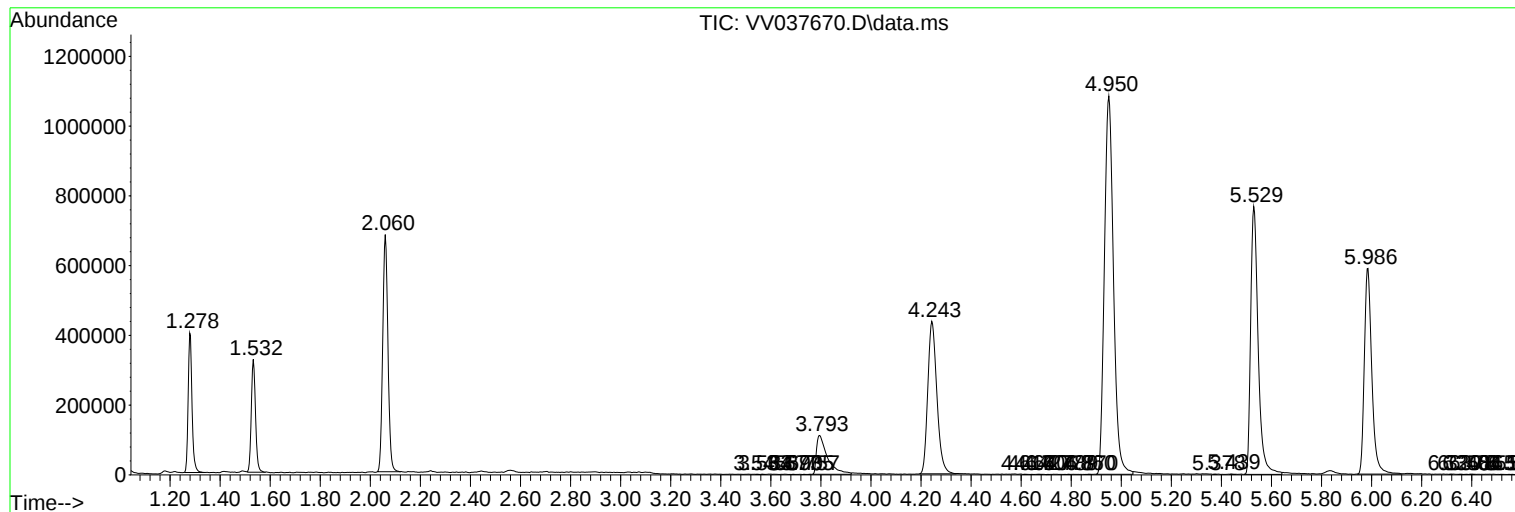

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037670.D
Acq On : 30 Sep 2024 21:00
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037670.D
Acq On : 30 Sep 2024 21:00
Operator : SY/MD
Sample : VV0930WBL02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK223

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc