

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037671.D
 Acq On : 30 Sep 2024 21:21
 Operator : SY/MD
 Sample : P4185-16DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY064DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	37	44	51	rBV2	7906	14238	0.54%	0.073%
2	1.278	67	74	90	rVB	277607	298352	11.33%	1.521%
3	1.423	111	119	126	rBV6	11880	19963	0.76%	0.102%
4	1.529	145	152	168	rVB	263933	318804	12.11%	1.625%
5	2.060	306	317	332	rBV	543538	797131	30.27%	4.064%
6	3.265	689	692	696	rVB4	701	538	0.02%	0.003%
7	3.288	696	699	701	rBV2	761	472	0.02%	0.002%
8	3.745	837	841	844	rBV2	804	730	0.03%	0.004%
9	3.793	847	856	895	rBV2	129172	378682	14.38%	1.931%
10	4.243	980	996	1031	rBV	434157	1111008	42.19%	5.665%
11	4.561	1092	1095	1096	rBV2	818	505	0.02%	0.003%
12	4.590	1102	1104	1107	rVB4	900	583	0.02%	0.003%
13	4.609	1107	1110	1113	rBV2	927	694	0.03%	0.004%
14	4.696	1134	1137	1141	rVV4	1019	726	0.03%	0.004%
15	4.722	1143	1145	1149	rVV5	630	546	0.02%	0.003%
16	4.748	1149	1153	1155	rVB3	852	548	0.02%	0.003%
17	4.950	1200	1216	1248	rBV2	1030157	2633635	100.00%	13.428%
18	5.259	1310	1312	1316	rBV3	760	710	0.03%	0.004%
19	5.304	1323	1326	1330	rBV6	785	807	0.03%	0.004%
20	5.529	1384	1396	1429	rBV	811347	1664495	63.20%	8.487%
21	5.767	1468	1470	1473	rBV3	886	626	0.02%	0.003%
22	5.783	1473	1475	1479	rVB5	1273	582	0.02%	0.003%
23	5.828	1479	1489	1507	rBV9	10741	27616	1.05%	0.141%
24	5.982	1524	1537	1580	rVV	589764	1240828	47.11%	6.326%
25	6.262	1622	1624	1629	rBV2	1069	827	0.03%	0.004%
26	6.365	1654	1656	1660	rVB4	1159	776	0.03%	0.004%
27	6.387	1660	1663	1667	rBV3	851	693	0.03%	0.004%
28	6.458	1682	1685	1691	rVB6	1007	943	0.04%	0.005%
29	6.490	1692	1695	1699	rVB5	808	554	0.02%	0.003%
30	6.529	1704	1707	1710	rVB4	742	483	0.02%	0.002%
31	6.687	1754	1756	1762	rVB4	1253	745	0.03%	0.004%
32	6.777	1780	1784	1789	rVB7	690	646	0.02%	0.003%
33	6.815	1792	1796	1801	rVB5	636	592	0.02%	0.003%
34	6.908	1815	1825	1851	rBV	314243	596072	22.63%	3.039%
35	7.236	1916	1927	1965	rBV	1173267	2079311	78.95%	10.601%
36	7.548	2015	2024	2053	rBV	206261	388425	14.75%	1.980%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037671.D
 Acq On : 30 Sep 2024 21:21
 Operator : SY/MD
 Sample : P4185-16DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY064DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.776	2091	2095	2097	rBV4	1039	702	0.03%	0.004%
38	7.908	2128	2136	2144	rBV9	5733	10685	0.41%	0.054%
39	8.024	2163	2172	2215	rBV	362334	765291	29.06%	3.902%
40	8.445	2300	2303	2311	rVB7	1308	1574	0.06%	0.008%
41	8.484	2312	2315	2320	rBV5	1155	1097	0.04%	0.006%
42	8.535	2325	2331	2332	rBV4	1056	1041	0.04%	0.005%
43	8.690	2375	2379	2382	rBV4	1106	688	0.03%	0.004%
44	8.706	2382	2384	2388	rVB4	737	492	0.02%	0.003%
45	8.780	2396	2407	2441	rBV	1237757	2062399	78.31%	10.515%
46	9.056	2490	2493	2494	rBV3	1218	591	0.02%	0.003%
47	9.149	2519	2522	2526	rBV5	471	473	0.02%	0.002%
48	9.201	2536	2538	2544	rVV4	1100	1092	0.04%	0.006%
49	9.281	2559	2563	2568	rVB4	894	764	0.03%	0.004%
50	9.397	2595	2599	2601	rBV2	936	479	0.02%	0.002%
51	9.445	2612	2614	2618	rBV4	982	835	0.03%	0.004%
52	9.526	2635	2639	2642	rVB4	1089	801	0.03%	0.004%
53	9.542	2642	2644	2646	rBV4	1039	616	0.02%	0.003%
54	9.580	2654	2656	2662	rVB5	735	502	0.02%	0.003%
55	9.622	2665	2669	2671	rBV4	822	633	0.02%	0.003%
56	9.857	2739	2742	2746	rBV4	990	744	0.03%	0.004%
57	10.079	2807	2811	2815	rBV4	690	787	0.03%	0.004%
58	10.146	2820	2832	2870	rVV	710603	1136590	43.16%	5.795%
59	10.394	2906	2909	2916	rVB6	1240	1399	0.05%	0.007%
60	10.423	2916	2918	2921	rBV2	764	616	0.02%	0.003%
61	10.481	2933	2936	2940	rVV6	1242	1264	0.05%	0.006%
62	10.510	2943	2945	2950	rVB4	837	580	0.02%	0.003%
63	10.702	3003	3005	3010	rVV2	784	678	0.03%	0.003%
64	10.834	3039	3046	3049	rBV5	929	996	0.04%	0.005%
65	10.866	3049	3056	3059	rBV6	1495	2152	0.08%	0.011%
66	10.937	3074	3078	3083	rBV5	780	862	0.03%	0.004%
67	11.046	3109	3112	3115	rBV3	753	663	0.03%	0.003%
68	11.066	3115	3118	3121	rBV4	545	471	0.02%	0.002%
69	11.178	3142	3153	3187	rBV	1237011	1958023	74.35%	9.983%
70	11.426	3228	3230	3235	rVB5	1104	737	0.03%	0.004%
71	11.554	3257	3270	3301	rBV	1266290	2033750	77.22%	10.369%
72	11.747	3327	3330	3334	rVB5	781	524	0.02%	0.003%
73	12.098	3436	3439	3444	rBV6	665	506	0.02%	0.003%
74	12.185	3462	3466	3470	rVB3	1259	791	0.03%	0.004%
75	12.249	3483	3486	3489	rBV3	1112	693	0.03%	0.004%
76	12.294	3499	3500	3503	rVV3	693	492	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037671.D
 Acq On : 30 Sep 2024 21:21
 Operator : SY/MD
 Sample : P4185-16DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY064DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.355	3515	3519	3523	rVB4	1046	918	0.03%	0.005%
78	12.378	3523	3526	3532	rBV3	1038	891	0.03%	0.005%
79	12.413	3534	3537	3541	rVB5	932	685	0.03%	0.003%
80	12.596	3587	3594	3602	rVV8	2696	3726	0.14%	0.019%
81	12.696	3621	3625	3628	rBV4	920	825	0.03%	0.004%
82	12.770	3645	3648	3651	rBV5	909	791	0.03%	0.004%
83	13.062	3736	3739	3745	rVB4	702	644	0.02%	0.003%
84	13.127	3755	3759	3763	rBV3	1277	1314	0.05%	0.007%
85	13.204	3778	3783	3785	rBV5	2777	2563	0.10%	0.013%
86	13.233	3790	3792	3798	rVB6	1862	1368	0.05%	0.007%
87	13.291	3805	3810	3812	rBV5	1022	1031	0.04%	0.005%
88	13.352	3825	3829	3830	rBV3	1131	683	0.03%	0.003%
89	13.406	3841	3846	3848	rBV6	1030	1003	0.04%	0.005%
90	13.458	3853	3862	3867	rBV3	3681	6316	0.24%	0.032%
91	13.683	3926	3932	3944	rVB3	3800	6383	0.24%	0.033%
92	13.763	3954	3957	3962	rBV3	948	736	0.03%	0.004%
93	13.792	3962	3966	3969	rBV3	1312	1167	0.04%	0.006%
94	13.895	3996	3998	4002	rBV3	694	481	0.02%	0.002%
95	13.963	4016	4019	4021	rBV4	936	536	0.02%	0.003%
96	14.037	4039	4042	4044	rBV2	919	472	0.02%	0.002%
97	14.098	4056	4061	4067	rBV7	1399	1764	0.07%	0.009%
98	14.451	4168	4171	4174	rBV4	871	558	0.02%	0.003%
99	15.098	4368	4372	4373	rBV4	1262	864	0.03%	0.004%
100	15.429	4473	4475	4477	rBV2	1500	706	0.03%	0.004%

Sum of corrected areas: 19613384




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037671.D
Acq On : 30 Sep 2024 21:21
Operator : SY/MD
Sample : P4185-16DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY064DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

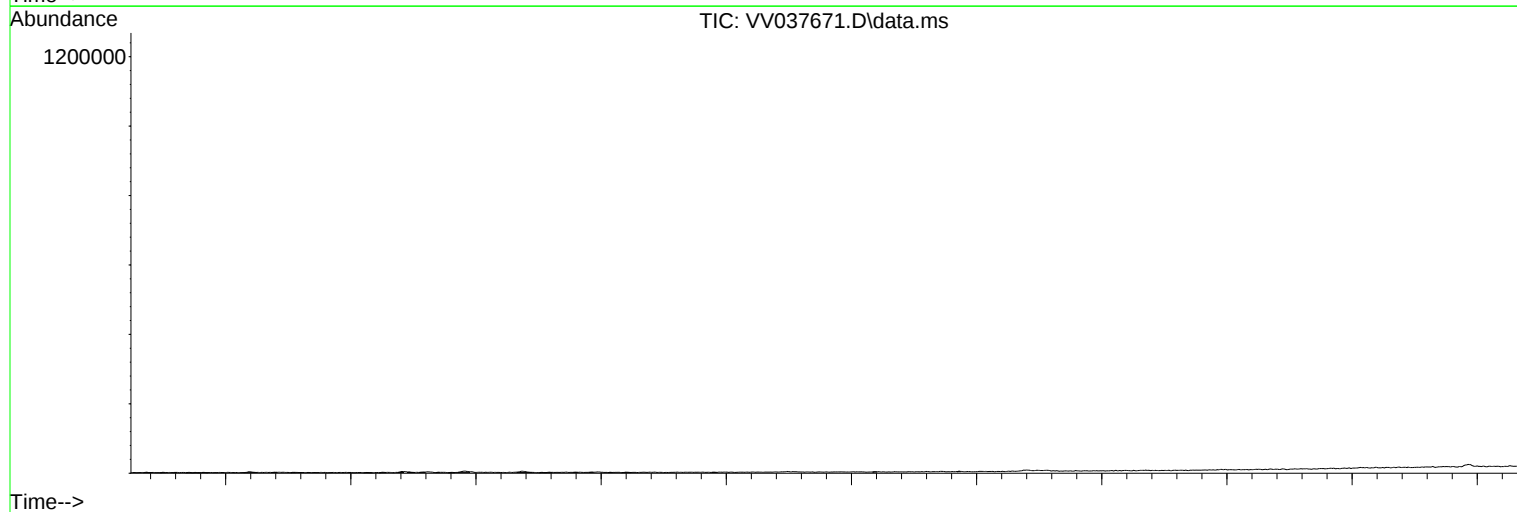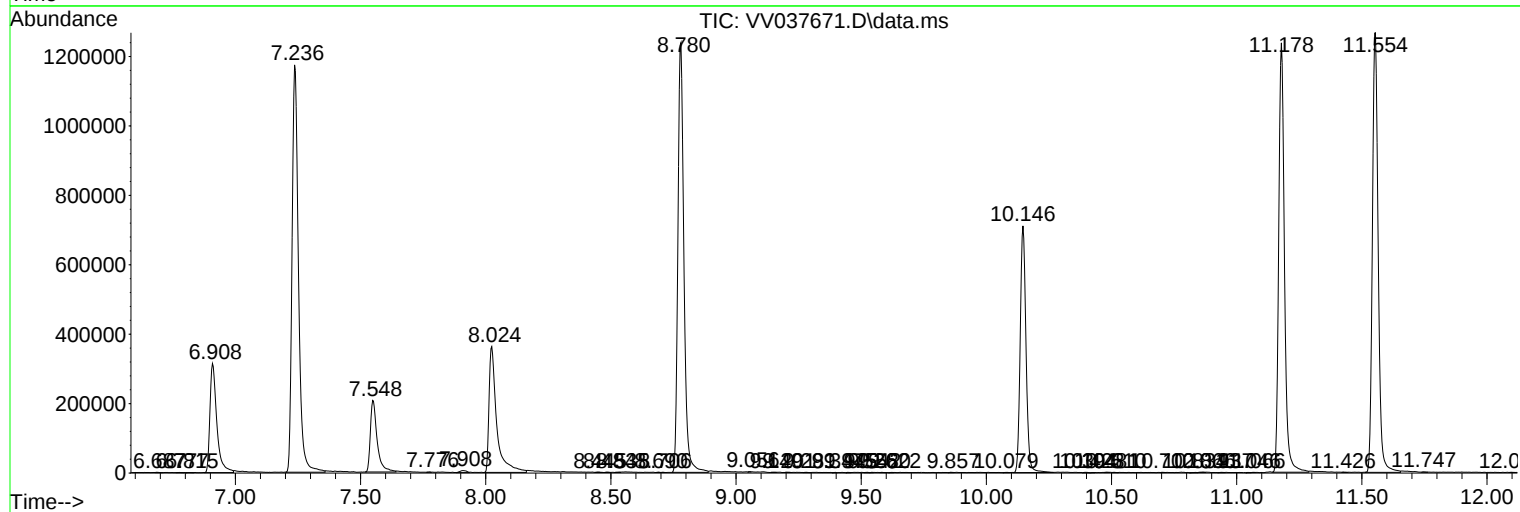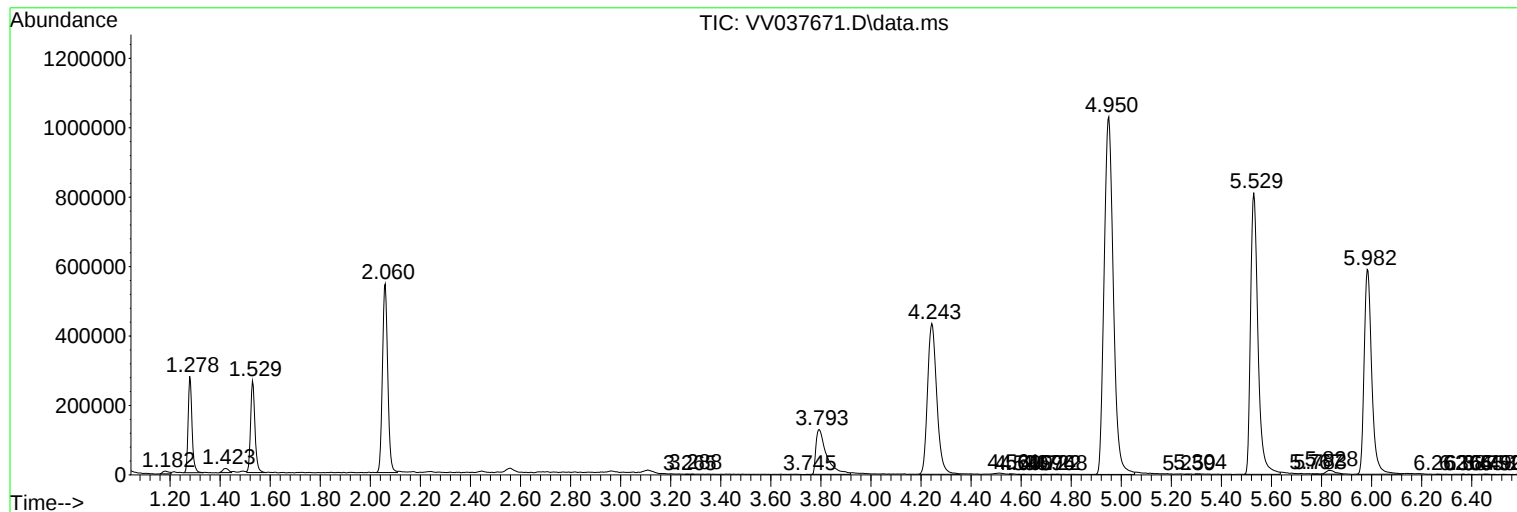

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037671.D
Acq On : 30 Sep 2024 21:21
Operator : SY/MD
Sample : P4185-16DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY064DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037671.D
Acq On : 30 Sep 2024 21:21
Operator : SY/MD
Sample : P4185-16DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY064DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
