

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037673.D
 Acq On : 30 Sep 2024 22:04
 Operator : SY/MD
 Sample : P4185-20DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037673.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB2	314342	350176	13.32%	1.722%
2	1.532	146	153	169	rVB	268949	347097	13.20%	1.707%
3	2.060	308	317	332	rBV	516643	747747	28.43%	3.677%
4	3.108	633	643	664	rVB	260726	534488	20.32%	2.628%
5	3.410	734	737	739	rBV2	980	595	0.02%	0.003%
6	3.500	761	765	769	rBV3	568	500	0.02%	0.002%
7	3.632	804	806	808	rBV2	605	211	0.01%	0.001%
8	3.696	823	826	828	rBV3	723	459	0.02%	0.002%
9	3.744	840	841	844	rBV	298	155	0.01%	0.001%
10	3.806	845	860	901	rBV2	516676	1435033	54.57%	7.057%
11	4.243	981	996	1022	rBV	437422	1099325	41.80%	5.406%
12	4.445	1057	1059	1064	rBV3	1016	889	0.03%	0.004%
13	4.690	1132	1135	1137	rBV3	920	623	0.02%	0.003%
14	4.719	1143	1144	1146	rBV2	520	216	0.01%	0.001%
15	4.757	1155	1156	1159	rVB2	892	311	0.01%	0.002%
16	4.777	1159	1162	1164	rBV2	637	442	0.02%	0.002%
17	4.812	1171	1173	1176	rBV2	284	163	0.01%	0.001%
18	4.847	1181	1184	1186	rBV2	543	376	0.01%	0.002%
19	4.950	1199	1216	1253	rBV2	1021958	2629810	100.00%	12.932%
20	5.265	1311	1314	1318	rBV4	1058	959	0.04%	0.005%
21	5.455	1370	1373	1374	rBV2	897	478	0.02%	0.002%
22	5.529	1385	1396	1435	rBV	718187	1480643	56.30%	7.281%
23	5.838	1480	1492	1514	rBV6	36531	89103	3.39%	0.438%
24	5.982	1525	1537	1567	rBV	601187	1244825	47.34%	6.121%
25	6.330	1643	1645	1647	rBV3	633	312	0.01%	0.002%
26	6.384	1660	1662	1666	rVB4	509	250	0.01%	0.001%
27	6.452	1682	1683	1684	rBV4	512	157	0.01%	0.001%
28	6.577	1720	1722	1726	rBV3	578	350	0.01%	0.002%
29	6.622	1733	1736	1740	rBV2	722	564	0.02%	0.003%
30	6.664	1746	1749	1751	rBV3	833	562	0.02%	0.003%
31	6.780	1783	1785	1789	rVB3	748	507	0.02%	0.002%
32	6.850	1806	1807	1813	rVB3	798	601	0.02%	0.003%
33	6.908	1813	1825	1864	rBV	307109	597727	22.73%	2.939%
34	7.240	1916	1928	1971	rBV	1099335	1990571	75.69%	9.789%
35	7.548	2016	2024	2054	rBV	210608	383528	14.58%	1.886%
36	7.908	2126	2136	2150	rVV5	16763	34286	1.30%	0.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037673.D
 Acq On : 30 Sep 2024 22:04
 Operator : SY/MD
 Sample : P4185-20DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.960	2150	2152	2158	rVB5	973	550	0.02%	0.003%
38	8.024	2163	2172	2223	rBV2	365010	790078	30.04%	3.885%
39	8.622	2356	2358	2359	rBV	713	309	0.01%	0.002%
40	8.712	2384	2386	2387	rBV2	593	221	0.01%	0.001%
41	8.780	2395	2407	2440	rBV	1086988	1813150	68.95%	8.916%
42	9.143	2516	2520	2521	rBV2	652	456	0.02%	0.002%
43	9.210	2537	2541	2543	rVB3	731	602	0.02%	0.003%
44	9.227	2543	2546	2551	rBV5	833	835	0.03%	0.004%
45	9.284	2560	2564	2565	rBV2	856	552	0.02%	0.003%
46	9.346	2579	2583	2585	rBV2	1001	709	0.03%	0.003%
47	9.358	2585	2587	2592	rVV2	674	544	0.02%	0.003%
48	9.458	2616	2618	2620	rBV3	548	192	0.01%	0.001%
49	9.628	2669	2671	2673	rBV2	456	231	0.01%	0.001%
50	9.651	2675	2678	2683	rVB5	1361	1325	0.05%	0.007%
51	9.677	2683	2686	2688	rBV2	646	329	0.01%	0.002%
52	9.699	2688	2693	2697	rBV6	937	1081	0.04%	0.005%
53	9.847	2736	2739	2743	rBV4	656	599	0.02%	0.003%
54	9.879	2743	2749	2752	rVV4	684	761	0.03%	0.004%
55	9.947	2769	2770	2772	rBV	484	210	0.01%	0.001%
56	9.963	2773	2775	2776	rVV2	503	133	0.01%	0.001%
57	10.018	2791	2792	2795	rVB2	352	129	0.00%	0.001%
58	10.037	2795	2798	2804	rBV3	763	860	0.03%	0.004%
59	10.066	2804	2807	2811	rBV2	588	398	0.02%	0.002%
60	10.088	2811	2814	2815	rBV	597	347	0.01%	0.002%
61	10.146	2820	2832	2857	rBV	716201	1147868	43.65%	5.645%
62	10.580	2964	2967	2969	rVB3	609	345	0.01%	0.002%
63	10.600	2969	2973	2978	rBV3	1106	1167	0.04%	0.006%
64	10.632	2981	2983	2985	rBV	751	392	0.01%	0.002%
65	10.648	2985	2988	2990	rBV	693	439	0.02%	0.002%
66	10.693	3000	3002	3004	rBV3	633	320	0.01%	0.002%
67	10.718	3008	3010	3013	rVB2	425	177	0.01%	0.001%
68	10.747	3016	3019	3021	rBV2	495	225	0.01%	0.001%
69	10.776	3024	3028	3029	rBV3	703	519	0.02%	0.003%
70	10.837	3044	3047	3053	rBV3	710	432	0.02%	0.002%
71	10.902	3064	3067	3068	rBV	382	275	0.01%	0.001%
72	11.069	3115	3119	3123	rBV5	933	881	0.03%	0.004%
73	11.108	3128	3131	3133	rBV2	664	379	0.01%	0.002%
74	11.133	3133	3139	3142	rBV7	1708	1810	0.07%	0.009%
75	11.178	3143	3153	3185	rBV	1056129	1661248	63.17%	8.169%
76	11.551	3258	3269	3300	rBV	1186960	1924643	73.19%	9.464%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037673.D
 Acq On : 30 Sep 2024 22:04
 Operator : SY/MD
 Sample : P4185-20DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY073DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.140	3450	3452	3454	rBV3	663	415	0.02%	0.002%
78	12.349	3513	3517	3520	rBV5	706	614	0.02%	0.003%
79	12.419	3536	3539	3543	rBV4	882	740	0.03%	0.004%
80	12.468	3551	3554	3556	rBV2	668	427	0.02%	0.002%
81	12.538	3574	3576	3580	rVB2	854	539	0.02%	0.003%
82	12.644	3604	3609	3610	rBV4	1214	993	0.04%	0.005%
83	12.718	3629	3632	3634	rBV3	851	628	0.02%	0.003%
84	12.950	3703	3704	3706	rBV2	642	327	0.01%	0.002%
85	13.101	3748	3751	3754	rBV2	906	719	0.03%	0.004%
86	13.419	3848	3850	3852	rBV	951	412	0.02%	0.002%

Sum of corrected areas: 20335574




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037673.D
Acq On : 30 Sep 2024 22:04
Operator : SY/MD
Sample : P4185-20DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

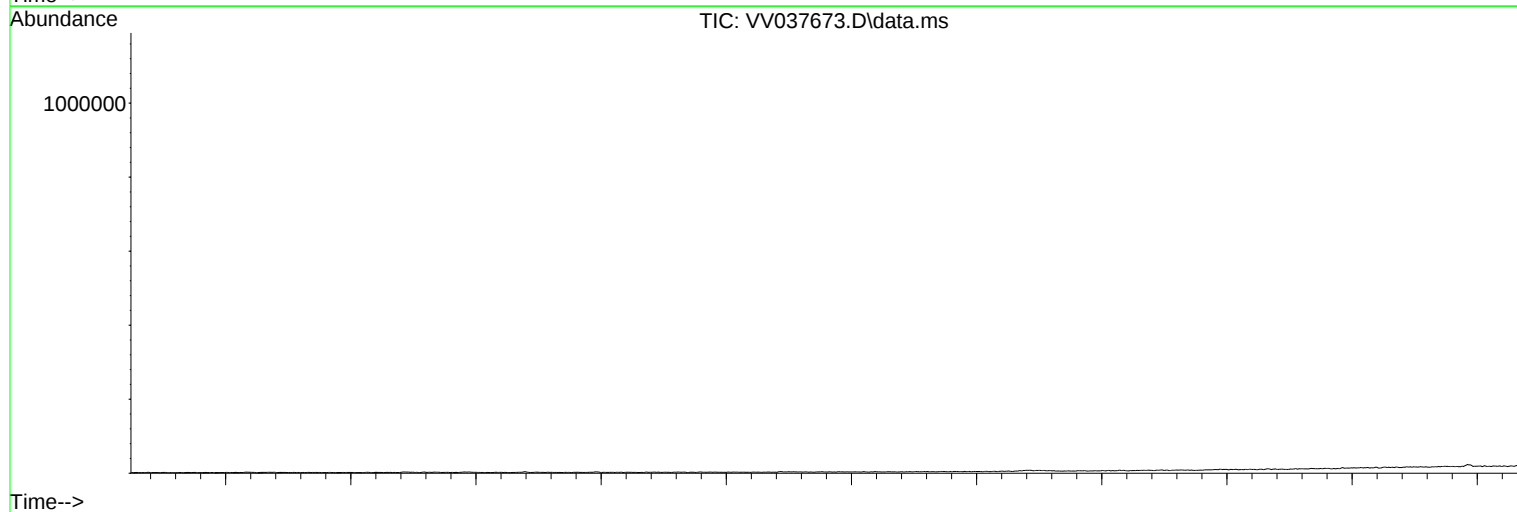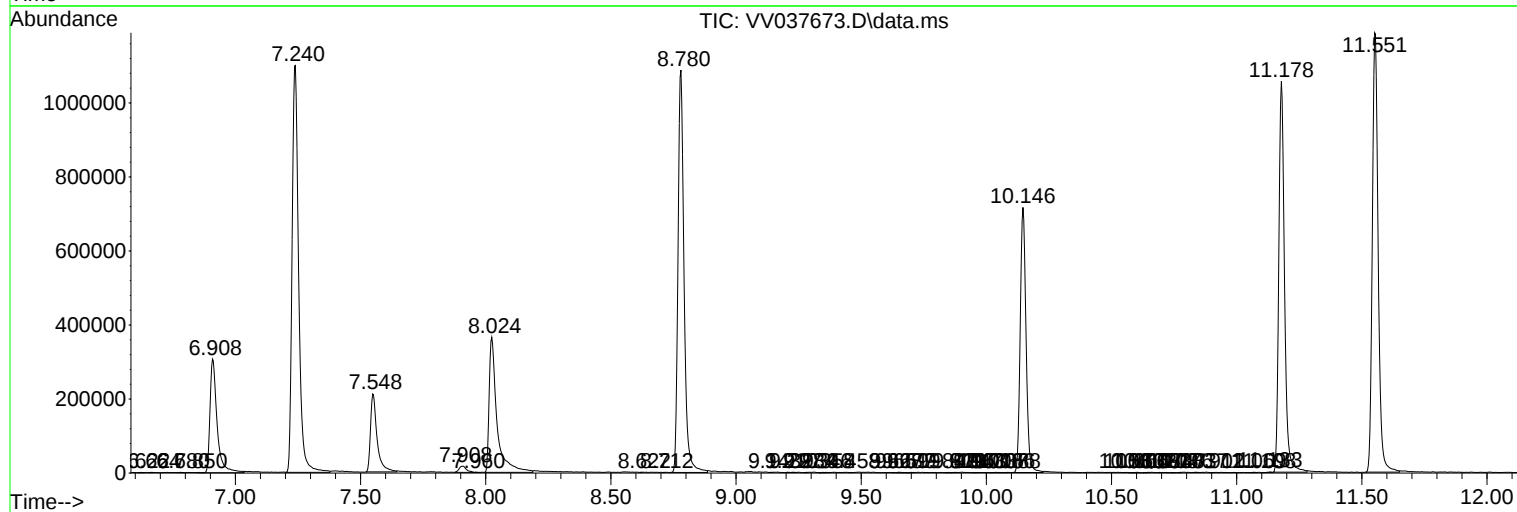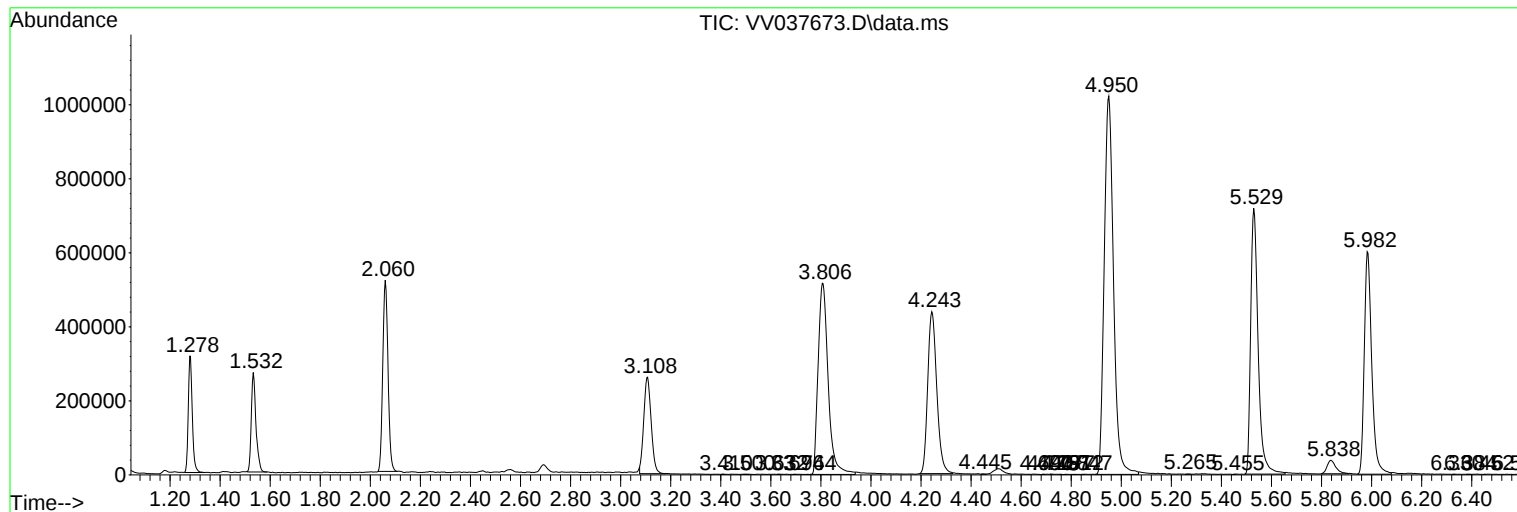

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037673.D
Acq On : 30 Sep 2024 22:04
Operator : SY/MD
Sample : P4185-20DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037673.D
Acq On : 30 Sep 2024 22:04
Operator : SY/MD
Sample : P4185-20DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY073DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------