

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037676.D
 Acq On : 30 Sep 2024 23:08
 Operator : SY/MD
 Sample : P4228-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037676.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	51	rBV2	8747	16512	0.63%	0.087%
2	1.282	67	75	89	rVB	278953	298467	11.34%	1.575%
3	1.532	145	153	168	rVB	268471	310778	11.81%	1.640%
4	2.060	307	317	331	rBV	541444	782211	29.73%	4.127%
5	3.278	693	696	699	rVB3	789	541	0.02%	0.003%
6	3.407	734	736	740	rVV4	937	660	0.03%	0.003%
7	3.484	756	760	762	rBV2	703	609	0.02%	0.003%
8	3.748	839	842	848	rBV5	615	500	0.02%	0.003%
9	3.793	848	856	895	rBV2	118130	350485	13.32%	1.849%
10	4.243	978	996	1028	rBV2	432573	1116860	42.45%	5.893%
11	4.375	1034	1037	1042	rVB5	1386	1216	0.05%	0.006%
12	4.404	1042	1046	1048	rBV4	1254	723	0.03%	0.004%
13	4.539	1084	1088	1092	rBV4	1182	774	0.03%	0.004%
14	4.712	1136	1142	1149	rVB7	1025	1207	0.05%	0.006%
15	4.748	1149	1153	1156	rVB4	850	653	0.02%	0.003%
16	4.812	1171	1173	1177	rVB3	819	474	0.02%	0.003%
17	4.838	1177	1181	1187	rVB4	1061	951	0.04%	0.005%
18	4.950	1200	1216	1250	rBV2	1028502	2631243	100.00%	13.884%
19	5.195	1290	1292	1296	rBV5	1064	569	0.02%	0.003%
20	5.330	1331	1334	1337	rVB3	1008	568	0.02%	0.003%
21	5.410	1353	1359	1361	rBV5	830	782	0.03%	0.004%
22	5.471	1373	1378	1382	rVB4	960	876	0.03%	0.005%
23	5.529	1382	1396	1432	rBV	737381	1532147	58.23%	8.084%
24	5.825	1477	1488	1490	rBV10	9479	11527	0.44%	0.061%
25	5.982	1525	1537	1570	rBV	589882	1225055	46.56%	6.464%
26	6.259	1619	1623	1626	rVB4	1198	771	0.03%	0.004%
27	6.320	1638	1642	1645	rBV4	963	694	0.03%	0.004%
28	6.449	1677	1682	1689	rVB8	1795	2174	0.08%	0.011%
29	6.555	1710	1715	1717	rBV4	999	811	0.03%	0.004%
30	6.577	1720	1722	1729	rVB3	748	551	0.02%	0.003%
31	6.783	1780	1786	1787	rBV3	625	642	0.02%	0.003%
32	6.908	1814	1825	1859	rBV	300855	585168	22.24%	3.088%
33	7.162	1901	1904	1906	rBV3	1003	582	0.02%	0.003%
34	7.236	1916	1927	1953	rBV	1158615	2048722	77.86%	10.810%
35	7.503	2007	2010	2013	rBV4	857	659	0.03%	0.003%
36	7.548	2016	2024	2048	rBV	206490	377876	14.36%	1.994%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037676.D
 Acq On : 30 Sep 2024 23:08
 Operator : SY/MD
 Sample : P4228-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.908	2124	2136	2148	rBV4	13136	25381	0.96%	0.134%
38	8.024	2161	2172	2213	rBV2	346177	758795	28.84%	4.004%
39	8.465	2306	2309	2313	rBV3	915	975	0.04%	0.005%
40	8.494	2313	2318	2320	rVV5	918	709	0.03%	0.004%
41	8.780	2396	2407	2432	rBV	1145560	1887249	71.72%	9.958%
42	9.101	2504	2507	2510	rBV3	601	487	0.02%	0.003%
43	9.137	2514	2518	2519	rBV3	708	572	0.02%	0.003%
44	9.198	2533	2537	2543	rBV5	803	879	0.03%	0.005%
45	9.230	2543	2547	2550	rBV6	942	753	0.03%	0.004%
46	9.378	2590	2593	2596	rBV3	760	621	0.02%	0.003%
47	9.445	2611	2614	2617	rBV3	546	473	0.02%	0.002%
48	9.494	2628	2629	2633	rVB2	882	475	0.02%	0.003%
49	9.519	2633	2637	2641	rBV3	653	551	0.02%	0.003%
50	9.539	2641	2643	2647	rVV4	936	621	0.02%	0.003%
51	9.670	2677	2684	2690	rVB6	3327	4707	0.18%	0.025%
52	9.696	2690	2692	2698	rVB2	848	691	0.03%	0.004%
53	9.744	2702	2707	2708	rBV3	669	500	0.02%	0.003%
54	9.780	2715	2718	2720	rBV3	1188	824	0.03%	0.004%
55	9.850	2737	2740	2743	rBV2	837	595	0.02%	0.003%
56	9.870	2743	2746	2752	rVB4	744	588	0.02%	0.003%
57	9.963	2773	2775	2780	rVB3	739	473	0.02%	0.002%
58	10.047	2796	2801	2805	rBV6	1204	1108	0.04%	0.006%
59	10.146	2816	2832	2856	rBV	717335	1140965	43.36%	6.020%
60	10.429	2917	2920	2923	rVB3	985	558	0.02%	0.003%
61	10.510	2939	2945	2948	rVV7	507	603	0.02%	0.003%
62	10.567	2959	2963	2967	rVB5	978	795	0.03%	0.004%
63	10.596	2969	2972	2976	rVB3	742	538	0.02%	0.003%
64	10.625	2976	2981	2984	rBV5	596	478	0.02%	0.003%
65	10.686	2995	3000	3003	rBV4	981	860	0.03%	0.005%
66	10.786	3023	3031	3036	rVB9	1782	2647	0.10%	0.014%
67	10.821	3037	3042	3045	rBV4	837	898	0.03%	0.005%
68	10.863	3052	3055	3060	rVV4	905	878	0.03%	0.005%
69	11.114	3130	3133	3135	rBV2	904	559	0.02%	0.003%
70	11.178	3141	3153	3185	rBV	1117157	1764215	67.05%	9.309%
71	11.551	3256	3269	3302	rBV	1251249	2022344	76.86%	10.671%
72	11.866	3364	3367	3369	rBV2	1098	678	0.03%	0.004%
73	11.931	3384	3387	3389	rBV3	1109	764	0.03%	0.004%
74	11.950	3389	3393	3395	rVV5	975	804	0.03%	0.004%
75	11.963	3395	3397	3401	rVV4	652	600	0.02%	0.003%
76	11.995	3405	3407	3410	rVB3	809	491	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037676.D
 Acq On : 30 Sep 2024 23:08
 Operator : SY/MD
 Sample : P4228-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0CP6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.046	3422	3423	3427	rVB4	961	576	0.02%	0.003%
78	12.149	3452	3455	3458	rBV4	890	595	0.02%	0.003%
79	12.394	3527	3531	3536	rVB4	804	595	0.02%	0.003%
80	12.442	3542	3546	3550	rBV4	649	476	0.02%	0.003%
81	12.481	3552	3558	3561	rBV4	1231	1137	0.04%	0.006%
82	12.841	3667	3670	3673	rVB3	632	491	0.02%	0.003%
83	12.908	3687	3691	3694	rBV3	776	513	0.02%	0.003%
84	12.947	3698	3703	3705	rBV3	749	623	0.02%	0.003%
85	13.053	3729	3736	3737	rBV4	1139	1209	0.05%	0.006%
86	13.120	3755	3757	3760	rVV3	826	494	0.02%	0.003%
87	13.191	3773	3779	3780	rBV5	885	689	0.03%	0.004%
88	13.307	3811	3815	3818	rBV3	1266	1128	0.04%	0.006%
89	13.583	3897	3901	3904	rBV6	771	617	0.02%	0.003%
90	13.686	3929	3933	3941	rVB7	2166	2245	0.09%	0.012%
91	14.037	4040	4042	4045	rBV3	799	653	0.02%	0.003%
92	14.098	4058	4061	4063	rBV3	654	497	0.02%	0.003%
93	14.133	4068	4072	4075	rBV3	875	768	0.03%	0.004%
94	14.493	4179	4184	4186	rBV5	1505	1392	0.05%	0.007%
95	14.506	4186	4188	4190	rVV2	1008	559	0.02%	0.003%
96	14.519	4190	4192	4196	rVB4	1136	788	0.03%	0.004%
97	14.667	4235	4238	4240	rBV2	1027	621	0.02%	0.003%
98	15.043	4353	4355	4357	rBV3	1066	638	0.02%	0.003%
99	15.336	4443	4446	4448	rBV2	1294	754	0.03%	0.004%
100	15.853	4605	4607	4609	rBV2	1613	888	0.03%	0.005%

Sum of corrected areas: 18951686




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037676.D
Acq On : 30 Sep 2024 23:08
Operator : SY/MD
Sample : P4228-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

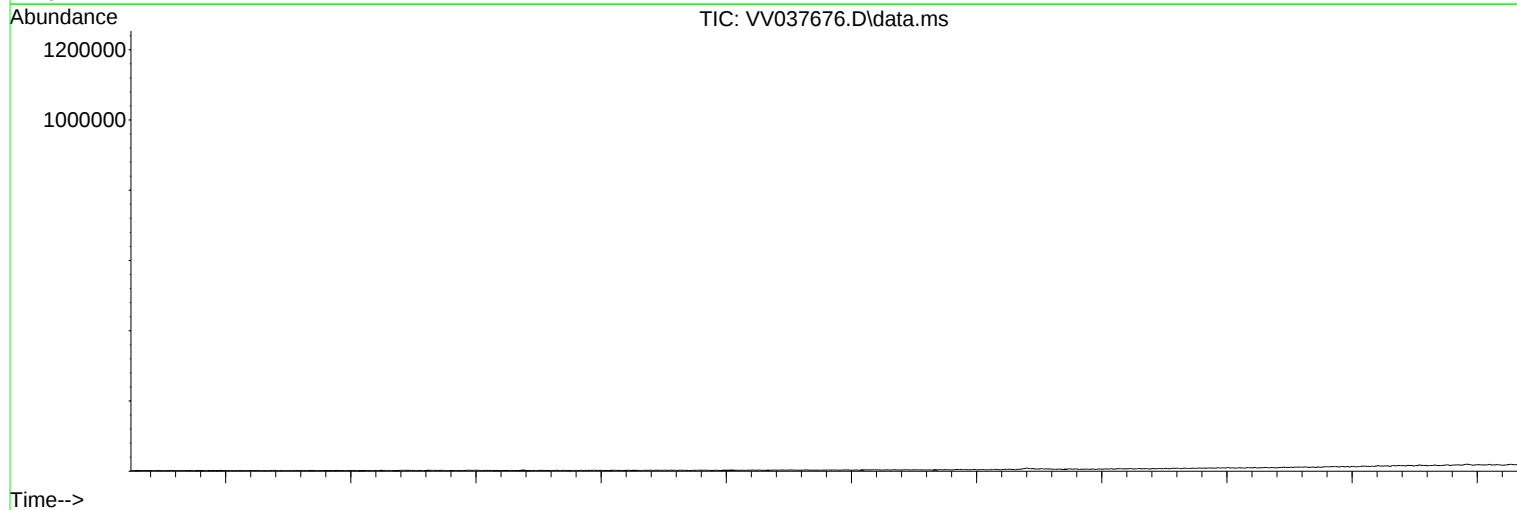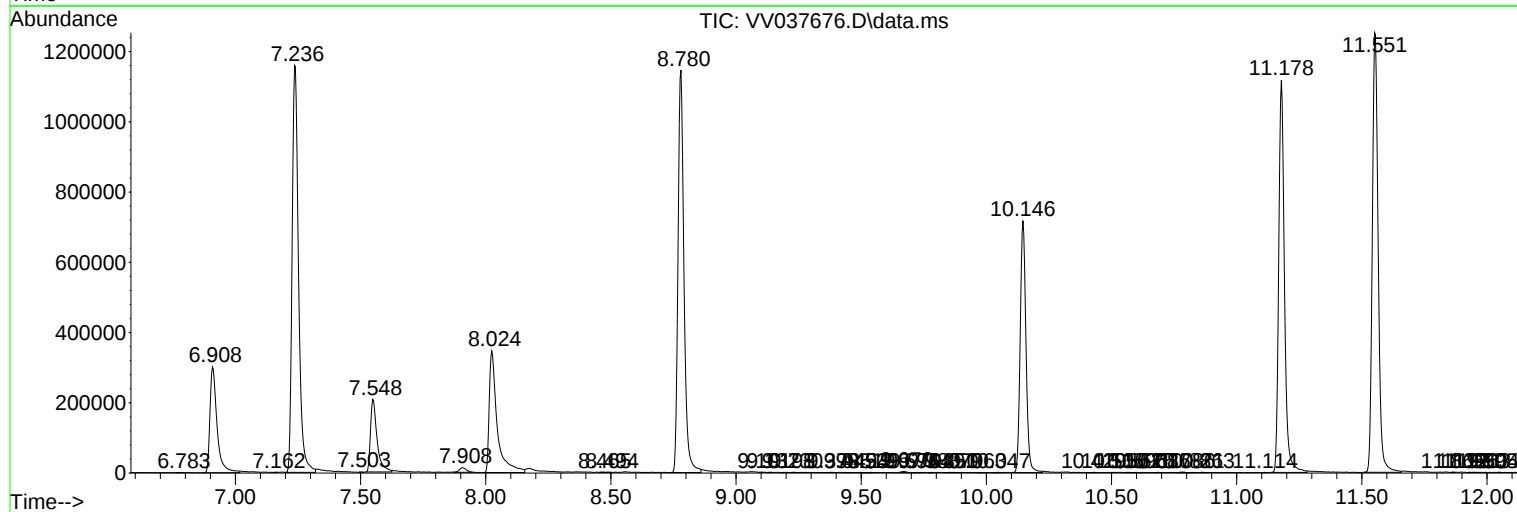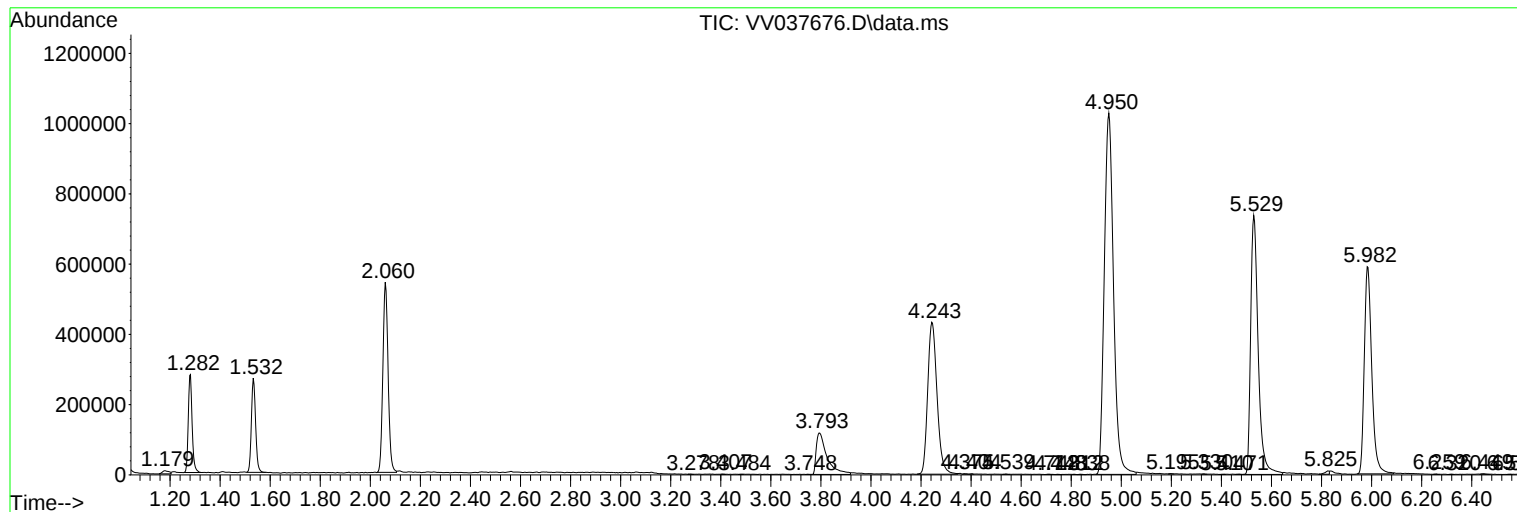

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037676.D
Acq On : 30 Sep 2024 23:08
Operator : SY/MD
Sample : P4228-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037676.D
Acq On : 30 Sep 2024 23:08
Operator : SY/MD
Sample : P4228-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0CP6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------