

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037678.D
 Acq On : 30 Sep 2024 23:51
 Operator : SY/MD
 Sample : VIBLK395
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037678.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	51	rBV	11421	19335	0.75%	0.108%
2	1.278	67	74	93	rVB	365919	396681	15.48%	2.223%
3	1.532	145	153	173	rVB	313209	365792	14.28%	2.050%
4	2.060	307	317	332	rBV	608735	878373	34.28%	4.922%
5	3.333	710	713	715	rBV2	837	632	0.02%	0.004%
6	3.413	735	738	742	rBV4	530	538	0.02%	0.003%
7	3.468	751	755	758	rVB5	827	681	0.03%	0.004%
8	3.793	848	856	887	rBV	103532	303872	11.86%	1.703%
9	4.098	947	951	955	rBV5	1041	861	0.03%	0.005%
10	4.243	978	996	1026	rBV	406400	1057065	41.26%	5.924%
11	4.519	1079	1082	1088	rBV4	825	837	0.03%	0.005%
12	4.574	1096	1099	1103	rBV3	852	594	0.02%	0.003%
13	4.751	1150	1154	1161	rBV4	878	1024	0.04%	0.006%
14	4.783	1161	1164	1168	rBV3	831	550	0.02%	0.003%
15	4.847	1177	1184	1185	rBV4	929	872	0.03%	0.005%
16	4.950	1200	1216	1245	rBV2	1002475	2562029	100.00%	14.358%
17	5.314	1326	1329	1331	rBV3	1065	737	0.03%	0.004%
18	5.375	1344	1348	1354	rVB6	951	917	0.04%	0.005%
19	5.400	1354	1356	1361	rVB4	1220	975	0.04%	0.005%
20	5.429	1361	1365	1369	rBV4	906	722	0.03%	0.004%
21	5.529	1385	1396	1431	rBV	675762	1417078	55.31%	7.941%
22	5.802	1478	1481	1482	rBV4	824	552	0.02%	0.003%
23	5.831	1482	1490	1505	rVV7	7360	16551	0.65%	0.093%
24	5.982	1524	1537	1569	rBV	560372	1170745	45.70%	6.561%
25	6.156	1588	1591	1594	rBV4	992	777	0.03%	0.004%
26	6.175	1595	1597	1600	rVV3	1502	960	0.04%	0.005%
27	6.191	1600	1602	1606	rVB3	1206	753	0.03%	0.004%
28	6.342	1648	1649	1654	rVB4	879	569	0.02%	0.003%
29	6.452	1680	1683	1688	rBV3	781	655	0.03%	0.004%
30	6.719	1763	1766	1772	rBV4	571	584	0.02%	0.003%
31	6.757	1772	1778	1782	rVB5	596	595	0.02%	0.003%
32	6.908	1815	1825	1863	rBV	288042	558788	21.81%	3.131%
33	7.175	1900	1908	1916	rBV5	4929	9703	0.38%	0.054%
34	7.239	1916	1928	1957	rBV	1106738	1965430	76.71%	11.014%
35	7.551	2016	2025	2046	rBV	186720	348172	13.59%	1.951%
36	7.641	2047	2053	2066	rVV3	18058	37533	1.46%	0.210%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037678.D
 Acq On : 30 Sep 2024 23:51
 Operator : SY/MD
 Sample : VIBLK395
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.937	2142	2145	2148	rBV3	1016	560	0.02%	0.003%
38	8.024	2160	2172	2209	rBV	320947	684547	26.72%	3.836%
39	8.555	2332	2337	2339	rBV5	1196	1228	0.05%	0.007%
40	8.722	2384	2389	2391	rBV4	951	775	0.03%	0.004%
41	8.780	2396	2407	2442	rBV	1035107	1725570	67.35%	9.670%
42	9.104	2506	2508	2513	rVB5	970	720	0.03%	0.004%
43	9.143	2518	2520	2523	rVB4	1254	571	0.02%	0.003%
44	9.162	2523	2526	2532	rBV5	832	920	0.04%	0.005%
45	9.191	2533	2535	2537	rVB3	1295	598	0.02%	0.003%
46	9.210	2540	2541	2545	rVB4	905	552	0.02%	0.003%
47	9.297	2565	2568	2571	rBV4	783	617	0.02%	0.003%
48	9.410	2600	2603	2608	rBV3	790	754	0.03%	0.004%
49	9.513	2633	2635	2641	rVB4	856	586	0.02%	0.003%
50	9.619	2664	2668	2671	rBV3	807	772	0.03%	0.004%
51	9.661	2678	2681	2685	rBV4	841	792	0.03%	0.004%
52	9.744	2702	2707	2709	rBV4	647	568	0.02%	0.003%
53	9.805	2719	2726	2727	rBV4	537	563	0.02%	0.003%
54	9.876	2745	2748	2750	rBV2	976	691	0.03%	0.004%
55	9.934	2763	2766	2769	rVV	719	556	0.02%	0.003%
56	10.146	2818	2832	2854	rBV	633190	990102	38.65%	5.549%
57	10.294	2876	2878	2882	rVB5	1253	698	0.03%	0.004%
58	10.313	2882	2884	2885	rBV2	1393	577	0.02%	0.003%
59	10.342	2890	2893	2896	rVV3	742	604	0.02%	0.003%
60	10.387	2904	2907	2909	rBV4	851	556	0.02%	0.003%
61	10.435	2918	2922	2926	rBV3	747	707	0.03%	0.004%
62	10.487	2935	2938	2944	rVB3	1466	1517	0.06%	0.009%
63	10.625	2976	2981	2986	rBV3	723	658	0.03%	0.004%
64	10.783	3024	3030	3032	rBV5	1005	958	0.04%	0.005%
65	10.866	3048	3056	3059	rBV5	1407	1794	0.07%	0.010%
66	11.130	3133	3138	3139	rBV2	1182	809	0.03%	0.005%
67	11.178	3142	3153	3183	rBV	971344	1556073	60.74%	8.720%
68	11.397	3217	3221	3225	rBV4	1425	1575	0.06%	0.009%
69	11.468	3241	3243	3248	rVB3	1361	875	0.03%	0.005%
70	11.554	3258	3270	3299	rBV	1069206	1717184	67.02%	9.623%
71	11.863	3362	3366	3368	rBV3	1349	919	0.04%	0.005%
72	11.940	3386	3390	3395	rBV6	1151	1131	0.04%	0.006%
73	12.056	3424	3426	3433	rVB5	830	615	0.02%	0.003%
74	12.185	3463	3466	3469	rVB2	1101	601	0.02%	0.003%
75	12.201	3469	3471	3476	rBV2	1328	944	0.04%	0.005%
76	12.242	3482	3484	3488	rBV3	712	585	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037678.D
 Acq On : 30 Sep 2024 23:51
 Operator : SY/MD
 Sample : VIBLK395
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK395

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.400	3528	3533	3535	rVV3	737	709	0.03%	0.004%
78	12.484	3554	3559	3563	rBV4	484	607	0.02%	0.003%
79	12.525	3568	3572	3575	rBV5	827	731	0.03%	0.004%
80	12.596	3591	3594	3597	rVB3	1419	933	0.04%	0.005%
81	12.683	3616	3621	3628	rVV6	1251	2002	0.08%	0.011%
82	12.712	3628	3630	3634	rVB3	1001	733	0.03%	0.004%
83	12.754	3640	3643	3648	rBV5	1061	1158	0.05%	0.006%
84	12.796	3654	3656	3665	rVB3	859	761	0.03%	0.004%
85	12.834	3665	3668	3670	rBV2	963	673	0.03%	0.004%
86	13.313	3813	3817	3819	rBV3	916	543	0.02%	0.003%
87	13.400	3842	3844	3848	rBV4	815	622	0.02%	0.003%
88	13.574	3895	3898	3902	rBV3	617	542	0.02%	0.003%
89	13.689	3929	3934	3938	rVV5	722	757	0.03%	0.004%
90	13.731	3944	3947	3950	rVB3	959	642	0.03%	0.004%
91	13.969	4019	4021	4022	rBV	1297	602	0.02%	0.003%
92	14.046	4042	4045	4047	rBV2	1215	744	0.03%	0.004%
93	14.387	4147	4151	4153	rVB4	1104	640	0.02%	0.004%
94	14.574	4205	4209	4211	rBV5	2618	1998	0.08%	0.011%
95	14.664	4235	4237	4241	rVB4	1059	602	0.02%	0.003%
96	14.988	4336	4338	4341	rBV2	1186	805	0.03%	0.005%
97	15.101	4370	4373	4374	rBV3	1291	697	0.03%	0.004%
98	15.172	4391	4395	4399	rBV6	1149	1168	0.05%	0.007%
99	15.432	4473	4476	4480	rBV6	1181	912	0.04%	0.005%
100	15.471	4486	4488	4490	rBV2	1252	586	0.02%	0.003%

Sum of corrected areas: 17844121




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037678.D
Acq On : 30 Sep 2024 23:51
Operator : SY/MD
Sample : VIBLK395
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

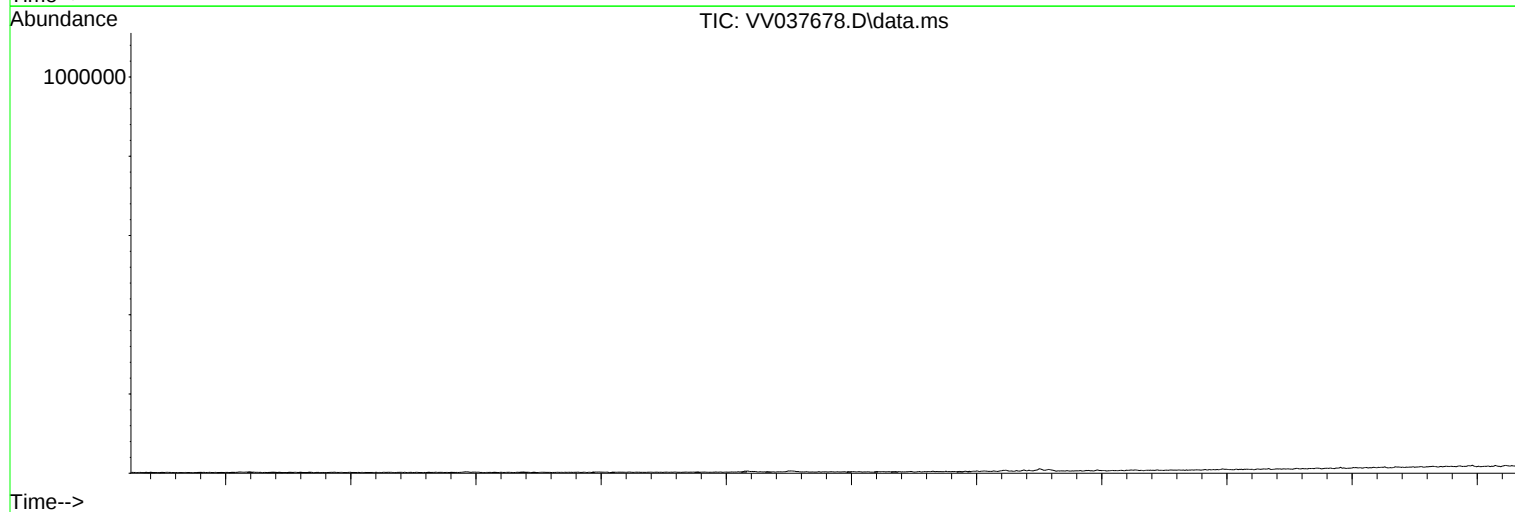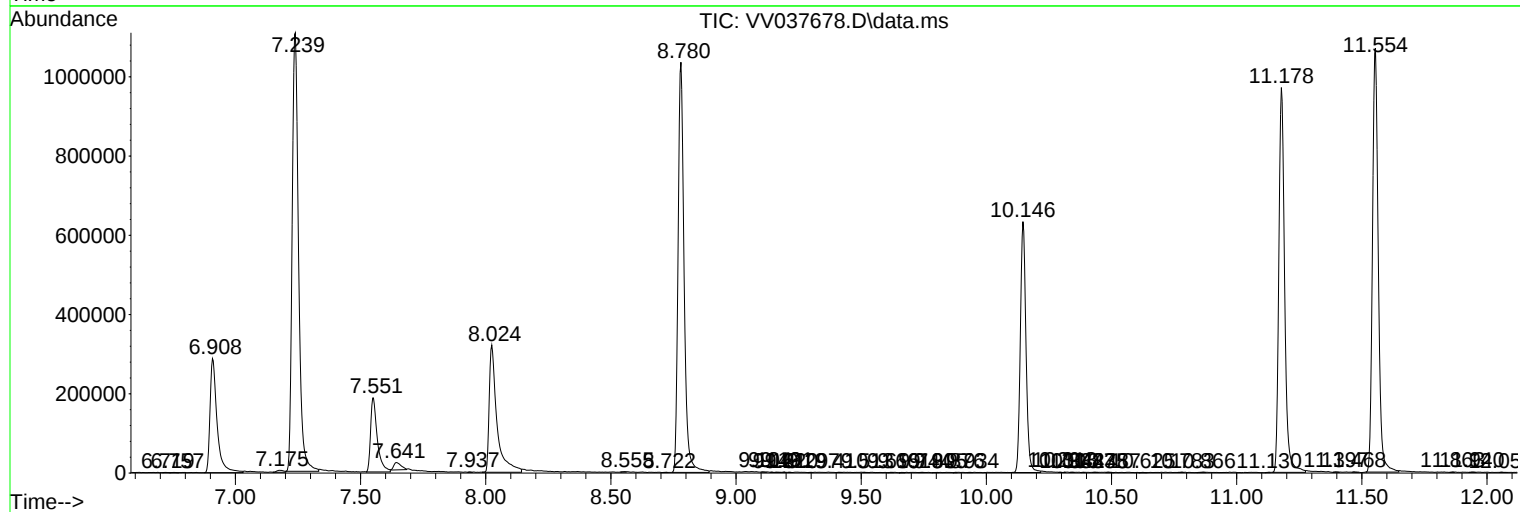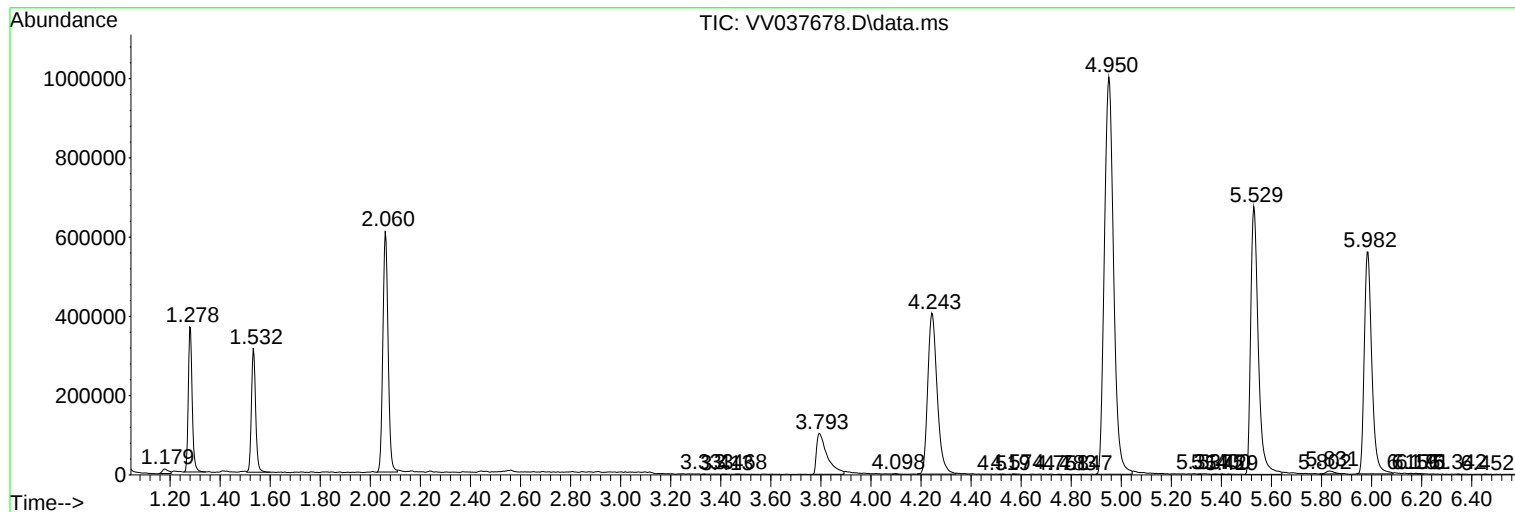

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037678.D
Acq On : 30 Sep 2024 23:51
Operator : SY/MD
Sample : VIBLK395
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037678.D
Acq On : 30 Sep 2024 23:51
Operator : SY/MD
Sample : VIBLK395
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK395

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
