

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037679.D
 Acq On : 01 Oct 2024 00:12
 Operator : SY/MD
 Sample : P4206-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037679.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV2	18766	25307	0.98%	0.136%
2	1.282	68	75	94	rVB	275711	294592	11.44%	1.588%
3	1.532	146	153	170	rVB	262506	310406	12.06%	1.673%
4	2.060	308	317	331	rVB	520915	744103	28.90%	4.010%
5	3.256	685	689	694	rBV6	1298	1360	0.05%	0.007%
6	3.407	734	736	740	rVB3	689	372	0.01%	0.002%
7	3.429	740	743	745	rVB2	534	320	0.01%	0.002%
8	3.442	745	747	749	rBV2	459	264	0.01%	0.001%
9	3.671	816	818	819	rBV	426	201	0.01%	0.001%
10	3.719	831	833	836	rVB2	546	250	0.01%	0.001%
11	3.793	847	856	892	rBV	123712	371325	14.42%	2.001%
12	4.243	980	996	1026	rBV	418035	1081370	42.00%	5.827%
13	4.632	1114	1117	1118	rBV	532	332	0.01%	0.002%
14	4.751	1152	1154	1159	rVB4	888	695	0.03%	0.004%
15	4.790	1159	1166	1169	rBV4	795	791	0.03%	0.004%
16	4.802	1169	1170	1174	rBV	229	139	0.01%	0.001%
17	4.835	1178	1180	1184	rVV3	526	330	0.01%	0.002%
18	4.883	1193	1195	1200	rVB4	840	524	0.02%	0.003%
19	4.950	1200	1216	1254	rBV2	1001093	2574510	100.00%	13.874%
20	5.275	1315	1317	1321	rVB4	1135	617	0.02%	0.003%
21	5.298	1322	1324	1326	rBV3	811	407	0.02%	0.002%
22	5.410	1357	1359	1360	rBV	495	209	0.01%	0.001%
23	5.529	1385	1396	1433	rBV	736309	1512077	58.73%	8.148%
24	5.828	1479	1489	1506	rBV	8678	22847	0.89%	0.123%
25	5.986	1524	1538	1568	rBV	580489	1209693	46.99%	6.519%
26	6.243	1616	1618	1621	rBV3	1465	867	0.03%	0.005%
27	6.330	1643	1645	1647	rBV2	588	310	0.01%	0.002%
28	6.429	1674	1676	1678	rVB3	704	311	0.01%	0.002%
29	6.442	1678	1680	1683	rVB4	583	248	0.01%	0.001%
30	6.597	1726	1728	1729	rBV	298	79	0.00%	0.000%
31	6.632	1734	1739	1742	rBV4	925	1066	0.04%	0.006%
32	6.654	1745	1746	1749	rVB3	389	196	0.01%	0.001%
33	6.671	1749	1751	1754	rVB3	612	331	0.01%	0.002%
34	6.693	1756	1758	1761	rVB2	413	163	0.01%	0.001%
35	6.716	1761	1765	1766	rBV2	513	343	0.01%	0.002%
36	6.738	1770	1772	1774	rBV	268	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037679.D
 Acq On : 01 Oct 2024 00:12
 Operator : SY/MD
 Sample : P4206-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.761	1776	1779	1787	rVB3	769	638	0.02%	0.003%
38	6.799	1787	1791	1793	rVB2	309	182	0.01%	0.001%
39	6.815	1793	1796	1800	rVB2	669	497	0.02%	0.003%
40	6.841	1800	1804	1805	rBV3	399	293	0.01%	0.002%
41	6.854	1805	1808	1812	rVB3	1037	662	0.03%	0.004%
42	6.873	1812	1814	1815	rBV	208	103	0.00%	0.001%
43	6.908	1815	1825	1853	rBV	292151	566113	21.99%	3.051%
44	7.236	1917	1927	1961	rBV	1132965	2010032	78.07%	10.832%
45	7.548	2015	2024	2048	rBV	200864	378113	14.69%	2.038%
46	7.889	2127	2130	2133	rBV5	900	656	0.03%	0.004%
47	8.024	2163	2172	2209	rBV	340401	717895	27.88%	3.869%
48	8.738	2392	2394	2395	rBV2	537	265	0.01%	0.001%
49	8.780	2395	2407	2440	rVV	1128305	1887516	73.32%	10.172%
50	9.217	2540	2543	2548	rBV4	1186	1110	0.04%	0.006%
51	9.268	2556	2559	2561	rBV2	703	422	0.02%	0.002%
52	9.362	2586	2588	2591	rVB2	812	379	0.01%	0.002%
53	9.413	2601	2604	2607	rBV3	777	410	0.02%	0.002%
54	9.429	2607	2609	2610	rBV2	479	161	0.01%	0.001%
55	9.497	2626	2630	2635	rVB5	1073	1031	0.04%	0.006%
56	9.545	2642	2645	2646	rBV	348	159	0.01%	0.001%
57	9.555	2646	2648	2650	rVV2	420	202	0.01%	0.001%
58	9.603	2661	2663	2664	rBV2	651	267	0.01%	0.001%
59	9.641	2674	2675	2680	rBV4	414	268	0.01%	0.001%
60	9.686	2686	2689	2692	rBB3	914	463	0.02%	0.002%
61	9.741	2702	2706	2709	rBV3	394	372	0.01%	0.002%
62	9.773	2714	2716	2720	rBV5	855	478	0.02%	0.003%
63	9.860	2740	2743	2746	rVB	1090	704	0.03%	0.004%
64	9.915	2759	2760	2761	rBV	507	176	0.01%	0.001%
65	9.985	2777	2782	2784	rBV2	614	485	0.02%	0.003%
66	9.998	2784	2786	2789	rVB3	539	309	0.01%	0.002%
67	10.063	2803	2806	2807	rBV3	417	188	0.01%	0.001%
68	10.079	2807	2811	2815	rVV2	513	523	0.02%	0.003%
69	10.146	2820	2832	2853	rBV	686466	1099962	42.73%	5.928%
70	10.439	2919	2923	2924	rBV3	350	284	0.01%	0.002%
71	10.632	2979	2983	2985	rBV3	559	411	0.02%	0.002%
72	10.690	2998	3001	3005	rBV4	610	528	0.02%	0.003%
73	10.741	3012	3017	3019	rBV4	610	491	0.02%	0.003%
74	10.783	3025	3030	3033	rBV4	1569	1394	0.05%	0.008%
75	10.825	3040	3043	3046	rBV2	740	505	0.02%	0.003%
76	10.908	3067	3069	3074	rBV4	458	487	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037679.D
 Acq On : 01 Oct 2024 00:12
 Operator : SY/MD
 Sample : P4206-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY052

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.040	3108	3110	3112	rVB2	393	183	0.01%	0.001%
78	11.104	3128	3130	3132	rBV2	849	386	0.01%	0.002%
79	11.178	3142	3153	3184	rBV	1091539	1746462	67.84%	9.411%
80	11.503	3253	3254	3256	rBV	676	333	0.01%	0.002%
81	11.551	3258	3269	3301	rVV	1220897	1968331	76.45%	10.607%
82	11.969	3397	3399	3402	rVB4	718	339	0.01%	0.002%
83	12.066	3428	3429	3431	rBV2	571	258	0.01%	0.001%
84	12.127	3443	3448	3450	rBV3	724	788	0.03%	0.004%
85	12.153	3454	3456	3459	rVV4	520	279	0.01%	0.002%
86	12.188	3465	3467	3469	rBV3	676	338	0.01%	0.002%
87	12.252	3484	3487	3489	rBV3	793	448	0.02%	0.002%
88	12.329	3509	3511	3512	rBV	778	389	0.02%	0.002%
89	12.416	3536	3538	3540	rBV	628	358	0.01%	0.002%
90	12.484	3557	3559	3562	rBV2	830	308	0.01%	0.002%
91	12.561	3580	3583	3586	rBV2	1015	747	0.03%	0.004%
92	12.635	3603	3606	3608	rBV3	913	676	0.03%	0.004%
93	12.680	3617	3620	3621	rBV2	834	377	0.01%	0.002%
94	12.741	3637	3639	3642	rBV4	1017	492	0.02%	0.003%
95	12.828	3664	3666	3672	rVB4	1612	1210	0.05%	0.007%
96	12.892	3683	3686	3687	rVB2	860	380	0.01%	0.002%
97	12.940	3697	3701	3703	rBV4	667	558	0.02%	0.003%
98	13.056	3733	3737	3739	rBV2	662	620	0.02%	0.003%
99	14.146	4074	4076	4078	rBV2	789	337	0.01%	0.002%

Sum of corrected areas: 18556818




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037679.D
Acq On : 01 Oct 2024 00:12
Operator : SY/MD
Sample : P4206-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

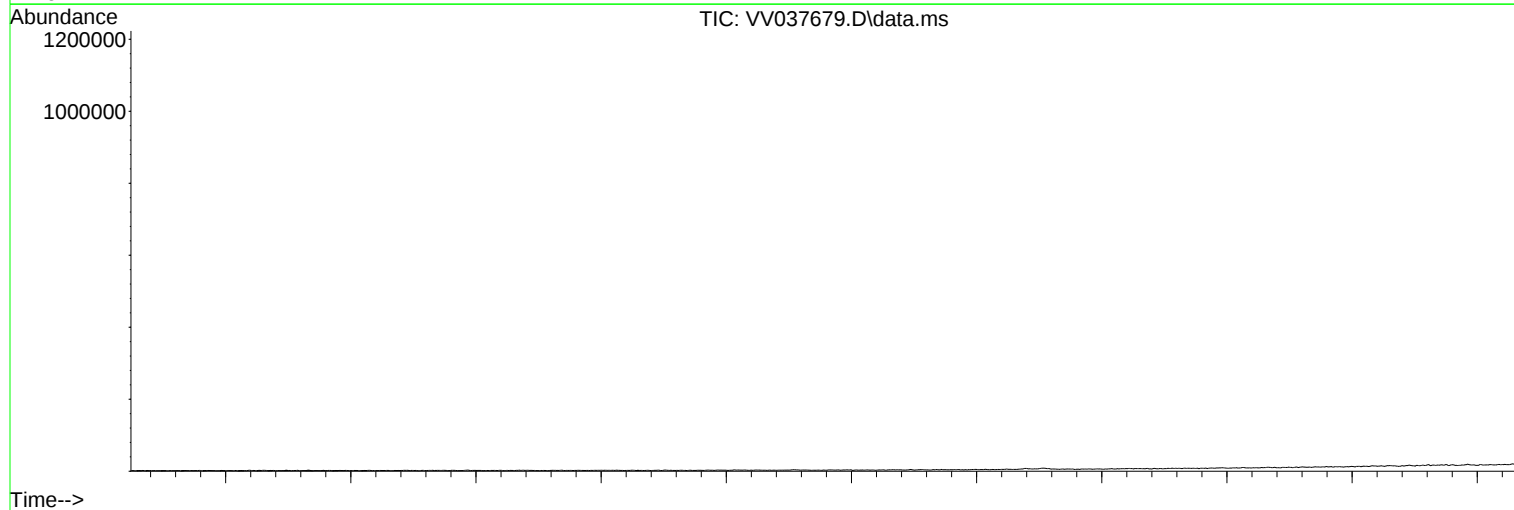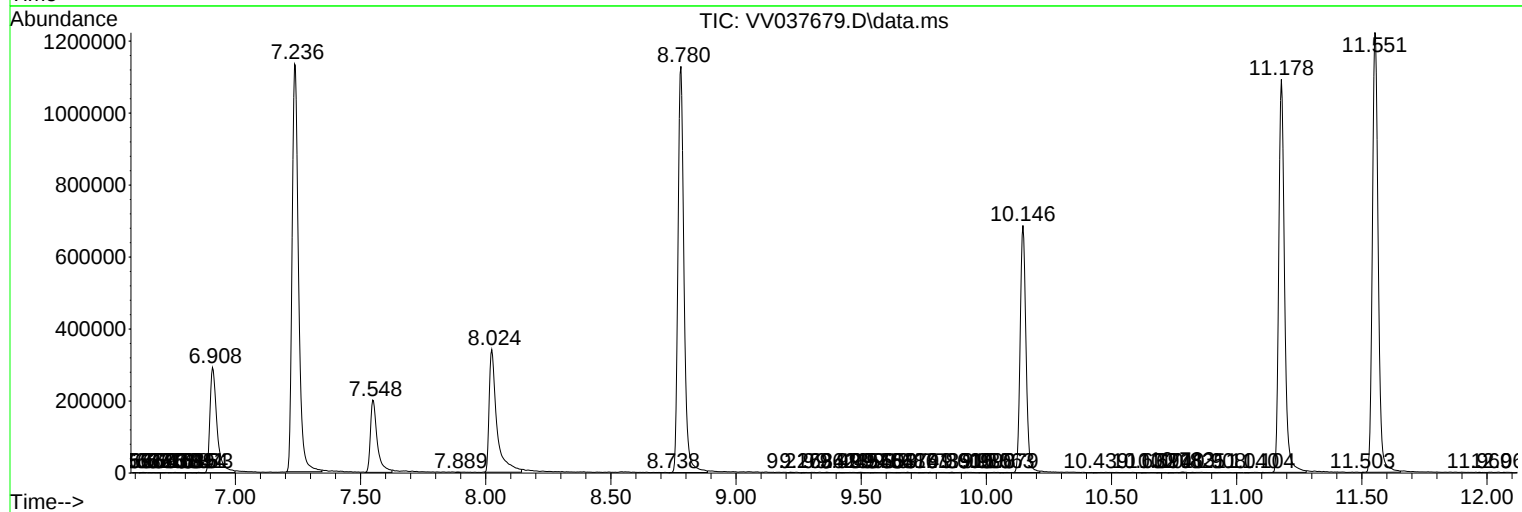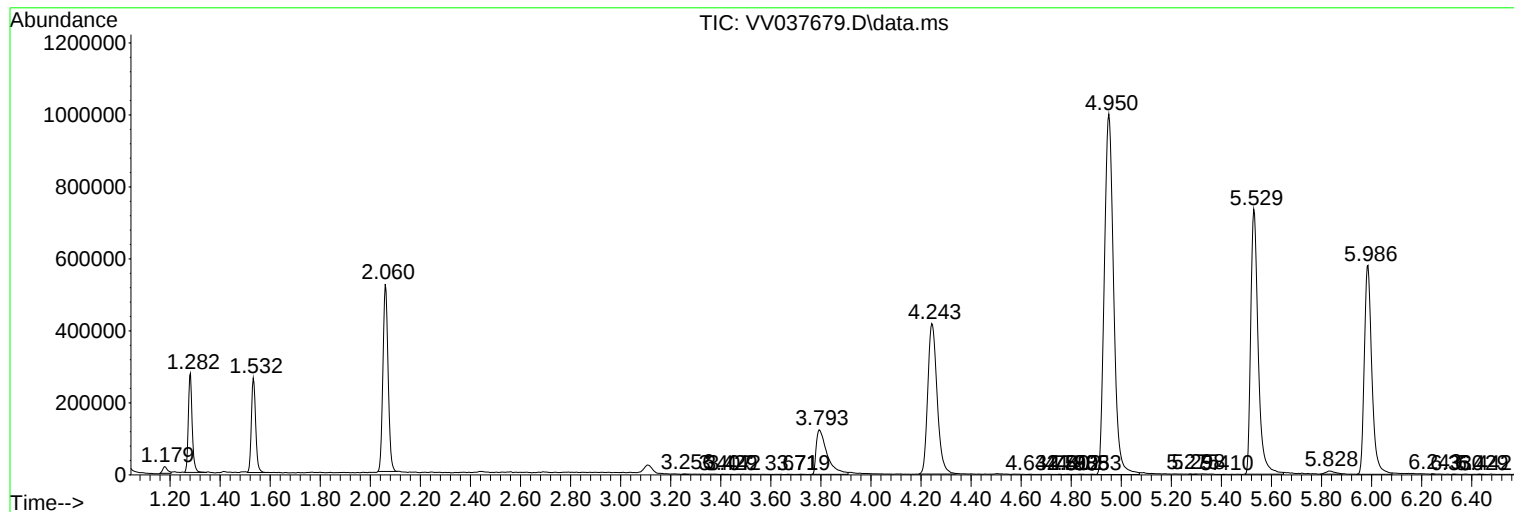

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037679.D
Acq On : 01 Oct 2024 00:12
Operator : SY/MD
Sample : P4206-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037679.D
Acq On : 01 Oct 2024 00:12
Operator : SY/MD
Sample : P4206-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY052

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
