

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037683.D
 Acq On : 01 Oct 2024 01:38
 Operator : SY/MD
 Sample : P4205-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV2	18538	29788	0.15%	0.050%
2	1.285	68	76	95	rBV2	1826782	1990238	9.70%	3.343%
3	1.548	146	158	181	rVB2	1767236	2345067	11.43%	3.939%
4	2.063	308	318	333	rBV3	612770	976955	4.76%	1.641%
5	2.693	504	514	534	rVB	377987	644813	3.14%	1.083%
6	3.104	627	642	672	rVB	5501298	11196628	54.58%	18.806%
7	3.574	786	788	792	rVB2	1044	482	0.00%	0.001%
8	3.600	792	796	797	rBV3	483	297	0.00%	0.000%
9	3.612	797	800	803	rBV4	498	274	0.00%	0.000%
10	3.731	832	837	838	rBV4	796	476	0.00%	0.001%
11	3.805	843	860	910	rBV	8783912	20514454	100.00%	34.457%
12	4.243	982	996	1027	rVB	419115	1064684	5.19%	1.788%
13	4.503	1059	1077	1112	rVB	1375713	3502947	17.08%	5.884%
14	4.950	1200	1216	1239	rBV2	994734	2614300	12.74%	4.391%
15	5.365	1344	1345	1350	rVB3	1315	636	0.00%	0.001%
16	5.529	1385	1396	1436	rBV	734926	1525468	7.44%	2.562%
17	5.828	1477	1489	1516	rBV	446116	914094	4.46%	1.535%
18	5.982	1526	1537	1566	rBV	580312	1187582	5.79%	1.995%
19	6.291	1631	1633	1634	rBV	488	186	0.00%	0.000%
20	6.471	1687	1689	1691	rBV	608	294	0.00%	0.000%
21	6.484	1691	1693	1695	rVV3	1098	567	0.00%	0.001%
22	6.506	1698	1700	1704	rVB3	899	674	0.00%	0.001%
23	6.603	1727	1730	1731	rBV2	577	290	0.00%	0.000%
24	6.638	1739	1741	1743	rBV2	372	169	0.00%	0.000%
25	6.725	1766	1768	1769	rBV	401	112	0.00%	0.000%
26	6.754	1773	1777	1783	rVB4	1001	1041	0.01%	0.002%
27	6.776	1783	1784	1787	rVB2	312	108	0.00%	0.000%
28	6.792	1787	1789	1792	rBV3	303	195	0.00%	0.000%
29	6.863	1808	1811	1813	rBV4	452	319	0.00%	0.001%
30	6.908	1813	1825	1852	rBV	300457	580969	2.83%	0.976%
31	7.236	1917	1927	1969	rBV	1137555	2034167	9.92%	3.417%
32	7.548	2015	2024	2050	rBV	199500	377058	1.84%	0.633%
33	7.902	2122	2134	2158	rBV	305889	525078	2.56%	0.882%
34	8.024	2163	2172	2206	rBV2	333395	692774	3.38%	1.164%
35	8.619	2353	2357	2359	rBV4	925	619	0.00%	0.001%
36	8.779	2396	2407	2442	rBV	1123847	1887174	9.20%	3.170%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037683.D
 Acq On : 01 Oct 2024 01:38
 Operator : SY/MD
 Sample : P4205-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	9.185	2531	2533	2534	rBV2	622	248	0.00%	0.000%
38	9.329	2576	2578	2584	rVB7	695	676	0.00%	0.001%
39	9.358	2584	2587	2590	rBV4	730	540	0.00%	0.001%
40	9.394	2596	2598	2601	rBV3	835	483	0.00%	0.001%
41	9.471	2620	2622	2625	rBV3	607	495	0.00%	0.001%
42	9.513	2633	2635	2637	rBV2	815	359	0.00%	0.001%
43	9.609	2662	2665	2667	rBV3	974	556	0.00%	0.001%
44	9.622	2667	2669	2672	rVB3	795	382	0.00%	0.001%
45	9.638	2672	2674	2675	rBV2	350	141	0.00%	0.000%
46	9.660	2678	2681	2682	rBV2	556	300	0.00%	0.001%
47	9.751	2707	2709	2712	rBV3	557	393	0.00%	0.001%
48	9.818	2728	2730	2734	rBV3	584	349	0.00%	0.001%
49	9.866	2739	2745	2747	rBV3	3674	3566	0.02%	0.006%
50	9.940	2766	2768	2770	rBV3	605	305	0.00%	0.001%
51	9.956	2771	2773	2777	rVB3	651	340	0.00%	0.001%
52	9.972	2777	2778	2780	rBV2	345	132	0.00%	0.000%
53	9.988	2780	2783	2787	rVB3	1000	738	0.00%	0.001%
54	10.014	2787	2791	2794	rBV4	1040	800	0.00%	0.001%
55	10.030	2794	2796	2800	rBV3	986	812	0.00%	0.001%
56	10.104	2815	2819	2820	rBV2	516	293	0.00%	0.000%
57	10.146	2820	2832	2857	rVV	691406	1088774	5.31%	1.829%
58	10.352	2894	2896	2898	rBV4	548	263	0.00%	0.000%
59	10.387	2905	2907	2911	rBV3	840	470	0.00%	0.001%
60	10.406	2911	2913	2914	rVV	686	233	0.00%	0.000%
61	10.439	2918	2923	2926	rBV4	938	800	0.00%	0.001%
62	10.558	2958	2960	2962	rVB3	670	275	0.00%	0.000%
63	10.612	2975	2977	2979	rVB2	1032	391	0.00%	0.001%
64	10.632	2979	2983	2986	rBV3	795	593	0.00%	0.001%
65	10.754	3017	3021	3022	rBV3	433	336	0.00%	0.001%
66	10.776	3024	3028	3031	rBV5	1178	1084	0.01%	0.002%
67	10.818	3038	3041	3043	rBV	399	289	0.00%	0.000%
68	10.860	3047	3054	3064	rVV6	3788	5897	0.03%	0.010%
69	10.934	3076	3077	3082	rVB2	329	175	0.00%	0.000%
70	11.024	3103	3105	3107	rBV	635	326	0.00%	0.001%
71	11.037	3107	3109	3110	rBV	505	140	0.00%	0.000%
72	11.104	3127	3130	3131	rBV3	620	366	0.00%	0.001%
73	11.178	3143	3153	3185	rBV	1102656	1765780	8.61%	2.966%
74	11.464	3234	3242	3250	rBV8	3617	5316	0.03%	0.009%
75	11.551	3258	3269	3308	rBV	1216847	1991110	9.71%	3.344%
76	11.898	3375	3377	3379	rBV2	646	300	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
 Data File : VV037683.D
 Acq On : 01 Oct 2024 01:38
 Operator : SY/MD
 Sample : P4205-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY075

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.078	3431	3433	3436	rBV2	902	636	0.00%	0.001%
78	12.107	3439	3442	3445	rVB4	1051	686	0.00%	0.001%
79	12.156	3455	3457	3459	rBV3	545	309	0.00%	0.001%
80	12.220	3475	3477	3478	rBV2	503	260	0.00%	0.000%
81	12.252	3481	3487	3491	rBV4	1321	1034	0.01%	0.002%
82	12.310	3501	3505	3509	rBV4	1269	861	0.00%	0.001%
83	12.332	3509	3512	3516	rVB2	894	474	0.00%	0.001%
84	12.406	3531	3535	3537	rBV4	1259	1044	0.01%	0.002%
85	12.451	3547	3549	3550	rBV	606	267	0.00%	0.000%
86	12.538	3573	3576	3577	rBV3	488	259	0.00%	0.000%
87	12.580	3584	3589	3600	rVB8	4308	7248	0.04%	0.012%
88	12.725	3632	3634	3637	rVB3	898	389	0.00%	0.001%
89	12.873	3673	3680	3682	rBV4	633	694	0.00%	0.001%
90	12.918	3693	3694	3695	rVB	469	91	0.00%	0.000%
91	12.979	3709	3713	3716	rBV4	740	697	0.00%	0.001%
92	13.033	3727	3730	3732	rBV2	463	371	0.00%	0.001%
93	13.117	3753	3756	3759	rBV4	774	520	0.00%	0.001%
94	13.204	3778	3783	3794	rVB8	5551	9058	0.04%	0.015%
95	13.336	3822	3824	3826	rBV2	568	282	0.00%	0.000%
96	13.410	3845	3847	3850	rBV3	1003	548	0.00%	0.001%
97	13.448	3851	3859	3871	rVV2	11711	22436	0.11%	0.038%
98	13.757	3953	3955	3961	rVB4	1047	477	0.00%	0.001%
99	13.789	3963	3965	3967	rBV2	810	456	0.00%	0.001%
100	13.969	4017	4021	4023	rBV2	1307	1062	0.01%	0.002%

Sum of corrected areas: 59535962




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037683.D
Acq On : 01 Oct 2024 01:38
Operator : SY/MD
Sample : P4205-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

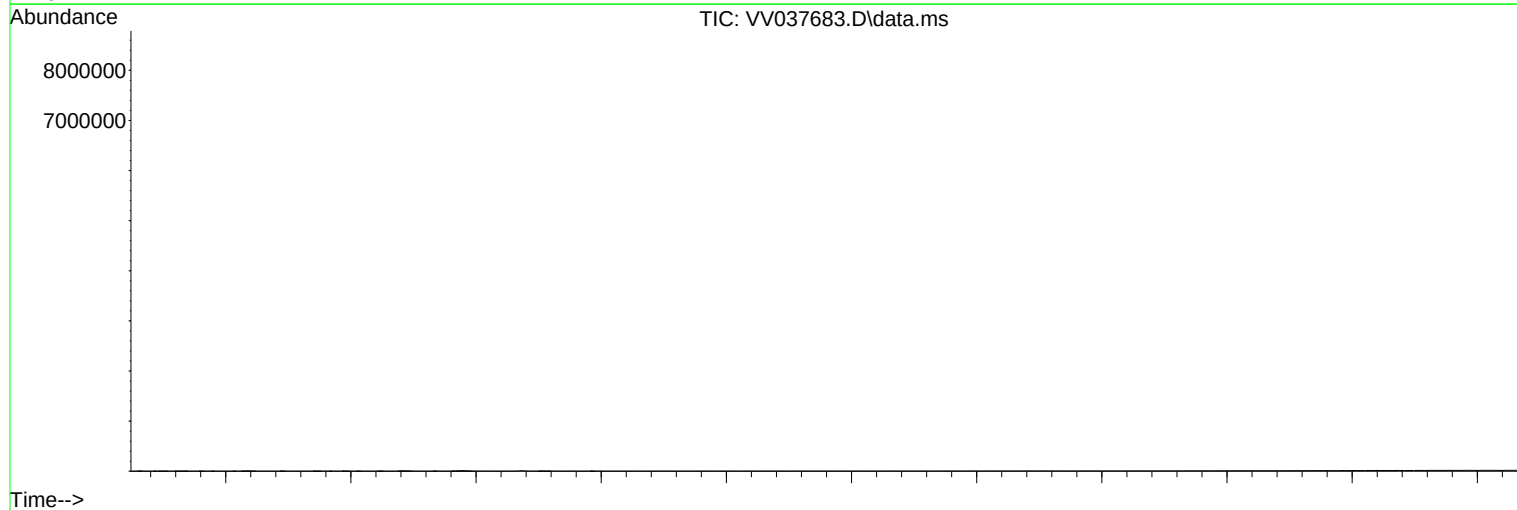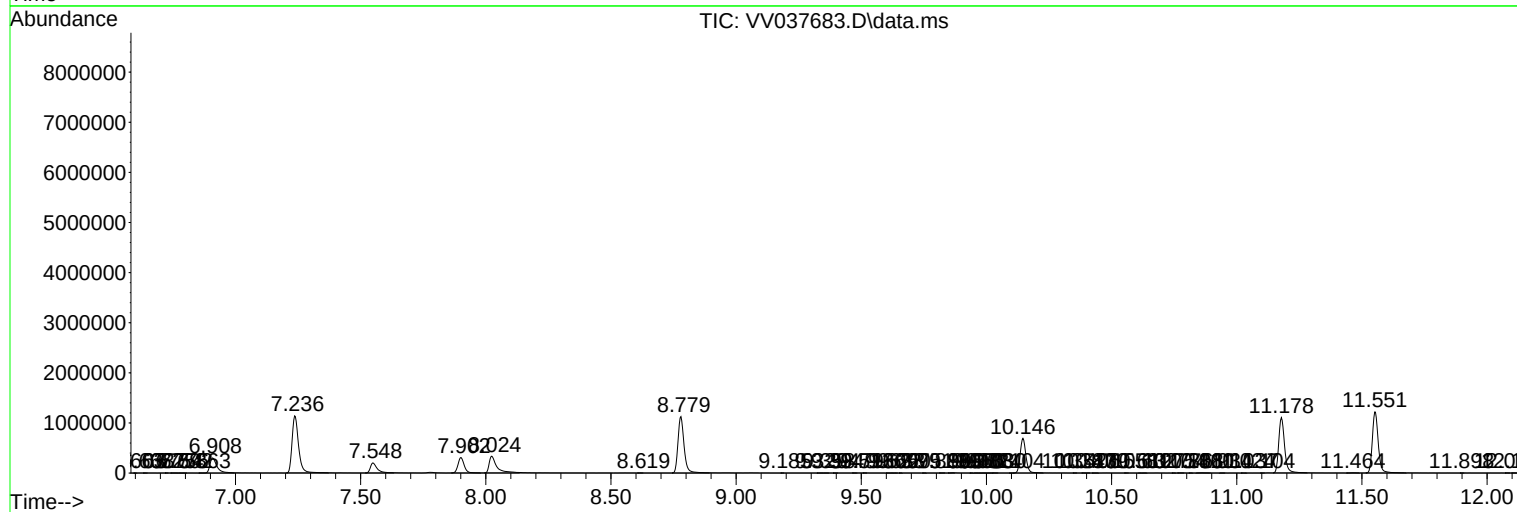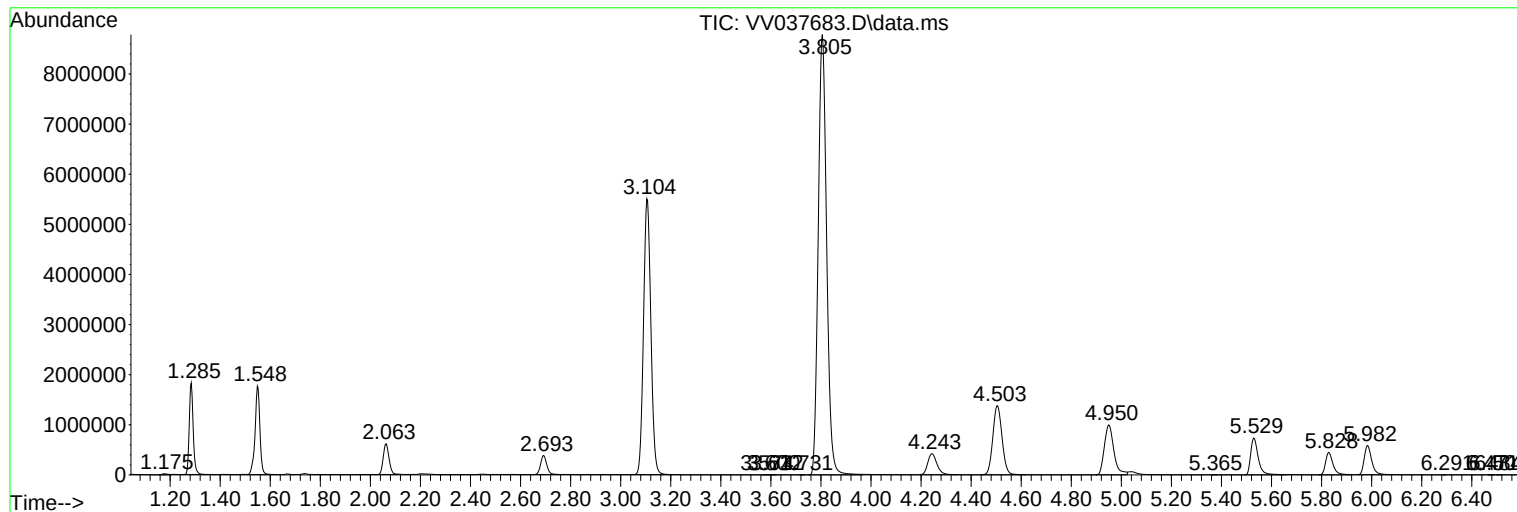

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037683.D
Acq On : 01 Oct 2024 01:38
Operator : SY/MD
Sample : P4205-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037683.D
Acq On : 01 Oct 2024 01:38
Operator : SY/MD
Sample : P4205-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY075

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
