
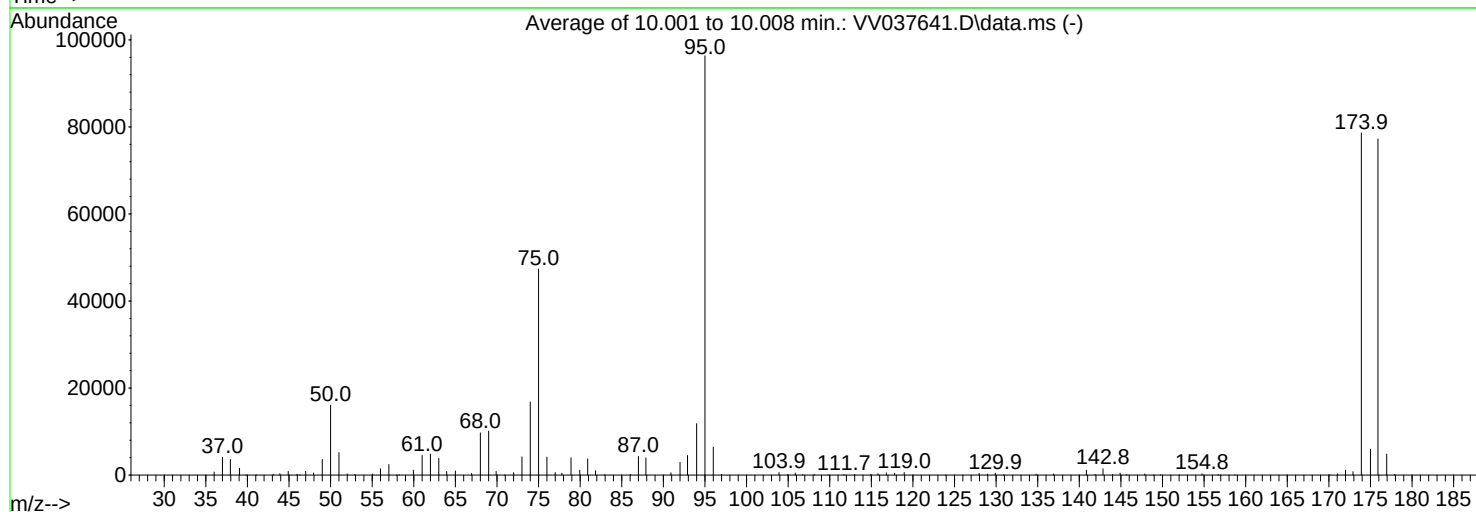


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV093024\
Data File : VV037641.D
Acq On : 30 Sep 2024 09:26
Operator : SY/MD
Sample : BFB383
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB383

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Tue Oct 01 04:32:07 2024

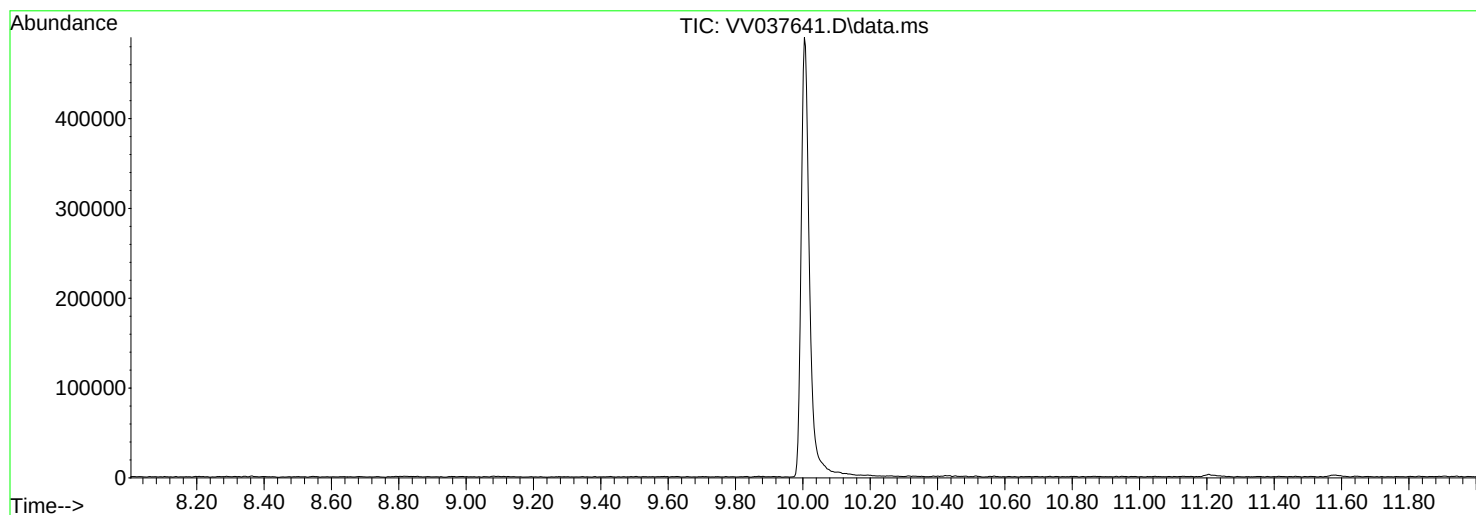

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	16046	PASS
75	95	30	80	49.1	47331	PASS
95	95	100	100	100.0	96363	PASS
96	95	5	9	6.7	6433	PASS
173	174	0.00	2	1.0	783	PASS
174	95	50	120	81.6	78603	PASS
175	174	5	9	7.6	5955	PASS
176	174	95	105	98.3	77232	PASS
177	176	5	10	6.2	4822	PASS

m/z	Abundance
37.90	163.0
39.90	237.0
44.00	752.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
36.00	569.0
37.00	4081.0
38.00	3785.0
39.10	1706.0
39.80	280.0
41.10	113.0
43.10	157.0
43.90	1012.0
44.90	817.0
45.90	157.0
46.30	237.0
47.00	823.0
48.00	491.0
49.00	3600.0
50.00	15458.0
51.00	5043.0
52.00	271.0
52.90	191.0
55.00	266.0
56.00	1432.0
57.00	2284.0
59.90	934.0
61.00	4489.0
62.00	4856.0
63.00	3589.0
63.90	843.0
65.00	911.0
66.90	318.0
68.00	9564.0
69.00	9638.0
69.90	873.0
72.00	513.0
73.00	4112.0
74.00	16227.0
75.00	46120.0
76.00	4097.0
77.00	629.0
77.80	452.0
78.90	3635.0
79.90	1151.0
80.90	3632.0
81.90	922.0
86.10	104.0
87.00	4019.0
87.90	3712.0
90.90	623.0
92.00	2814.0
92.90	4339.0
94.00	11462.0
95.00	91712.0
96.00	6435.0
97.00	207.0
103.90	516.0
104.90	124.0
105.90	501.0
106.80	167.0
108.20	139.0
109.80	131.0
111.70	117.0
113.00	141.0
115.80	322.0
116.80	537.0
117.80	418.0
118.90	591.0
123.90	106.0
127.90	394.0
129.00	207.0
129.80	378.0
134.80	160.0
137.00	226.0
140.90	1055.0
141.90	155.0
142.80	1375.0
144.00	153.0
144.90	476.0
145.70	106.0
147.80	235.0
148.90	102.0
149.80	104.0
154.70	317.0
156.70	130.0
157.00	114.0
158.70	120.0
170.10	103.0
171.00	273.0
172.00	1048.0
172.90	1122.0
173.90	73552.0
175.00	5483.0
175.90	71512.0
176.90	4720.0
177.90	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
36.00	706.0
37.00	4177.0
38.00	3943.0
39.10	1605.0
39.90	303.0
43.20	139.0
43.90	1098.0
44.90	879.0
46.00	180.0
47.00	845.0
48.00	495.0
49.00	3690.0
50.00	16520.0
51.00	5400.0
52.00	266.0
52.90	159.0
55.00	263.0
56.00	1515.0
57.00	2557.0
58.20	130.0
60.00	1189.0
61.00	4676.0
62.00	5002.0
63.00	3942.0
64.00	835.0
65.00	953.0
67.00	376.0
68.00	10049.0
69.00	10581.0
69.90	914.0
72.00	572.0
73.00	4269.0
74.00	17472.0
75.00	48912.0
76.00	4210.0
77.00	564.0
77.80	491.0
78.90	4078.0
79.90	1130.0
80.90	3832.0
81.80	1021.0
83.00	130.0
86.10	112.0
87.00	4434.0
87.90	4081.0
90.90	543.0
92.00	2989.0
92.90	4664.0
94.00	12069.0
95.00	99184.0
96.00	6592.0
97.00	175.0
103.90	629.0
104.90	111.0
105.80	507.0
106.70	131.0
108.10	137.0
109.80	117.0
111.70	142.0
113.00	170.0
114.90	121.0
115.80	362.0
116.80	522.0
117.80	448.0
119.00	680.0
128.00	403.0
129.00	246.0
129.90	424.0
130.90	124.0
134.80	228.0
136.90	210.0
140.90	1204.0
141.90	145.0
142.80	1487.0
144.00	142.0
144.80	461.0
145.70	158.0
147.00	107.0
147.90	215.0
149.70	114.0
154.80	338.0
156.70	147.0
170.10	114.0
171.00	336.0
172.00	1131.0
172.90	1227.0
173.90	81112.0
175.00	6123.0
175.90	79904.0
177.00	4945.0
177.90	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383

m/z	Abundance
36.00	849.0
37.00	3929.0
38.00	3570.0
39.00	1463.0
39.90	316.0
43.90	1099.0
44.90	833.0
45.90	215.0
47.00	844.0
47.90	473.0
49.00	3555.0
50.00	16161.0
51.00	5094.0
52.00	223.0
52.90	104.0
55.10	216.0
56.00	1423.0
57.00	2475.0
57.90	108.0
58.30	135.0
60.00	1293.0
61.00	4472.0
62.00	4679.0
63.00	3996.0
64.00	764.0
65.00	1024.0
67.00	396.0
68.00	9521.0
69.00	10112.0
69.90	786.0
70.90	106.0
72.00	564.0
73.00	4168.0
74.00	16592.0
75.00	46960.0
76.00	4120.0
77.00	525.0
77.80	381.0
78.90	4190.0
80.00	1072.0
80.90	3726.0
81.80	1101.0
82.90	173.0
86.00	128.0
87.00	4381.0
87.90	4027.0
90.90	441.0
92.00	3004.0
92.90	4545.0
94.00	11954.0
95.00	98192.0
96.00	6272.0
97.00	130.0
103.90	646.0
104.90	120.0
105.80	428.0
108.10	155.0
111.70	136.0
113.00	146.0
114.90	126.0
115.80	355.0
116.80	529.0
117.80	420.0
119.00	606.0
128.00	406.0
128.90	232.0
130.00	544.0
130.90	137.0
134.80	268.0
136.80	215.0
140.80	1149.0
141.90	116.0
142.90	1468.0
145.00	449.0
145.70	185.0
147.90	249.0
152.00	108.0
154.80	263.0
156.70	127.0
170.10	103.0
171.10	264.0
172.00	1216.0
173.90	81144.0
175.00	6260.0
175.90	80280.0
177.00	4800.0
177.90	141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB383