

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037697.D
 Acq On : 01 Oct 2024 12:58
 Operator : SY/MD
 Sample : P4183-19ME
 Misc : 4.80G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EM5ME

Quant Time: Oct 02 04:39:21 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 01 04:32:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	696761	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	665418	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	325766	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	229216	37.475	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	74.960%
7) Chloroethane-d5	1.510	69	112825	23.764	ug/L	-0.02
Spiked Amount	50.000	Range	70 - 130	Recovery	=	47.520%#
11) 1,1-Dichloroethene-d2	2.044	65	103105	40.348	ug/L	-0.02
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.700%
21) 2-Butanone-d5	3.799	46	144618	66.382	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	66.380%
24) Chloroform-d	4.240	84	412628	37.919	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	75.840%
26) 1,2-Dichloroethane-d4	4.934	65	264172	41.475	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.940%
32) Benzene-d6	4.947	84	868849	41.727	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	83.460%
36) 1,2-Dichloropropane-d6	5.982	67	276188	41.655	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	83.300%
41) Toluene-d8	7.236	98	765825	40.561	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.120%
43) trans-1,3-Dichloroprop...	7.548	79	119851	38.911	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	77.820%
47) 2-Hexanone-d5	8.031	63	116716	83.364	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.360%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	305286	39.627	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	79.260%
66) 1,2-Dichlorobenzene-d4	11.555	152	293695	42.784	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	85.560%
Target Compounds					Qvalue	
15) Methyl Acetate	2.375	43	7625	2.046	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037697.D
Acq On : 01 Oct 2024 12:58
Operator : SY/MD
Sample : P4183-19ME
Misc : 4.80G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EM5ME


Quant Time: Oct 02 04:39:21 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 01 04:32:07 2024
Response via : Initial Calibration

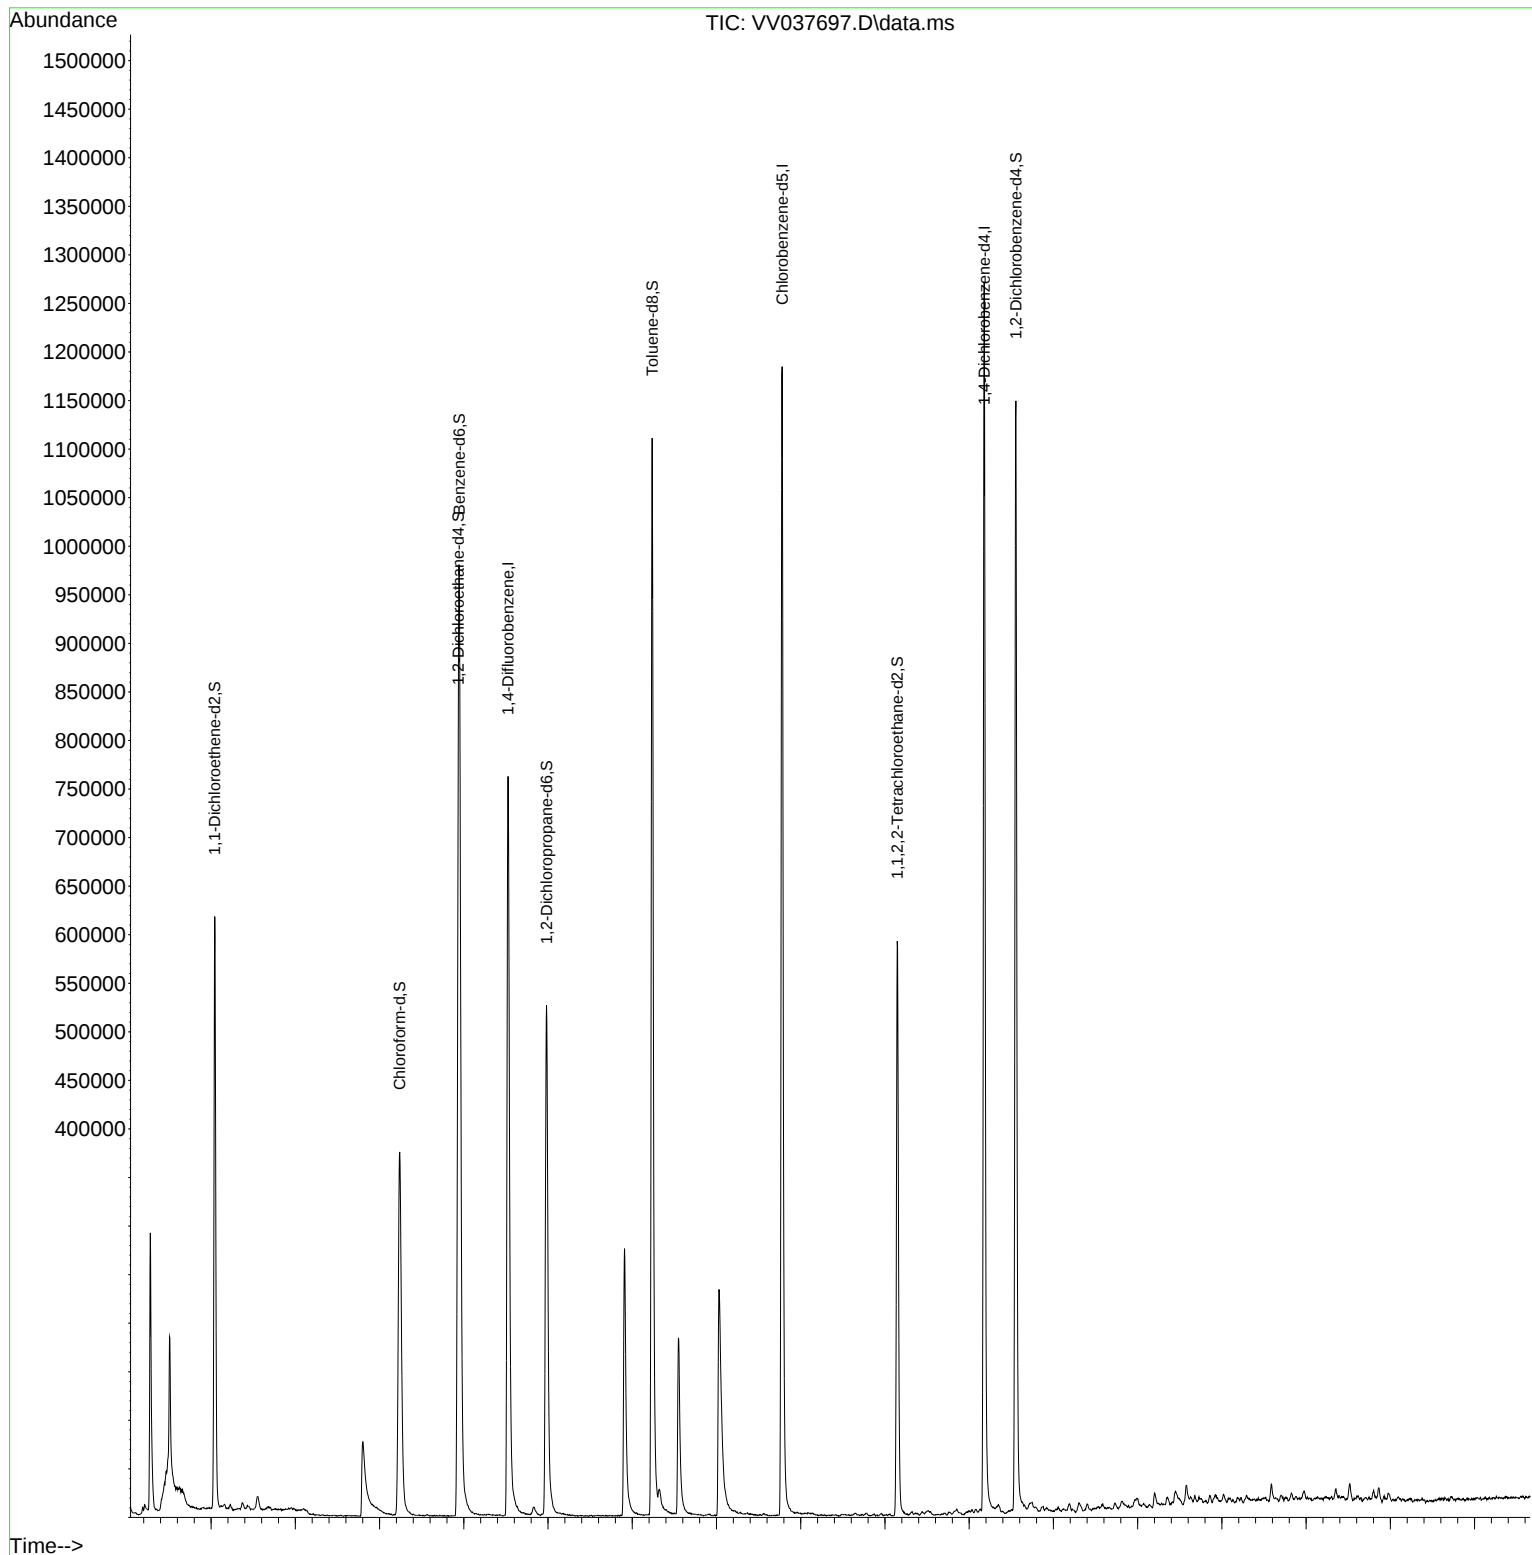

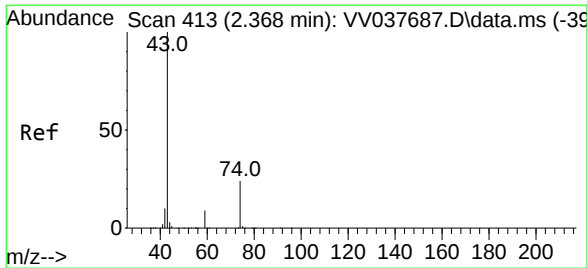

#15
Methyl Acetate
Concen: 2.046 ug/L
RT: 2.375 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV037697.D
Acq: 01 Oct 2024 12:58

Instrument :
MSVOA_V
ClientSampleId :
A4EM5ME

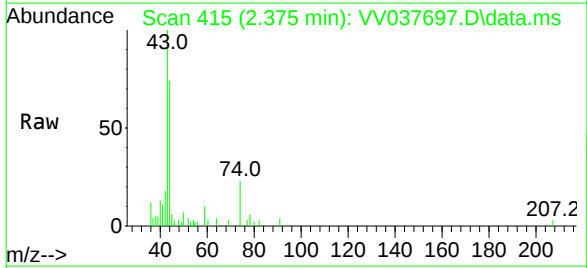

Tgt Ion: 43 Resp: 7625
Ion Ratio Lower Upper
43 100
74 27.2 19.4 29.0

