

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037702.D
 Acq On : 01 Oct 2024 14:56
 Operator : SY/MD
 Sample : P4238-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD1

Quant Time: Oct 02 04:39:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 01 04:32:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	622231	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	610021	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	286109	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	176334	32.283	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	64.560%		
7) Chloroethane-d5	1.532	69	165771	39.099	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	78.200%		
11) 1,1-Dichloroethene-d2	2.059	65	84565	37.057	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	74.120%		
21) 2-Butanone-d5	3.793	46	206089	105.929	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	105.930%		
24) Chloroform-d	4.243	84	450864	46.395	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.800%		
26) 1,2-Dichloroethane-d4	4.937	65	285040	50.111	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.220%		
32) Benzene-d6	4.953	84	846011	44.320	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.640%		
36) 1,2-Dichloropropane-d6	5.985	67	289228	47.583	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.160%		
41) Toluene-d8	7.239	98	751907	43.440	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.880%		
43) trans-1,3-Dichloroprop...	7.551	79	125661	44.503	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.000%		
47) 2-Hexanone-d5	8.024	63	121806	94.900	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	94.900%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	345415	48.907	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	97.820%		
66) 1,2-Dichlorobenzene-d4	11.554	152	317941	52.736	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.480%		
Target Compounds					Qvalue	
13) Acetone	2.114	43	24857	13.033	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037702.D
Acq On : 01 Oct 2024 14:56
Operator : SY/MD
Sample : P4238-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD1

Quant Time: Oct 02 04:39:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 01 04:32:07 2024
Response via : Initial Calibration

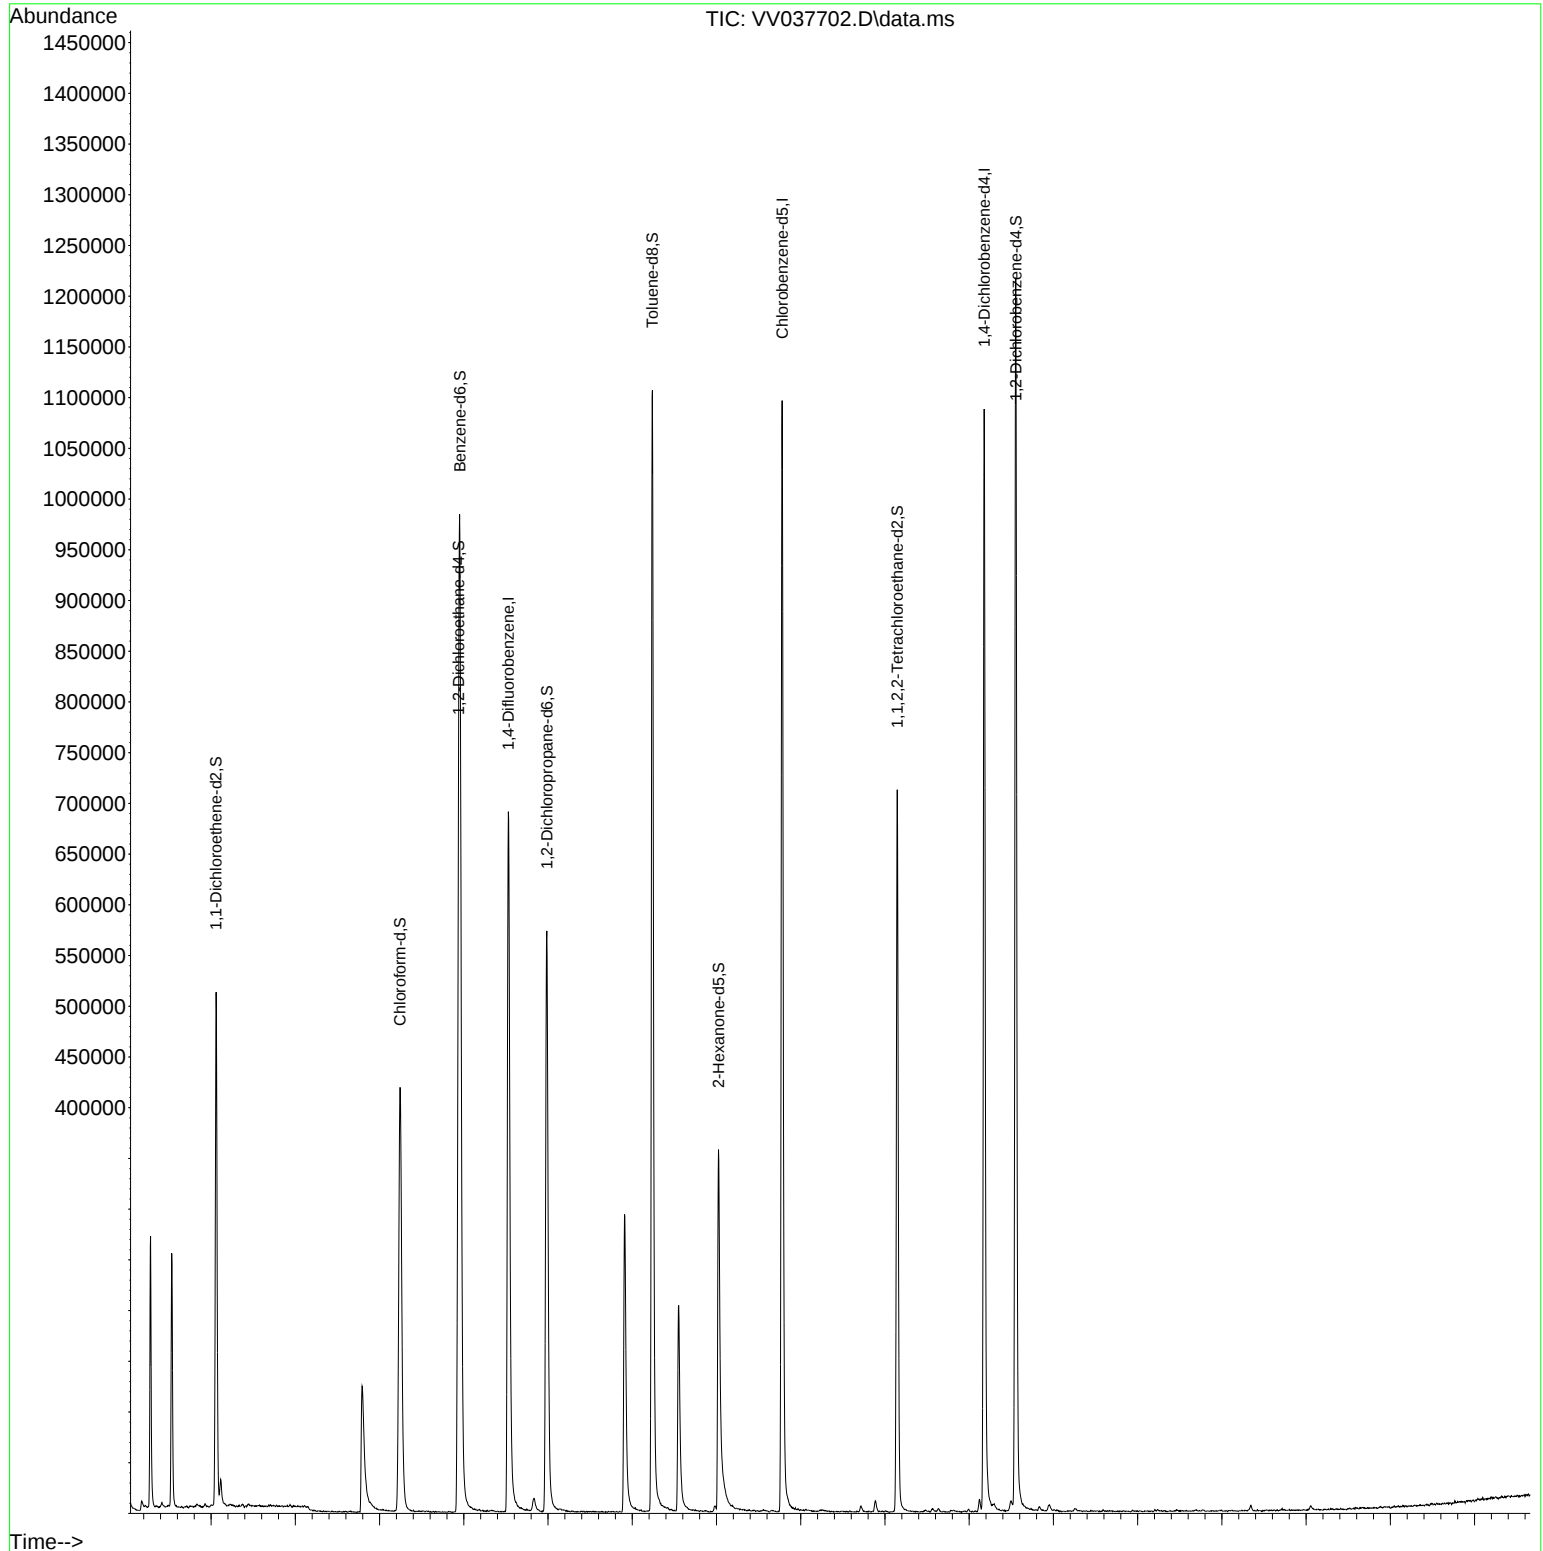

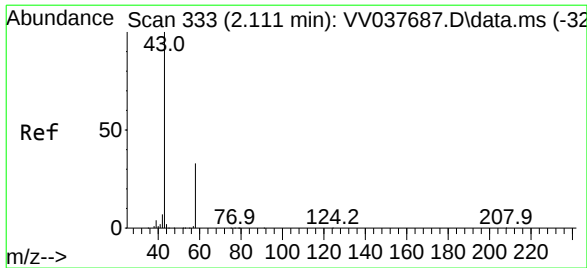

#13
 Acetone
 Concen: 13.033 ug/L
 RT: 2.114 min Scan# 33
 Delta R.T. 0.003 min
 Lab File: VV037702.D
 Acq: 01 Oct 2024 14:56

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD1

Tgt Ion: 43 Resp: 24857
 Ion Ratio Lower Upper
 43 100
 58 35.6 0.0 66.6

