

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037689.D
 Acq On : 01 Oct 2024 09:50
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037689.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV	8141	14127	0.55%	0.074%
2	1.281	68	75	92	rVB	368144	397687	15.47%	2.090%
3	1.532	146	153	168	rVB	302128	357773	13.92%	1.881%
4	2.059	307	317	338	rBV	635705	930238	36.19%	4.889%
5	3.513	766	769	773	rVB5	815	448	0.02%	0.002%
6	3.577	786	789	793	rBV2	704	667	0.03%	0.004%
7	3.641	804	809	811	rBV2	490	434	0.02%	0.002%
8	3.661	813	815	820	rVB3	643	546	0.02%	0.003%
9	3.793	848	856	886	rBV	100982	299060	11.63%	1.572%
10	4.047	932	935	937	rBV3	953	715	0.03%	0.004%
11	4.101	949	952	954	rBV4	726	434	0.02%	0.002%
12	4.169	971	973	975	rBV3	984	505	0.02%	0.003%
13	4.243	979	996	1027	rBV	401856	1045142	40.66%	5.493%
14	4.391	1040	1042	1045	rBV3	747	522	0.02%	0.003%
15	4.487	1068	1072	1074	rBV4	849	654	0.03%	0.003%
16	4.821	1170	1176	1178	rBV5	754	766	0.03%	0.004%
17	4.838	1178	1181	1183	rVB3	1292	659	0.03%	0.003%
18	4.950	1200	1216	1249	rBV2	1003533	2570446	100.00%	13.511%
19	5.162	1280	1282	1286	rVB6	1474	805	0.03%	0.004%
20	5.307	1323	1327	1331	rBV5	954	759	0.03%	0.004%
21	5.346	1337	1339	1344	rVB4	1419	995	0.04%	0.005%
22	5.400	1353	1356	1360	rVB3	728	465	0.02%	0.002%
23	5.529	1382	1396	1431	rBV	794829	1639659	63.79%	8.618%
24	5.831	1481	1490	1503	rBV10	8807	21787	0.85%	0.115%
25	5.985	1524	1538	1570	rBV	558085	1161089	45.17%	6.103%
26	6.509	1698	1701	1705	rVB4	952	630	0.02%	0.003%
27	6.587	1722	1725	1729	rVB4	756	605	0.02%	0.003%
28	6.741	1769	1773	1774	rBV3	931	622	0.02%	0.003%
29	6.809	1791	1794	1798	rVB4	619	446	0.02%	0.002%
30	6.908	1814	1825	1859	rBV	292013	574885	22.37%	3.022%
31	7.175	1905	1908	1910	rBV4	953	452	0.02%	0.002%
32	7.236	1916	1927	1966	rBV	1179740	2085389	81.13%	10.961%
33	7.548	2011	2024	2054	rBV	192002	370423	14.41%	1.947%
34	7.908	2132	2136	2142	rVB7	900	1030	0.04%	0.005%
35	8.024	2163	2172	2216	rBV2	303067	676250	26.31%	3.554%
36	8.493	2315	2318	2322	rBV4	950	818	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037689.D
 Acq On : 01 Oct 2024 09:50
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	8.558	2332	2338	2343	rBV6	1194	1392	0.05%	0.007%
38	8.638	2359	2363	2368	rVB6	925	962	0.04%	0.005%
39	8.696	2378	2381	2385	rVB5	610	513	0.02%	0.003%
40	8.776	2395	2406	2445	rBV	1218340	2038678	79.31%	10.716%
41	9.159	2522	2525	2530	rVB5	895	625	0.02%	0.003%
42	9.281	2560	2563	2567	rVV4	974	837	0.03%	0.004%
43	9.304	2567	2570	2571	rVV2	947	434	0.02%	0.002%
44	9.355	2582	2586	2589	rVV4	1029	806	0.03%	0.004%
45	9.461	2614	2619	2622	rBV4	901	829	0.03%	0.004%
46	9.484	2622	2626	2627	rBV2	1103	580	0.02%	0.003%
47	9.593	2656	2660	2667	rBV6	739	822	0.03%	0.004%
48	9.683	2685	2688	2691	rVB4	924	583	0.02%	0.003%
49	9.734	2699	2704	2706	rBV3	507	458	0.02%	0.002%
50	9.776	2712	2717	2723	rVB6	829	776	0.03%	0.004%
51	9.834	2730	2735	2738	rBV5	781	574	0.02%	0.003%
52	9.869	2742	2746	2748	rBV4	1197	822	0.03%	0.004%
53	10.030	2791	2796	2798	rBV2	1036	853	0.03%	0.004%
54	10.082	2809	2812	2815	rBV4	699	499	0.02%	0.003%
55	10.146	2820	2832	2859	rBV	611393	978984	38.09%	5.146%
56	10.291	2875	2877	2881	rBV4	598	428	0.02%	0.002%
57	10.381	2901	2905	2911	rBV4	982	942	0.04%	0.005%
58	10.451	2924	2927	2930	rBV3	685	494	0.02%	0.003%
59	10.474	2930	2934	2935	rBV	1118	565	0.02%	0.003%
60	10.660	2990	2992	2996	rVV2	593	498	0.02%	0.003%
61	10.866	3051	3056	3058	rBV4	1321	1286	0.05%	0.007%
62	10.895	3064	3065	3071	rVB4	952	628	0.02%	0.003%
63	10.995	3092	3096	3101	rVB3	948	879	0.03%	0.005%
64	11.053	3109	3114	3120	rBV3	963	1135	0.04%	0.006%
65	11.130	3130	3138	3142	rBV7	2792	3669	0.14%	0.019%
66	11.178	3142	3153	3187	rBV	1200844	1929249	75.06%	10.140%
67	11.551	3258	3269	3297	rBV	1133569	1832357	71.29%	9.631%
68	11.863	3364	3366	3369	rBV3	814	581	0.02%	0.003%
69	12.021	3413	3415	3417	rBV3	796	452	0.02%	0.002%
70	12.037	3417	3420	3425	rVV5	1098	1010	0.04%	0.005%
71	12.059	3425	3427	3430	rVV2	870	577	0.02%	0.003%
72	12.075	3430	3432	3438	rVV5	839	687	0.03%	0.004%
73	12.204	3469	3472	3477	rBV6	899	611	0.02%	0.003%
74	12.278	3492	3495	3498	rBV4	896	540	0.02%	0.003%
75	12.368	3518	3523	3525	rBV3	836	662	0.03%	0.003%
76	12.451	3545	3549	3551	rBV2	988	734	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037689.D
 Acq On : 01 Oct 2024 09:50
 Operator : SY/MD
 Sample : VV1001WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK225

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.496	3560	3563	3568	rVB5	1080	857	0.03%	0.005%
78	12.590	3584	3592	3596	rBV8	3082	4638	0.18%	0.024%
79	12.683	3618	3621	3626	rVB2	754	541	0.02%	0.003%
80	12.757	3641	3644	3646	rBV2	690	424	0.02%	0.002%
81	12.966	3706	3709	3712	rBV3	943	567	0.02%	0.003%
82	13.011	3720	3723	3726	rBV3	640	553	0.02%	0.003%
83	13.101	3747	3751	3754	rBV3	551	470	0.02%	0.002%
84	13.210	3776	3785	3797	rVV8	5162	10910	0.42%	0.057%
85	13.316	3816	3818	3822	rBV2	670	461	0.02%	0.002%
86	13.390	3838	3841	3843	rBV2	657	445	0.02%	0.002%
87	13.448	3848	3859	3870	rBV2	10398	21001	0.82%	0.110%
88	13.680	3925	3931	3942	rVV8	6263	10006	0.39%	0.053%
89	14.088	4055	4058	4060	rBV4	774	447	0.02%	0.002%
90	14.175	4082	4085	4090	rVB3	905	633	0.02%	0.003%
91	14.201	4090	4093	4095	rBV	843	583	0.02%	0.003%
92	14.307	4122	4126	4129	rBV4	1051	935	0.04%	0.005%
93	14.374	4144	4147	4149	rBV3	1057	732	0.03%	0.004%
94	14.512	4185	4190	4193	rBV5	941	948	0.04%	0.005%
95	14.593	4212	4215	4220	rBV4	937	877	0.03%	0.005%
96	14.709	4248	4251	4252	rBV2	982	601	0.02%	0.003%
97	14.815	4280	4284	4287	rBV5	810	661	0.03%	0.003%
98	14.879	4300	4304	4307	rBV5	910	871	0.03%	0.005%
99	15.155	4388	4390	4394	rVB4	1095	578	0.02%	0.003%
100	15.390	4461	4463	4467	rBV4	1151	634	0.02%	0.003%

Sum of corrected areas: 19025316




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037689.D
Acq On : 01 Oct 2024 09:50
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

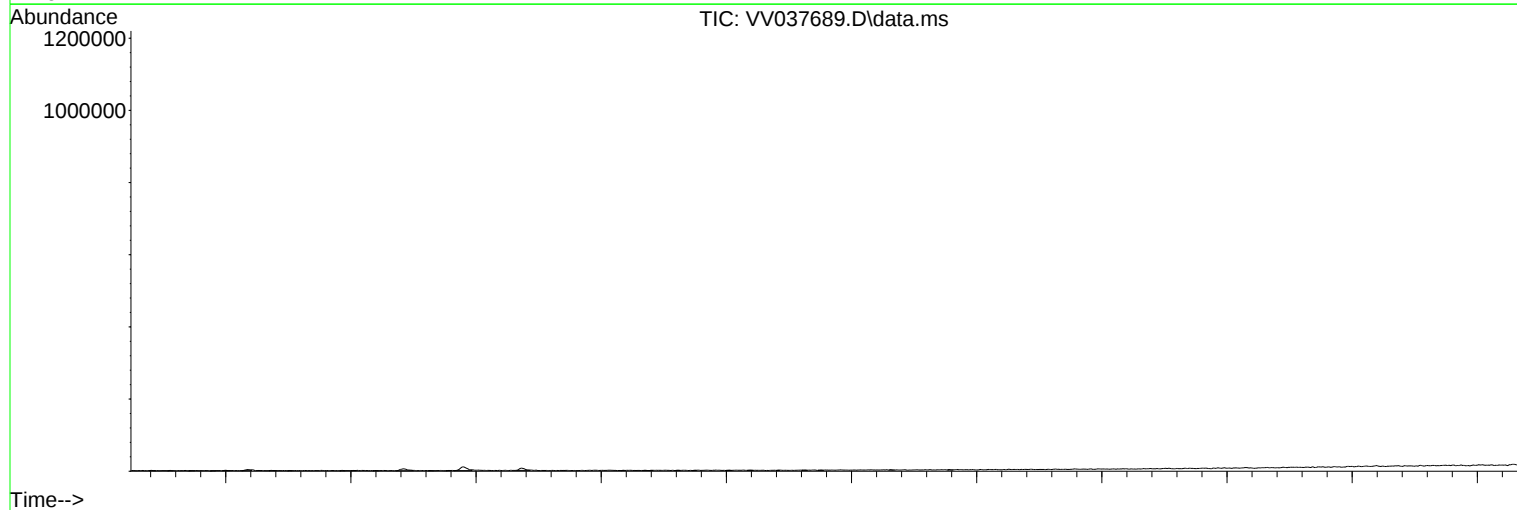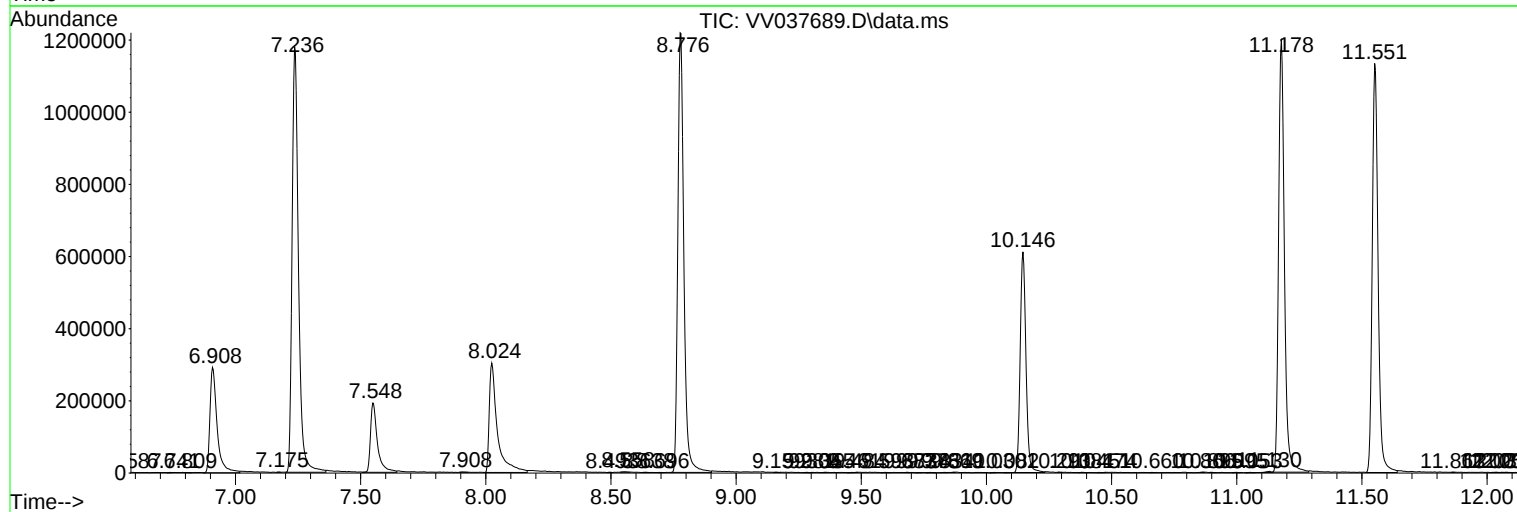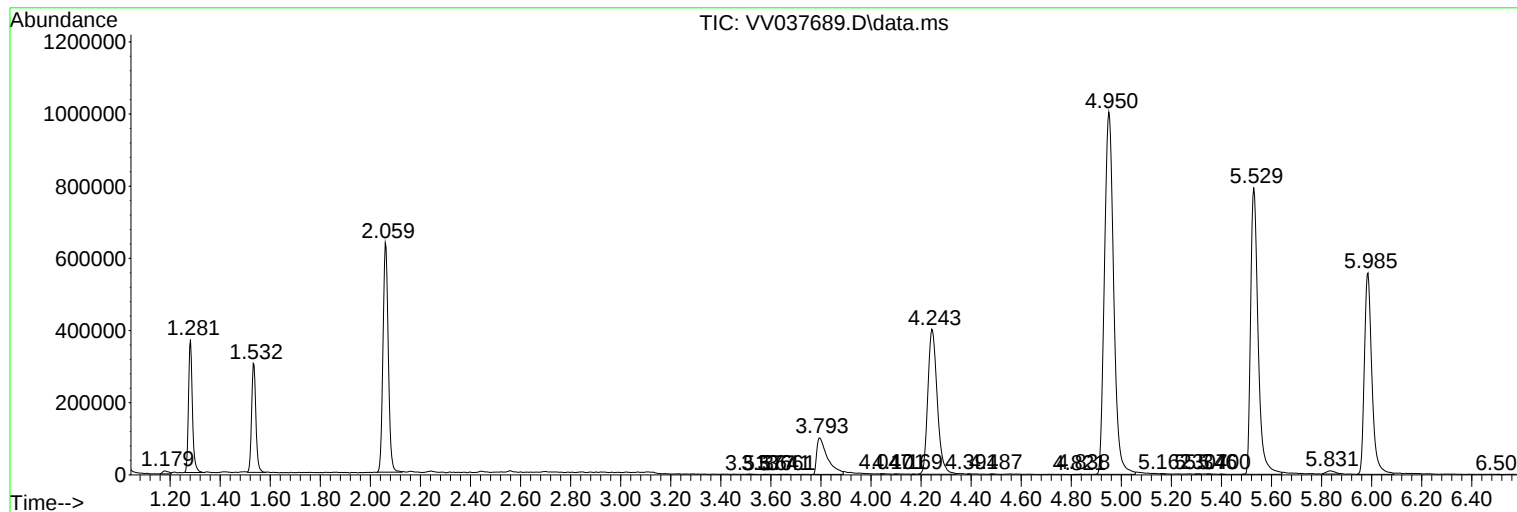

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037689.D
Acq On : 01 Oct 2024 09:50
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037689.D
Acq On : 01 Oct 2024 09:50
Operator : SY/MD
Sample : VV1001WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK225

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc