

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037690.D
 Acq On : 01 Oct 2024 10:28
 Operator : SY/MD
 Sample : P4185-21DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	52	rBV	9722	17421	0.67%	0.081%
2	1.282	67	75	93	rVB2	441780	490351	18.84%	2.290%
3	1.532	145	153	166	rBV	312333	401629	15.43%	1.876%
4	2.060	307	317	341	rVB	654746	949652	36.48%	4.436%
5	2.690	506	513	526	rVB2	23555	40756	1.57%	0.190%
6	3.105	628	642	667	rVB	296777	625063	24.01%	2.920%
7	3.674	815	819	824	rBV3	618	781	0.03%	0.004%
8	3.802	841	859	896	rBV2	560114	1477441	56.76%	6.901%
9	4.137	960	963	966	rBV3	789	492	0.02%	0.002%
10	4.156	966	969	970	rBV2	625	446	0.02%	0.002%
11	4.240	979	995	1023	rVV	409384	1051533	40.40%	4.911%
12	4.507	1064	1078	1094	rVB3	17699	45384	1.74%	0.212%
13	4.780	1161	1163	1165	rBV3	705	450	0.02%	0.002%
14	4.857	1182	1187	1192	rBV4	584	714	0.03%	0.003%
15	4.947	1199	1215	1245	rBV2	1014393	2603004	100.00%	12.158%
16	5.333	1333	1335	1337	rBV3	876	531	0.02%	0.002%
17	5.388	1349	1352	1354	rBV2	1044	682	0.03%	0.003%
18	5.526	1384	1395	1427	rBV	836569	1711568	65.75%	7.994%
19	5.786	1473	1476	1478	rBV4	1485	1003	0.04%	0.005%
20	5.834	1480	1491	1513	rVB5	40529	98274	3.78%	0.459%
21	5.979	1523	1536	1567	rBV	563667	1177984	45.25%	5.502%
22	6.368	1654	1657	1661	rVB4	1347	901	0.03%	0.004%
23	6.387	1661	1663	1665	rBV3	733	434	0.02%	0.002%
24	6.400	1665	1667	1670	rVV3	1149	719	0.03%	0.003%
25	6.439	1673	1679	1684	rBV5	691	749	0.03%	0.003%
26	6.481	1687	1692	1697	rVB5	1014	996	0.04%	0.005%
27	6.523	1697	1705	1708	rBV5	857	883	0.03%	0.004%
28	6.548	1710	1713	1716	rBV3	886	461	0.02%	0.002%
29	6.568	1716	1719	1722	rBV3	699	522	0.02%	0.002%
30	6.606	1727	1731	1734	rBV4	578	620	0.02%	0.003%
31	6.751	1773	1776	1778	rBV	926	473	0.02%	0.002%
32	6.825	1795	1799	1801	rBV3	568	423	0.02%	0.002%
33	6.905	1812	1824	1852	rBV	298464	571971	21.97%	2.672%
34	7.153	1899	1901	1905	rBV4	529	443	0.02%	0.002%
35	7.172	1905	1907	1910	rVV4	754	485	0.02%	0.002%
36	7.236	1916	1927	1966	rBV	1177746	2099289	80.65%	9.805%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037690.D
 Acq On : 01 Oct 2024 10:28
 Operator : SY/MD
 Sample : P4185-21DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.548	2014	2024	2049	rBV	195291	365783	14.05%	1.708%
38	7.728	2078	2080	2082	rBV3	1060	495	0.02%	0.002%
39	7.905	2125	2135	2154	rBV3	22430	41698	1.60%	0.195%
40	8.021	2163	2171	2218	rBV2	277875	640292	24.60%	2.991%
41	8.535	2328	2331	2333	rBV3	1248	851	0.03%	0.004%
42	8.699	2377	2382	2384	rBV4	676	447	0.02%	0.002%
43	8.719	2384	2388	2392	rBV3	663	565	0.02%	0.003%
44	8.776	2395	2406	2448	rBV	1271211	2125109	81.64%	9.926%
45	9.159	2522	2525	2526	rBV2	992	517	0.02%	0.002%
46	9.169	2526	2528	2532	rVB4	947	535	0.02%	0.002%
47	9.265	2554	2558	2559	rBV2	672	421	0.02%	0.002%
48	9.329	2575	2578	2581	rBV4	503	440	0.02%	0.002%
49	9.474	2619	2623	2625	rBV3	780	449	0.02%	0.002%
50	9.497	2628	2630	2634	rVV4	826	595	0.02%	0.003%
51	9.561	2647	2650	2657	rVB5	1017	978	0.04%	0.005%
52	9.638	2668	2674	2678	rBV5	1276	1329	0.05%	0.006%
53	9.789	2717	2721	2725	rVB3	688	616	0.02%	0.003%
54	9.828	2730	2733	2736	rBV4	740	696	0.03%	0.003%
55	9.886	2749	2751	2754	rVB3	748	443	0.02%	0.002%
56	9.944	2767	2769	2773	rVB4	953	604	0.02%	0.003%
57	9.969	2773	2777	2779	rBV3	619	478	0.02%	0.002%
58	10.146	2813	2832	2858	rBV	603287	969154	37.23%	4.527%
59	10.323	2884	2887	2890	rVB3	795	484	0.02%	0.002%
60	10.487	2933	2938	2943	rBV5	681	649	0.02%	0.003%
61	10.751	3015	3020	3026	rVB7	800	753	0.03%	0.004%
62	10.863	3050	3055	3059	rVV6	804	854	0.03%	0.004%
63	11.034	3103	3108	3111	rBV3	659	671	0.03%	0.003%
64	11.130	3131	3138	3142	rBV7	2048	3130	0.12%	0.015%
65	11.178	3142	3153	3185	rVV	1237243	1997266	76.73%	9.329%
66	11.423	3227	3229	3231	rBV2	795	480	0.02%	0.002%
67	11.490	3248	3250	3253	rBV2	601	418	0.02%	0.002%
68	11.551	3257	3269	3302	rBV	1137045	1833829	70.45%	8.565%
69	11.802	3345	3347	3352	rVB4	844	575	0.02%	0.003%
70	11.927	3383	3386	3388	rVB3	787	442	0.02%	0.002%
71	11.940	3388	3390	3393	rBV3	972	525	0.02%	0.002%
72	11.989	3402	3405	3409	rVB3	790	583	0.02%	0.003%
73	12.021	3409	3415	3419	rBV6	1414	1654	0.06%	0.008%
74	12.040	3419	3421	3425	rVB3	936	580	0.02%	0.003%
75	12.063	3425	3428	3433	rBV3	677	533	0.02%	0.002%
76	12.172	3459	3462	3465	rBV3	1139	743	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037690.D
 Acq On : 01 Oct 2024 10:28
 Operator : SY/MD
 Sample : P4185-21DL 20X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY074DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.239	3478	3483	3487	rVB3	594	673	0.03%	0.003%
78	12.397	3527	3532	3534	rBV3	904	511	0.02%	0.002%
79	12.599	3584	3595	3607	rVB10	2161	5039	0.19%	0.024%
80	12.738	3635	3638	3641	rBV3	550	441	0.02%	0.002%
81	12.947	3697	3703	3709	rBV7	681	884	0.03%	0.004%
82	13.159	3766	3769	3771	rBV3	607	440	0.02%	0.002%
83	13.210	3776	3785	3790	rBV7	3430	4805	0.18%	0.022%
84	13.259	3799	3800	3807	rVB4	798	491	0.02%	0.002%
85	13.455	3851	3861	3866	rBV3	5714	9254	0.36%	0.043%
86	13.680	3925	3931	3942	rBV9	3166	6006	0.23%	0.028%
87	13.722	3942	3944	3947	rVV4	858	532	0.02%	0.002%
88	13.860	3982	3987	3990	rBV4	880	892	0.03%	0.004%
89	13.931	4006	4009	4012	rVB5	1380	782	0.03%	0.004%
90	13.972	4019	4022	4027	rVV3	881	728	0.03%	0.003%
91	14.037	4039	4042	4045	rVB3	789	565	0.02%	0.003%
92	14.075	4049	4054	4057	rBV4	612	688	0.03%	0.003%
93	14.159	4078	4080	4084	rBV4	896	693	0.03%	0.003%
94	14.365	4141	4144	4147	rVB3	1183	736	0.03%	0.003%
95	14.429	4160	4164	4166	rBV3	854	697	0.03%	0.003%
96	14.570	4204	4208	4210	rBV3	1068	744	0.03%	0.003%
97	14.606	4217	4219	4225	rVB5	902	677	0.03%	0.003%
98	14.632	4225	4227	4231	rBV2	799	652	0.03%	0.003%
99	15.152	4387	4389	4390	rBV2	997	484	0.02%	0.002%
100	15.631	4535	4538	4542	rBV4	1563	1171	0.04%	0.005%

Sum of corrected areas: 21409777




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037690.D
Acq On : 01 Oct 2024 10:28
Operator : SY/MD
Sample : P4185-21DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

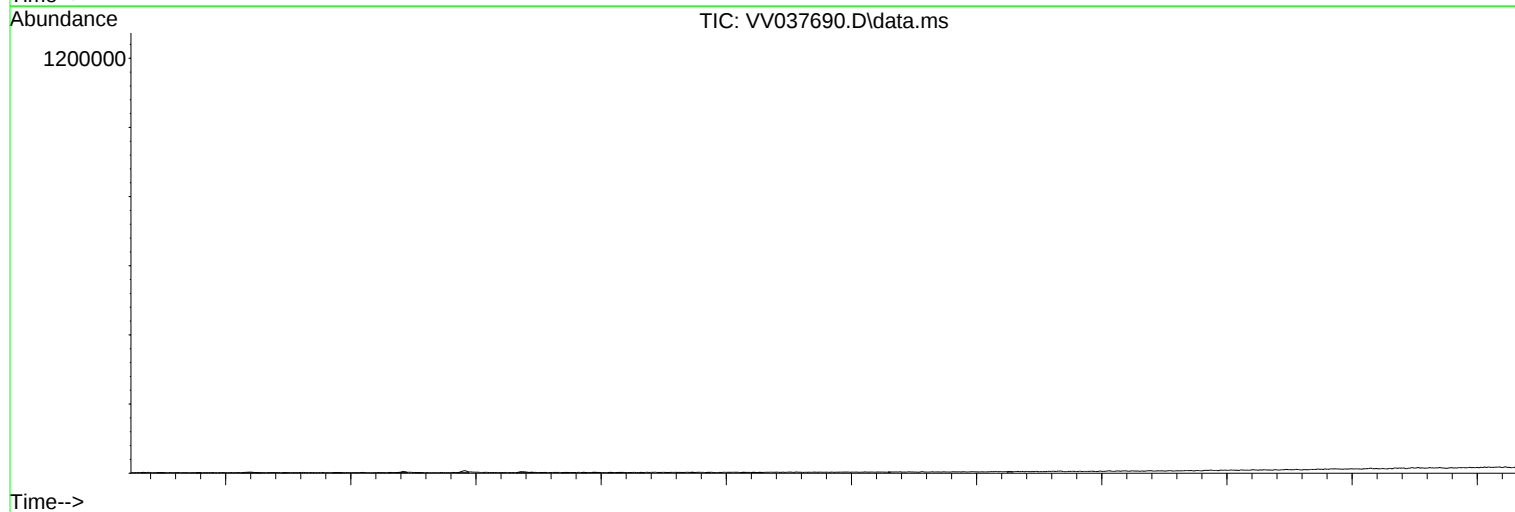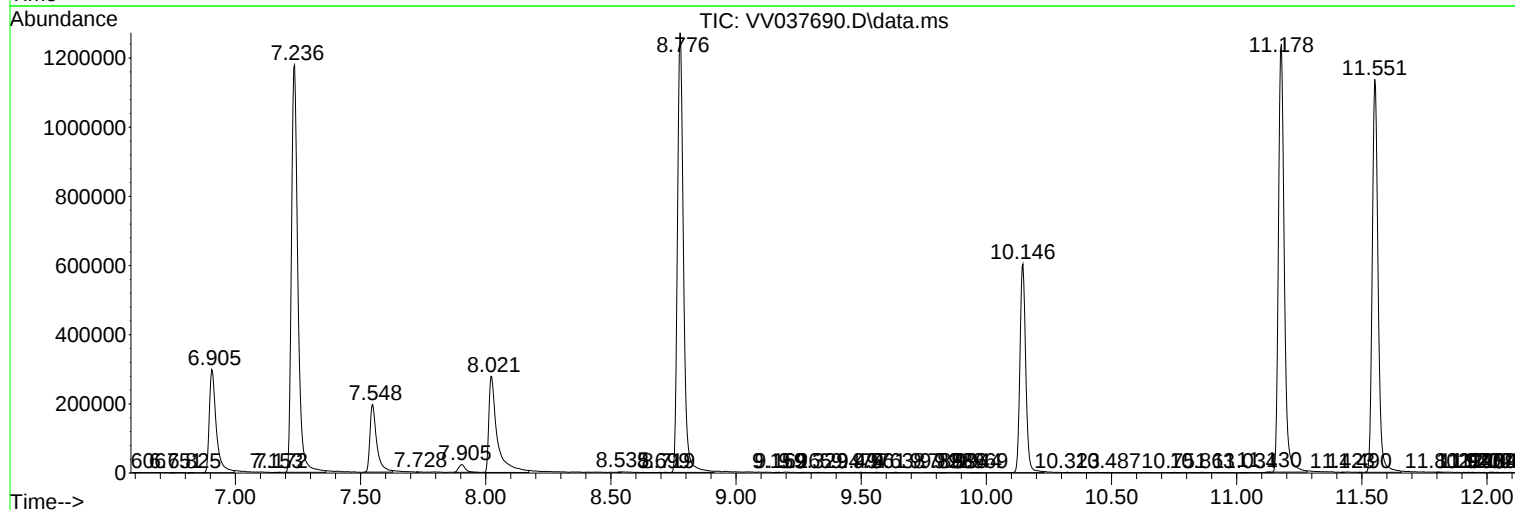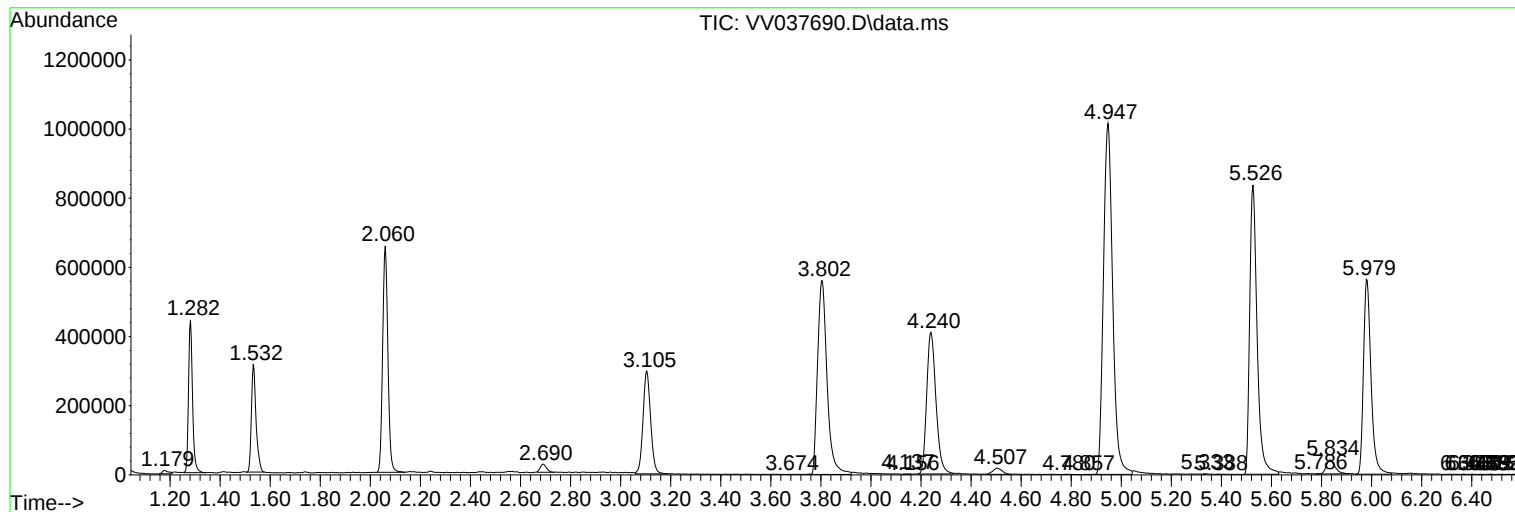

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037690.D
Acq On : 01 Oct 2024 10:28
Operator : SY/MD
Sample : P4185-21DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037690.D
Acq On : 01 Oct 2024 10:28
Operator : SY/MD
Sample : P4185-21DL 20X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY074DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------