

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037691.D
 Acq On : 01 Oct 2024 10:49
 Operator : SY/MD
 Sample : P4185-06DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY028DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037691.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	385483	416774	15.68%	2.108%
2	1.532	146	153	169	rVB	308589	378543	14.24%	1.915%
3	2.060	308	317	332	rVB	661084	950979	35.77%	4.810%
4	3.568	784	786	787	rVB2	518	188	0.01%	0.001%
5	3.577	787	789	791	rBV2	491	312	0.01%	0.002%
6	3.632	803	806	809	rBV4	553	370	0.01%	0.002%
7	3.658	812	814	816	rVV2	702	343	0.01%	0.002%
8	3.687	820	823	826	rVB3	711	460	0.02%	0.002%
9	3.699	826	827	830	rVB	411	151	0.01%	0.001%
10	3.719	830	833	836	rBV4	768	531	0.02%	0.003%
11	3.735	836	838	839	rVB	179	65	0.00%	0.000%
12	3.806	847	860	890	rBV3	356767	991207	37.28%	5.014%
13	4.243	981	996	1028	rBV	422055	1072727	40.35%	5.426%
14	4.507	1066	1078	1106	rVB3	97824	255076	9.59%	1.290%
15	4.712	1139	1142	1143	rBV2	607	341	0.01%	0.002%
16	4.809	1168	1172	1175	rBV3	620	411	0.02%	0.002%
17	4.825	1175	1177	1181	rVV4	636	453	0.02%	0.002%
18	4.950	1200	1216	1261	rBV2	1042534	2658751	100.00%	13.449%
19	5.490	1381	1384	1385	rBV2	1012	602	0.02%	0.003%
20	5.529	1385	1396	1426	rVV	731661	1491109	56.08%	7.543%
21	5.982	1525	1537	1567	rBV	572143	1200077	45.14%	6.071%
22	6.352	1649	1652	1656	rVB5	679	341	0.01%	0.002%
23	6.452	1681	1683	1687	rVB4	743	422	0.02%	0.002%
24	6.471	1687	1689	1691	rBV3	452	171	0.01%	0.001%
25	6.484	1691	1693	1695	rBV2	545	323	0.01%	0.002%
26	6.516	1701	1703	1706	rBV	706	465	0.02%	0.002%
27	6.551	1711	1714	1716	rVB4	673	372	0.01%	0.002%
28	6.596	1727	1728	1729	rBV4	563	207	0.01%	0.001%
29	6.625	1734	1737	1742	rBV4	591	511	0.02%	0.003%
30	6.645	1742	1743	1745	rBV2	197	91	0.00%	0.000%
31	6.658	1745	1747	1753	rBV3	359	309	0.01%	0.002%
32	6.690	1753	1757	1758	rBV2	556	413	0.02%	0.002%
33	6.712	1763	1764	1765	rVB	267	52	0.00%	0.000%
34	6.722	1765	1767	1770	rVB3	990	503	0.02%	0.003%
35	6.738	1770	1772	1775	rBV2	899	602	0.02%	0.003%
36	6.844	1800	1805	1808	rBV5	1085	900	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037691.D
 Acq On : 01 Oct 2024 10:49
 Operator : SY/MD
 Sample : P4185-06DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY028DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.860	1808	1810	1813	rBV3	393	312	0.01%	0.002%
38	6.908	1813	1825	1862	rBV	301596	590619	22.21%	2.988%
39	7.236	1917	1927	1952	rBV	1199292	2113813	79.50%	10.693%
40	7.548	2016	2024	2055	rBV	196457	374248	14.08%	1.893%
41	7.902	2128	2134	2135	rBV4	5162	4554	0.17%	0.023%
42	8.024	2164	2172	2206	rBV2	311229	674817	25.38%	3.414%
43	8.468	2306	2310	2315	rBV6	1036	1317	0.05%	0.007%
44	8.780	2395	2407	2443	rBV	1111991	1872353	70.42%	9.471%
45	9.326	2574	2577	2583	rBV5	621	730	0.03%	0.004%
46	9.413	2602	2604	2607	rVB3	653	289	0.01%	0.001%
47	9.429	2607	2609	2610	rBV	396	136	0.01%	0.001%
48	9.439	2610	2612	2615	rVB3	570	261	0.01%	0.001%
49	9.484	2618	2626	2635	rBV5	8739	14850	0.56%	0.075%
50	9.571	2651	2653	2657	rVB3	786	668	0.03%	0.003%
51	9.590	2657	2659	2662	rBV2	543	423	0.02%	0.002%
52	9.609	2663	2665	2668	rVV4	901	500	0.02%	0.003%
53	9.696	2690	2692	2696	rVB4	732	374	0.01%	0.002%
54	9.719	2696	2699	2700	rBV2	500	244	0.01%	0.001%
55	9.741	2704	2706	2707	rBV2	374	182	0.01%	0.001%
56	9.754	2709	2710	2713	rBV2	650	200	0.01%	0.001%
57	9.828	2732	2733	2735	rVB2	395	114	0.00%	0.001%
58	9.850	2738	2740	2742	rBV3	457	221	0.01%	0.001%
59	9.870	2742	2746	2749	rBV5	860	875	0.03%	0.004%
60	9.928	2762	2764	2770	rBV3	557	569	0.02%	0.003%
61	9.956	2770	2773	2775	rVV2	700	401	0.02%	0.002%
62	9.973	2775	2778	2784	rVV4	1208	1145	0.04%	0.006%
63	9.998	2784	2786	2788	rVB3	295	122	0.00%	0.001%
64	10.040	2796	2799	2801	rBV2	360	189	0.01%	0.001%
65	10.075	2808	2810	2812	rBV2	411	273	0.01%	0.001%
66	10.146	2820	2832	2859	rBV	620631	996454	37.48%	5.041%
67	10.394	2902	2909	2914	rBV7	3616	5796	0.22%	0.029%
68	10.571	2961	2964	2966	rBV4	631	338	0.01%	0.002%
69	10.612	2975	2977	2979	rVB3	469	154	0.01%	0.001%
70	10.625	2979	2981	2982	rBV	383	145	0.01%	0.001%
71	10.747	3017	3019	3023	rVB3	742	406	0.02%	0.002%
72	10.786	3028	3031	3034	rVB4	1262	795	0.03%	0.004%
73	10.815	3037	3040	3042	rBV	445	206	0.01%	0.001%
74	10.850	3045	3051	3060	rBV3	9705	15811	0.59%	0.080%
75	10.950	3078	3082	3084	rBV2	811	665	0.03%	0.003%
76	11.021	3101	3104	3109	rVB5	932	773	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037691.D
 Acq On : 01 Oct 2024 10:49
 Operator : SY/MD
 Sample : P4185-06DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EY028DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.050	3109	3113	3115	rBV3	331	207	0.01%	0.001%
78	11.082	3121	3123	3126	rVB4	1151	547	0.02%	0.003%
79	11.130	3130	3138	3142	rBV6	2993	4063	0.15%	0.021%
80	11.178	3142	3153	3179	rBV	1121004	1771832	66.64%	8.963%
81	11.551	3258	3269	3300	rBV	1181173	1886401	70.95%	9.542%
82	12.464	3551	3553	3555	rVB2	756	284	0.01%	0.001%
83	12.477	3555	3557	3559	rBV	850	439	0.02%	0.002%
84	12.545	3575	3578	3581	rBV3	821	618	0.02%	0.003%
85	12.738	3636	3638	3641	rBV3	560	373	0.01%	0.002%
86	12.866	3676	3678	3682	rVB3	987	546	0.02%	0.003%
87	12.918	3691	3694	3697	rBV4	610	610	0.02%	0.003%
88	13.011	3718	3723	3725	rBV4	577	471	0.02%	0.002%
89	13.075	3740	3743	3747	rBV3	951	536	0.02%	0.003%
90	13.265	3799	3802	3804	rBV4	1002	472	0.02%	0.002%




Sum of corrected areas: 19768893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037691.D
Acq On : 01 Oct 2024 10:49
Operator : SY/MD
Sample : P4185-06DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY028DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

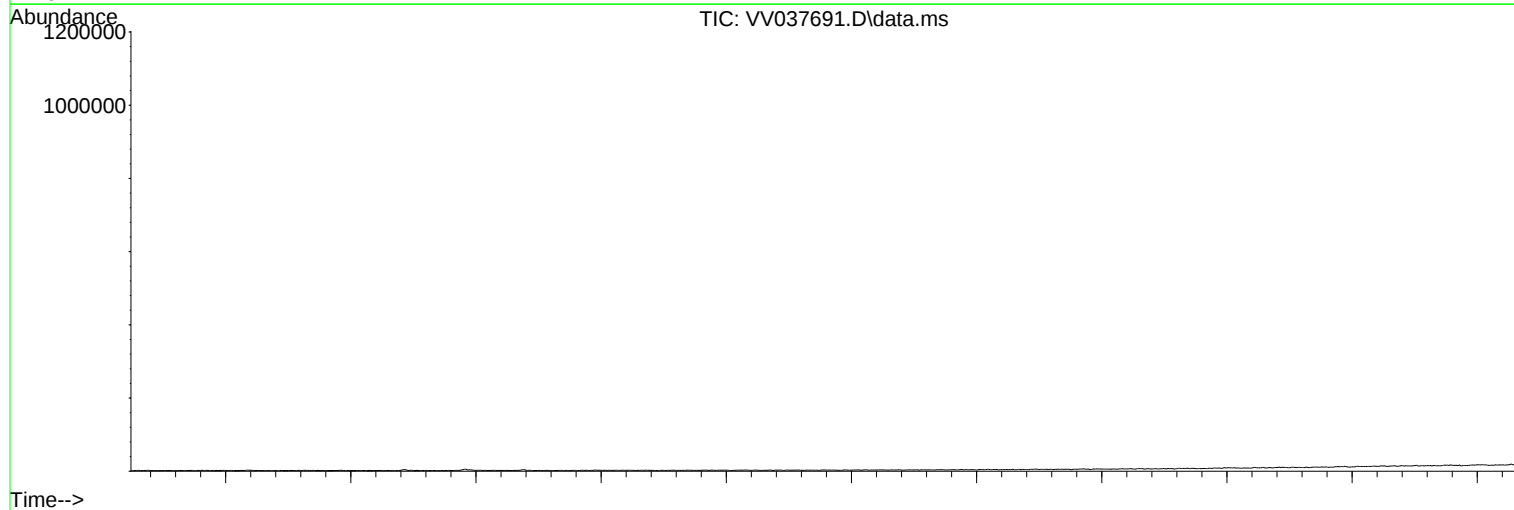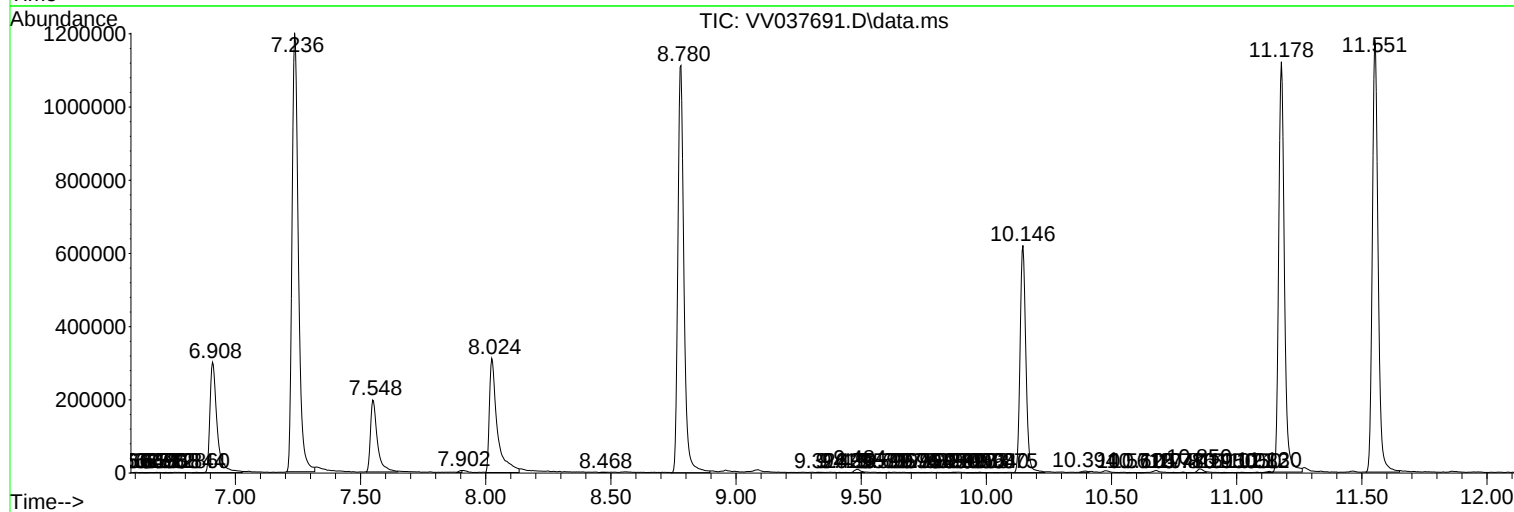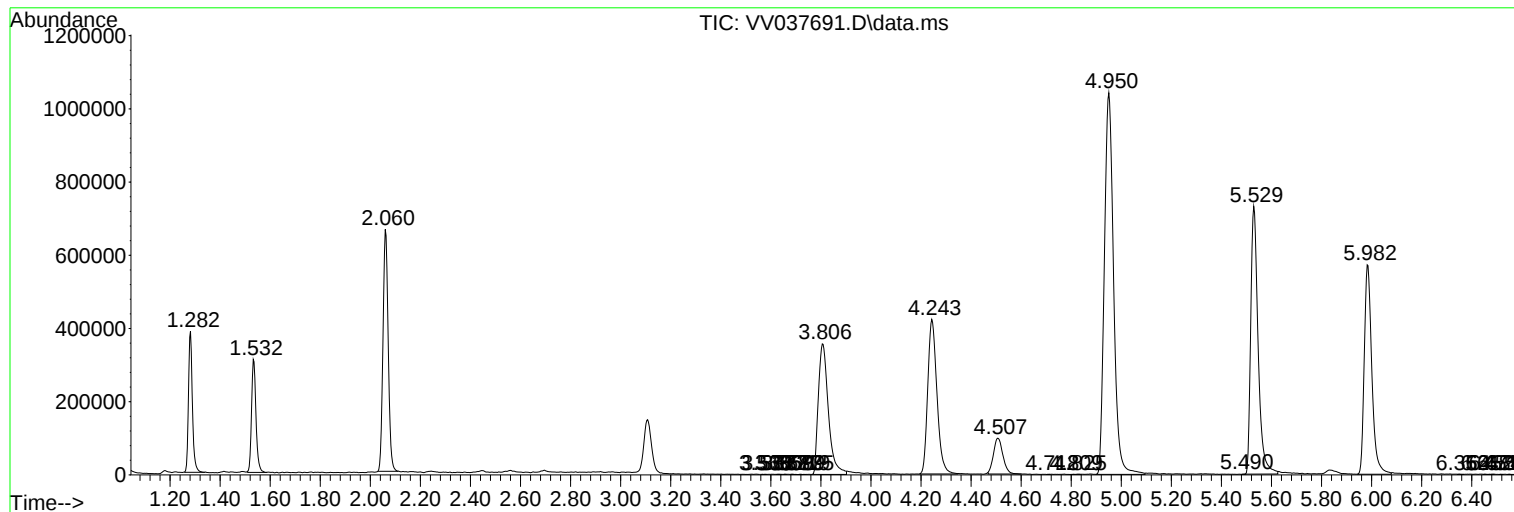

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037691.D
Acq On : 01 Oct 2024 10:49
Operator : SY/MD
Sample : P4185-06DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY028DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037691.D
Acq On : 01 Oct 2024 10:49
Operator : SY/MD
Sample : P4185-06DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EY028DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------