

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037693.D
 Acq On : 01 Oct 2024 11:33
 Operator : SY/MD
 Sample : P4184-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037693.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	38	43	53	rBV2	9812	17389	0.66%	0.092%
2	1.282	68	75	89	rBV	377896	406956	15.37%	2.159%
3	1.536	146	154	179	rVB	310373	375427	14.18%	1.992%
4	2.063	308	318	339	rVB	651029	950032	35.87%	5.040%
5	3.478	756	758	761	rVB2	427	194	0.01%	0.001%
6	3.603	794	797	798	rBV	501	277	0.01%	0.001%
7	3.796	849	857	888	rBV	105724	300927	11.36%	1.596%
8	4.140	961	964	967	rBV5	1165	656	0.02%	0.003%
9	4.246	982	997	1032	rVB	420308	1075110	40.59%	5.703%
10	4.558	1093	1094	1095	rBV	682	191	0.01%	0.001%
11	4.693	1132	1136	1140	rBV3	928	847	0.03%	0.004%
12	4.732	1145	1148	1151	rBV3	627	526	0.02%	0.003%
13	4.764	1155	1158	1160	rBV2	668	475	0.02%	0.003%
14	4.799	1165	1169	1174	rVB4	512	540	0.02%	0.003%
15	4.838	1177	1181	1182	rBV2	478	260	0.01%	0.001%
16	4.851	1182	1185	1188	rVB3	516	257	0.01%	0.001%
17	4.873	1189	1192	1194	rBV4	533	296	0.01%	0.002%
18	4.899	1197	1200	1201	rBV3	1107	591	0.02%	0.003%
19	4.950	1201	1216	1249	rBV2	1034448	2648390	100.00%	14.049%
20	5.532	1385	1397	1437	rBV	727666	1524249	57.55%	8.086%
21	5.986	1526	1538	1565	rBV	579178	1186210	44.79%	6.293%
22	6.359	1651	1654	1656	rBV3	668	393	0.01%	0.002%
23	6.442	1676	1680	1683	rBV5	716	688	0.03%	0.004%
24	6.500	1696	1698	1700	rVB	361	128	0.00%	0.001%
25	6.513	1700	1702	1704	rBV2	648	311	0.01%	0.002%
26	6.539	1708	1710	1712	rVB2	827	324	0.01%	0.002%
27	6.551	1712	1714	1717	rBV2	1156	595	0.02%	0.003%
28	6.571	1717	1720	1721	rBV2	768	382	0.01%	0.002%
29	6.603	1728	1730	1731	rBV	224	85	0.00%	0.000%
30	6.651	1742	1745	1747	rBV4	604	327	0.01%	0.002%
31	6.683	1752	1755	1758	rBV2	641	309	0.01%	0.002%
32	6.699	1758	1760	1764	rBV3	637	435	0.02%	0.002%
33	6.719	1764	1766	1768	rBV3	327	167	0.01%	0.001%
34	6.728	1768	1769	1771	rVB2	469	135	0.01%	0.001%
35	6.751	1774	1776	1778	rVB2	441	184	0.01%	0.001%
36	6.777	1781	1784	1786	rVB2	519	312	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037693.D
 Acq On : 01 Oct 2024 11:33
 Operator : SY/MD
 Sample : P4184-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.789	1786	1788	1792	rBV3	628	473	0.02%	0.003%
38	6.838	1800	1803	1806	rBV2	724	428	0.02%	0.002%
39	6.854	1806	1808	1810	rBV2	802	380	0.01%	0.002%
40	6.908	1814	1825	1854	rBV	300734	580222	21.91%	3.078%
41	7.240	1917	1928	1952	rBV	1204035	2126883	80.31%	11.283%
42	7.551	2016	2025	2056	rBV	197256	370996	14.01%	1.968%
43	7.838	2112	2114	2118	rVB4	1423	642	0.02%	0.003%
44	7.860	2119	2121	2127	rBV5	961	859	0.03%	0.005%
45	8.024	2164	2172	2211	rBV2	322119	696114	26.28%	3.693%
46	8.780	2396	2407	2435	rBV	1131198	1886265	71.22%	10.006%
47	9.236	2547	2549	2552	rBV3	497	269	0.01%	0.001%
48	9.272	2557	2560	2564	rVV4	970	711	0.03%	0.004%
49	9.313	2568	2573	2574	rBV3	775	704	0.03%	0.004%
50	9.378	2587	2593	2597	rBV5	974	946	0.04%	0.005%
51	9.439	2608	2612	2614	rBV2	1085	671	0.03%	0.004%
52	9.516	2634	2636	2639	rBV2	450	294	0.01%	0.002%
53	9.635	2670	2673	2676	rVB3	459	234	0.01%	0.001%
54	9.673	2683	2685	2686	rBV	294	124	0.00%	0.001%
55	9.690	2686	2690	2696	rVV4	725	730	0.03%	0.004%
56	9.744	2704	2707	2709	rBV3	720	357	0.01%	0.002%
57	9.783	2717	2719	2723	rVB3	740	392	0.01%	0.002%
58	9.815	2723	2729	2731	rBV3	498	433	0.02%	0.002%
59	9.860	2741	2743	2744	rBV2	717	218	0.01%	0.001%
60	10.011	2787	2790	2791	rBV3	566	297	0.01%	0.002%
61	10.085	2807	2813	2816	rBV5	770	728	0.03%	0.004%
62	10.146	2820	2832	2860	rBV	634172	1023504	38.65%	5.429%
63	10.464	2929	2931	2932	rBV	558	180	0.01%	0.001%
64	10.577	2963	2966	2969	rVB3	503	339	0.01%	0.002%
65	10.600	2969	2973	2976	rBV3	1033	765	0.03%	0.004%
66	10.751	3015	3020	3022	rBV2	647	494	0.02%	0.003%
67	10.866	3046	3056	3058	rBV6	1112	1403	0.05%	0.007%
68	10.886	3061	3062	3067	rVB2	994	602	0.02%	0.003%
69	10.927	3073	3075	3077	rBV3	526	264	0.01%	0.001%
70	10.960	3082	3085	3088	rBV4	710	512	0.02%	0.003%
71	11.001	3094	3098	3100	rBV3	488	357	0.01%	0.002%
72	11.040	3108	3110	3111	rBV	372	174	0.01%	0.001%
73	11.066	3116	3118	3119	rBV	397	184	0.01%	0.001%
74	11.178	3142	3153	3188	rBV	1113207	1772441	66.93%	9.402%
75	11.551	3257	3269	3296	rBV	1144019	1879984	70.99%	9.973%
76	12.053	3424	3425	3429	rBV2	554	397	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037693.D
Acq On : 01 Oct 2024 11:33
Operator : SY/MD
Sample : P4184-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	12.535	3572	3575	3578	rBV3	547	333	0.01%	0.002%
78	12.667	3614	3616	3618	rBV2	651	317	0.01%	0.002%
79	12.706	3622	3628	3630	rBV3	823	992	0.04%	0.005%
80	12.866	3676	3678	3683	rBV4	672	459	0.02%	0.002%
81	13.014	3721	3724	3726	rBV3	701	415	0.02%	0.002%
82	13.120	3754	3757	3760	rBV	869	595	0.02%	0.003%
83	13.677	3928	3930	3932	rBV3	1289	734	0.03%	0.004%
84	13.770	3958	3959	3963	rBV2	1082	572	0.02%	0.003%




Sum of corrected areas: 18850962

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037693.D
Acq On : 01 Oct 2024 11:33
Operator : SY/MD
Sample : P4184-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

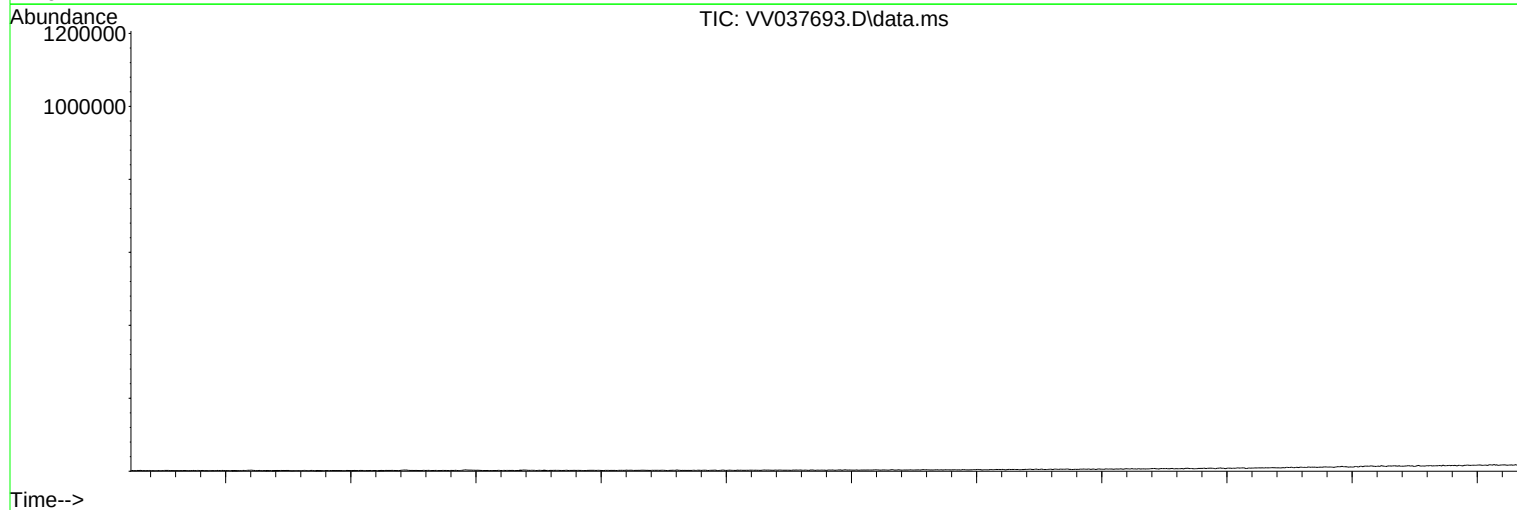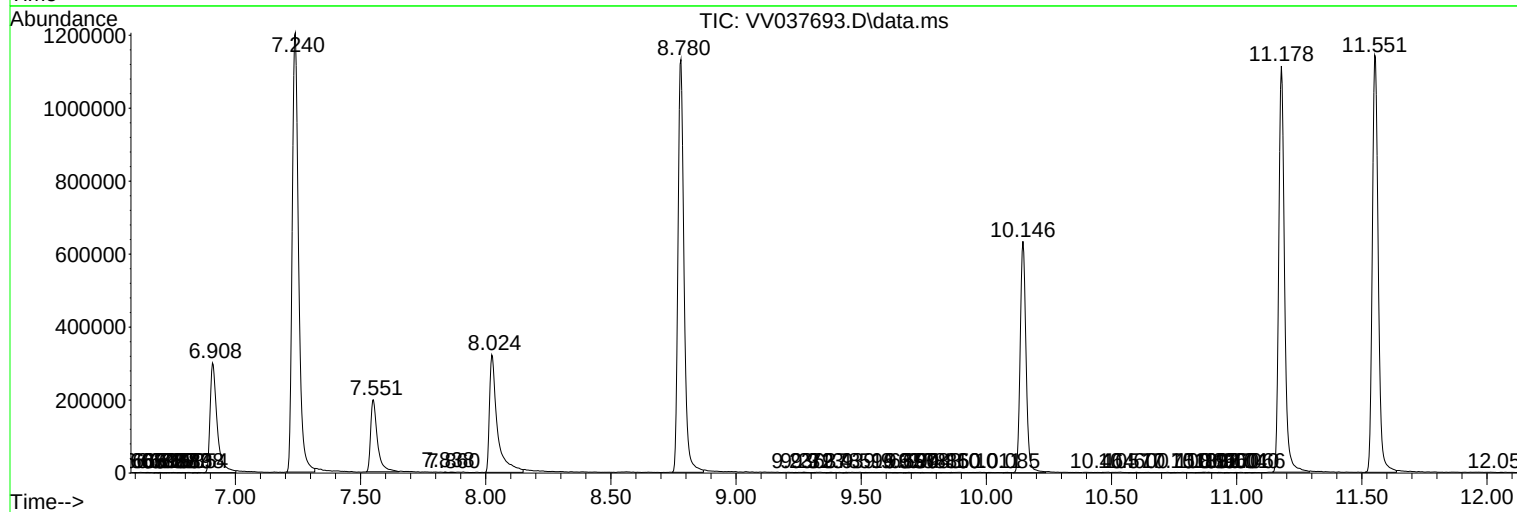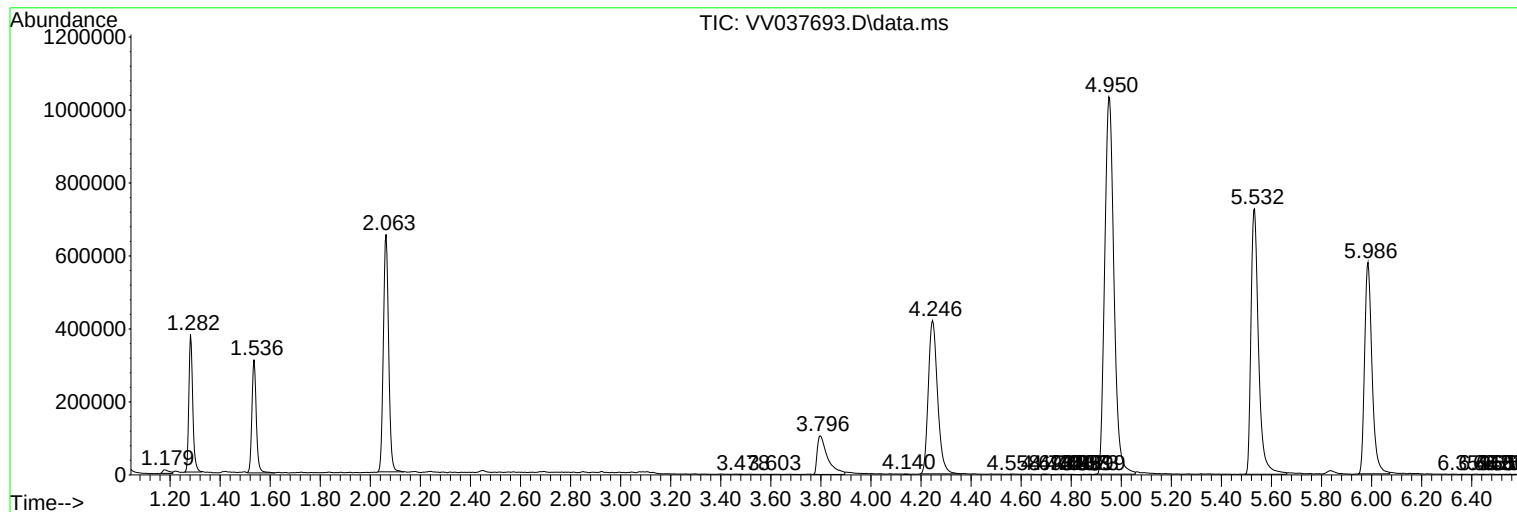

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037693.D
Acq On : 01 Oct 2024 11:33
Operator : SY/MD
Sample : P4184-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037693.D
Acq On : 01 Oct 2024 11:33
Operator : SY/MD
Sample : P4184-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------