

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037694.D
 Acq On : 01 Oct 2024 11:54
 Operator : SY/MD
 Sample : P4228-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	51	rBV	11925	18454	0.72%	0.101%
2	1.282	68	75	93	rVB	359994	392368	15.20%	2.139%
3	1.532	146	153	169	rVB	297359	353981	13.72%	1.930%
4	2.060	307	317	336	rBV	644460	929322	36.01%	5.066%
5	3.539	776	777	780	rVB	517	216	0.01%	0.001%
6	3.555	780	782	784	rBV	649	285	0.01%	0.002%
7	3.642	806	809	811	rBV	587	346	0.01%	0.002%
8	3.670	816	818	823	rVV5	418	347	0.01%	0.002%
9	3.754	840	844	845	rBV2	631	322	0.01%	0.002%
10	3.796	849	857	886	rBV	104756	292409	11.33%	1.594%
11	4.092	947	949	952	rBV4	696	426	0.02%	0.002%
12	4.246	979	997	1030	rBV	413069	1058592	41.02%	5.771%
13	4.558	1091	1094	1095	rBV2	494	263	0.01%	0.001%
14	4.596	1101	1106	1109	rVB4	844	783	0.03%	0.004%
15	4.613	1109	1111	1112	rBV2	481	164	0.01%	0.001%
16	4.674	1128	1130	1131	rBV2	448	218	0.01%	0.001%
17	4.699	1136	1138	1143	rVB3	782	460	0.02%	0.003%
18	4.732	1143	1148	1150	rBV3	830	674	0.03%	0.004%
19	4.780	1158	1163	1164	rBV3	733	588	0.02%	0.003%
20	4.883	1193	1195	1198	rBV2	316	195	0.01%	0.001%
21	4.950	1200	1216	1250	rBV2	1015739	2580849	100.00%	14.069%
22	5.490	1382	1384	1385	rBV	865	413	0.02%	0.002%
23	5.529	1385	1396	1428	rVV	704553	1454398	56.35%	7.928%
24	5.985	1524	1538	1564	rBV	567763	1169442	45.31%	6.375%
25	6.236	1614	1616	1619	rBV4	751	491	0.02%	0.003%
26	6.423	1672	1674	1678	rVB4	501	268	0.01%	0.001%
27	6.558	1714	1716	1717	rBV	361	176	0.01%	0.001%
28	6.638	1738	1741	1742	rBV3	572	309	0.01%	0.002%
29	6.651	1742	1745	1749	rVB4	942	742	0.03%	0.004%
30	6.674	1749	1752	1757	rVB2	698	543	0.02%	0.003%
31	6.696	1757	1759	1761	rBV3	346	174	0.01%	0.001%
32	6.728	1765	1769	1771	rBV4	545	424	0.02%	0.002%
33	6.770	1778	1782	1786	rBV4	652	645	0.02%	0.004%
34	6.821	1794	1798	1799	rVB	441	276	0.01%	0.002%
35	6.838	1799	1803	1806	rVB4	538	345	0.01%	0.002%
36	6.854	1806	1808	1813	rBV2	406	316	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037694.D
 Acq On : 01 Oct 2024 11:54
 Operator : SY/MD
 Sample : P4228-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.908	1815	1825	1855	rBV	295164	567859	22.00%	3.095%
38	7.236	1917	1927	1962	rBV	1173984	2080666	80.62%	11.342%
39	7.551	2016	2025	2047	rBV	194841	358545	13.89%	1.954%
40	8.024	2164	2172	2221	rBV2	319004	703812	27.27%	3.837%
41	8.622	2355	2358	2361	rVB4	992	586	0.02%	0.003%
42	8.638	2361	2363	2365	rBV	847	570	0.02%	0.003%
43	8.741	2391	2395	2396	rBV3	889	628	0.02%	0.003%
44	8.780	2396	2407	2445	rVV	1085999	1825107	70.72%	9.949%
45	9.143	2518	2520	2523	rVB4	1228	521	0.02%	0.003%
46	9.159	2523	2525	2527	rBV3	891	435	0.02%	0.002%
47	9.204	2537	2539	2542	rBV4	1067	734	0.03%	0.004%
48	9.371	2587	2591	2593	rBV3	792	531	0.02%	0.003%
49	9.439	2609	2612	2616	rVB3	380	328	0.01%	0.002%
50	9.461	2616	2619	2622	rBV4	481	281	0.01%	0.002%
51	9.481	2622	2625	2627	rBV3	1016	785	0.03%	0.004%
52	9.548	2642	2646	2649	rBV2	562	470	0.02%	0.003%
53	9.619	2666	2668	2671	rBV3	489	303	0.01%	0.002%
54	9.654	2678	2679	2680	rBV3	565	212	0.01%	0.001%
55	9.690	2688	2690	2693	rBV	515	286	0.01%	0.002%
56	9.747	2705	2708	2709	rBV2	679	316	0.01%	0.002%
57	9.776	2715	2717	2719	rBV	865	345	0.01%	0.002%
58	9.825	2729	2732	2733	rBV2	670	340	0.01%	0.002%
59	9.850	2738	2740	2743	rBV4	509	353	0.01%	0.002%
60	9.873	2743	2747	2749	rBV5	715	511	0.02%	0.003%
61	9.902	2754	2756	2758	rBV2	488	268	0.01%	0.001%
62	9.976	2775	2779	2780	rBV	582	284	0.01%	0.002%
63	9.998	2784	2786	2787	rBV	313	166	0.01%	0.001%
64	10.008	2787	2789	2792	rVB2	660	367	0.01%	0.002%
65	10.024	2792	2794	2798	rBV4	531	331	0.01%	0.002%
66	10.062	2804	2806	2809	rVB2	767	363	0.01%	0.002%
67	10.088	2809	2814	2818	rBV4	718	771	0.03%	0.004%
68	10.146	2820	2832	2855	rBV	630799	1003614	38.89%	5.471%
69	10.345	2890	2894	2895	rBV	592	345	0.01%	0.002%
70	10.374	2900	2903	2905	rVV2	1275	666	0.03%	0.004%
71	10.387	2905	2907	2909	rVB2	938	434	0.02%	0.002%
72	10.432	2919	2921	2923	rBV	812	363	0.01%	0.002%
73	10.471	2931	2933	2935	rBV3	1074	667	0.03%	0.004%
74	10.532	2948	2952	2954	rVB2	617	406	0.02%	0.002%
75	10.548	2955	2957	2959	rBV	657	359	0.01%	0.002%
76	10.657	2988	2991	2993	rBV2	735	476	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037694.D
 Acq On : 01 Oct 2024 11:54
 Operator : SY/MD
 Sample : P4228-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.696	3001	3003	3004	rBV	400	156	0.01%	0.001%
78	10.783	3026	3030	3040	rVB7	1614	2442	0.09%	0.013%
79	10.834	3040	3046	3048	rBV3	985	695	0.03%	0.004%
80	10.902	3065	3067	3070	rVB3	1182	568	0.02%	0.003%
81	10.921	3070	3073	3079	rBV4	639	839	0.03%	0.005%
82	10.956	3082	3084	3086	rBV3	315	175	0.01%	0.001%
83	10.989	3090	3094	3095	rBV	413	294	0.01%	0.002%
84	10.998	3095	3097	3099	rVB2	654	281	0.01%	0.002%
85	11.095	3125	3127	3133	rBV5	601	592	0.02%	0.003%
86	11.127	3133	3137	3138	rBV2	1425	881	0.03%	0.005%
87	11.178	3142	3153	3178	rBV	1053929	1683563	65.23%	9.177%
88	11.551	3258	3269	3297	rBV	1138778	1830720	70.93%	9.980%
89	12.085	3431	3435	3443	rVB7	956	1173	0.05%	0.006%
90	12.300	3497	3502	3504	rBV3	718	755	0.03%	0.004%
91	12.365	3519	3522	3524	rBV2	886	557	0.02%	0.003%
92	12.525	3570	3572	3575	rBV4	775	473	0.02%	0.003%
93	12.599	3590	3595	3602	rVB5	1608	2235	0.09%	0.012%
94	12.628	3602	3604	3612	rBV3	761	855	0.03%	0.005%
95	12.831	3665	3667	3668	rBV	446	167	0.01%	0.001%
96	12.889	3682	3685	3687	rBV3	873	469	0.02%	0.003%
97	13.078	3741	3744	3746	rBV	754	448	0.02%	0.002%
98	13.432	3852	3854	3857	rBV	422	305	0.01%	0.002%
99	13.455	3857	3861	3862	rBV4	1558	1078	0.04%	0.006%
100	13.738	3946	3949	3950	rBV	607	342	0.01%	0.002%

Sum of corrected areas: 18344691




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037694.D
Acq On : 01 Oct 2024 11:54
Operator : SY/MD
Sample : P4228-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

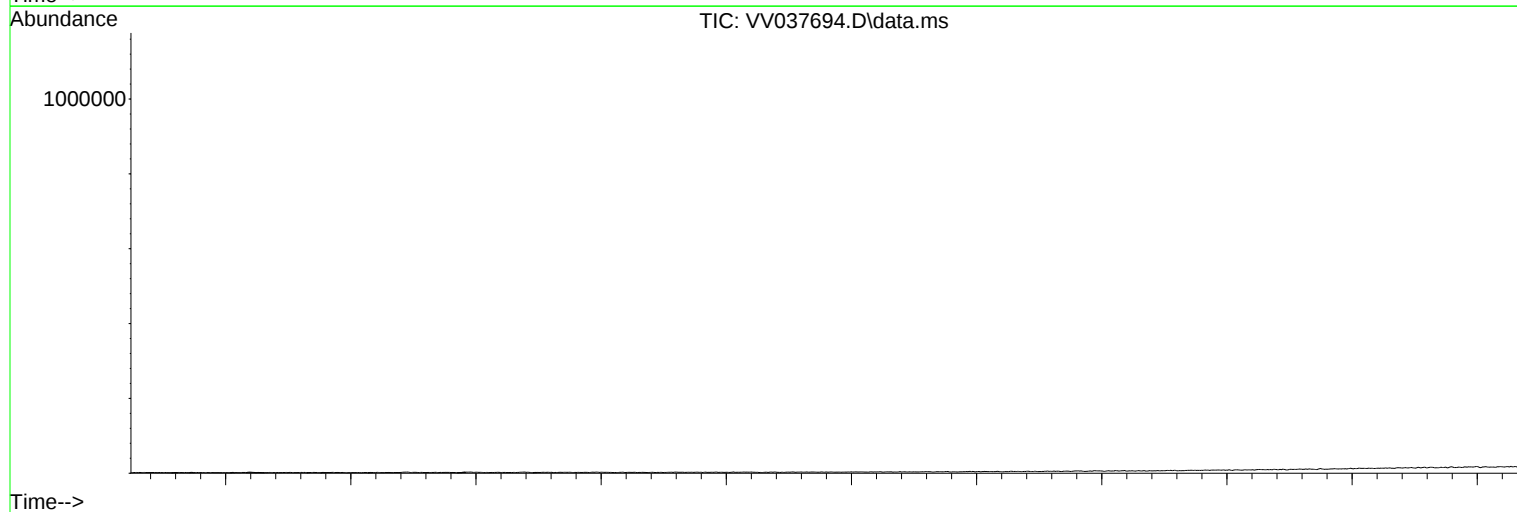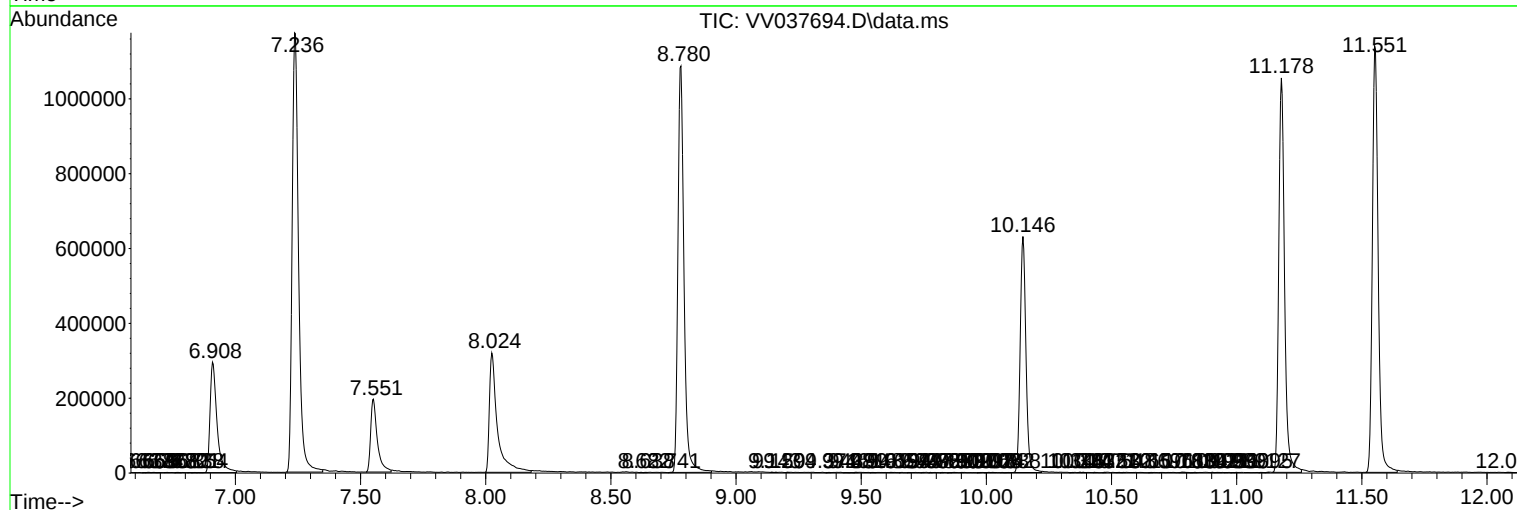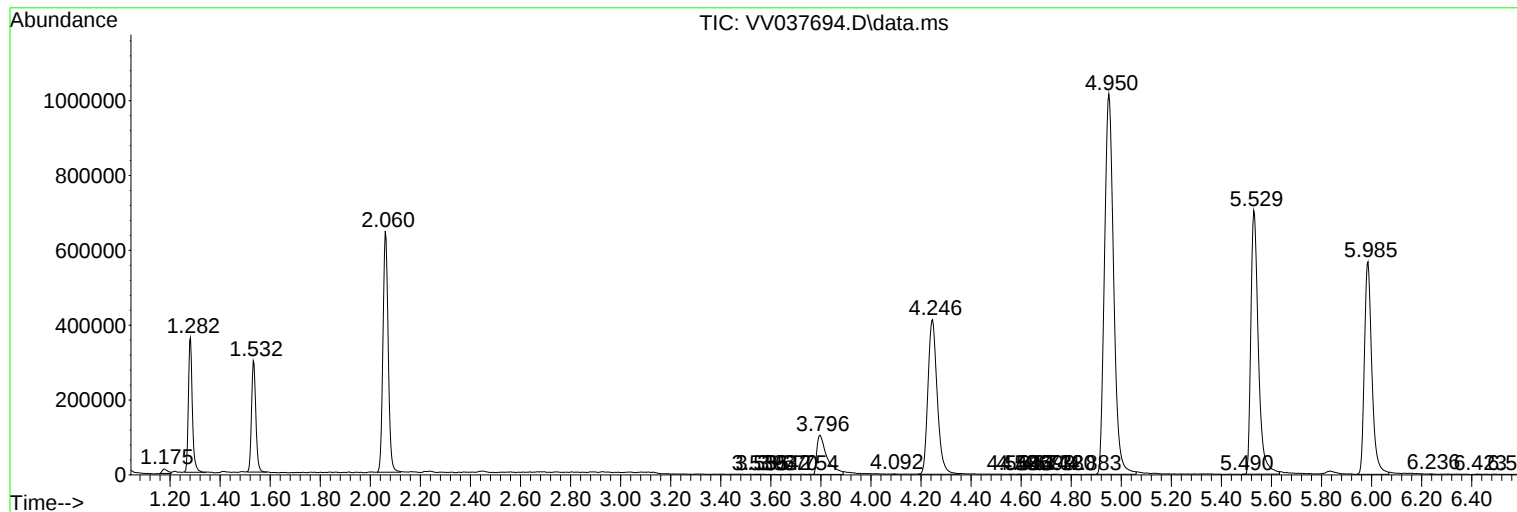

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037694.D
Acq On : 01 Oct 2024 11:54
Operator : SY/MD
Sample : P4228-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037694.D
Acq On : 01 Oct 2024 11:54
Operator : SY/MD
Sample : P4228-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------