

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037698.D
 Acq On : 01 Oct 2024 13:20
 Operator : SY/MD
 Sample : P4203-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037698.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	35	43	52	rBV2	12293	22772	0.93%	0.128%
2	1.278	68	74	90	rVB	337900	370163	15.19%	2.074%
3	1.532	146	153	170	rVB	291113	343554	14.09%	1.925%
4	2.059	307	317	329	rBV	601478	860338	35.29%	4.820%
5	3.336	712	714	717	rBV2	985	650	0.03%	0.004%
6	3.368	722	724	729	rVB5	845	758	0.03%	0.004%
7	3.391	729	731	735	rBV3	702	547	0.02%	0.003%
8	3.796	848	857	894	rBV2	103664	303544	12.45%	1.700%
9	4.021	925	927	931	rBV4	937	654	0.03%	0.004%
10	4.149	963	967	971	rVB3	793	662	0.03%	0.004%
11	4.243	979	996	1028	rBV	392439	993549	40.76%	5.566%
12	4.426	1050	1053	1057	rVB3	1254	786	0.03%	0.004%
13	4.548	1089	1091	1097	rVB6	1036	983	0.04%	0.006%
14	4.580	1097	1101	1102	rBV4	888	579	0.02%	0.003%
15	4.690	1131	1135	1139	rVB3	852	830	0.03%	0.005%
16	4.712	1139	1142	1144	rBV2	1130	801	0.03%	0.004%
17	4.793	1161	1167	1170	rBV3	734	789	0.03%	0.004%
18	4.828	1175	1178	1182	rVB3	864	704	0.03%	0.004%
19	4.950	1200	1216	1247	rBV2	959847	2437581	100.00%	13.655%
20	5.403	1356	1357	1362	rVB3	806	501	0.02%	0.003%
21	5.439	1364	1368	1373	rBV5	711	615	0.03%	0.003%
22	5.529	1385	1396	1429	rBV	707752	1457009	59.77%	8.162%
23	5.831	1480	1490	1503	rBV5	9636	20479	0.84%	0.115%
24	5.915	1513	1516	1519	rVB3	1452	800	0.03%	0.004%
25	5.934	1519	1522	1525	rBV5	1180	879	0.04%	0.005%
26	5.985	1525	1538	1568	rBV	531622	1110337	45.55%	6.220%
27	6.149	1584	1589	1592	rBV7	2081	1782	0.07%	0.010%
28	6.288	1628	1632	1635	rVB5	828	741	0.03%	0.004%
29	6.320	1640	1642	1649	rVB6	952	741	0.03%	0.004%
30	6.355	1649	1653	1655	rBV3	778	564	0.02%	0.003%
31	6.551	1712	1714	1718	rVV5	695	590	0.02%	0.003%
32	6.606	1724	1731	1734	rVB5	673	628	0.03%	0.004%
33	6.908	1815	1825	1859	rBV	277324	538541	22.09%	3.017%
34	7.130	1890	1894	1900	rVB5	1188	1131	0.05%	0.006%
35	7.185	1909	1911	1915	rVB5	1035	691	0.03%	0.004%
36	7.239	1916	1928	1955	rBV	1086417	1935484	79.40%	10.842%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037698.D
 Acq On : 01 Oct 2024 13:20
 Operator : SY/MD
 Sample : P4203-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.551	2016	2025	2053	rVV	184551	350535	14.38%	1.964%
38	7.754	2085	2088	2093	rVB4	966	908	0.04%	0.005%
39	7.911	2134	2137	2142	rVB8	861	772	0.03%	0.004%
40	7.979	2152	2158	2164	rBV3	6042	8096	0.33%	0.045%
41	8.024	2164	2172	2210	rVV2	308312	657471	26.97%	3.683%
42	8.558	2334	2338	2343	rVB6	1244	1138	0.05%	0.006%
43	8.648	2359	2366	2368	rVV7	1138	1353	0.06%	0.008%
44	8.738	2390	2394	2396	rBV3	1136	962	0.04%	0.005%
45	8.780	2396	2407	2432	rBV	1102857	1817196	74.55%	10.180%
46	9.014	2477	2480	2485	rBV8	905	843	0.03%	0.005%
47	9.223	2538	2545	2553	rBV10	5163	9834	0.40%	0.055%
48	9.397	2596	2599	2602	rBV3	815	600	0.02%	0.003%
49	9.455	2613	2617	2620	rVB3	726	510	0.02%	0.003%
50	9.484	2624	2626	2630	rBV2	817	672	0.03%	0.004%
51	9.532	2638	2641	2644	rVB3	637	528	0.02%	0.003%
52	9.551	2644	2647	2651	rBV3	1250	908	0.04%	0.005%
53	9.715	2691	2698	2709	rVB10	5356	9149	0.38%	0.051%
54	9.763	2709	2713	2715	rBV4	1111	842	0.03%	0.005%
55	9.796	2719	2723	2724	rBV2	868	549	0.02%	0.003%
56	9.889	2741	2752	2762	rBV10	10875	18621	0.76%	0.104%
57	10.050	2799	2802	2806	rVB4	1210	897	0.04%	0.005%
58	10.146	2819	2832	2853	rBV	604577	958338	39.32%	5.369%
59	10.313	2880	2884	2886	rBV3	846	670	0.03%	0.004%
60	10.493	2936	2940	2946	rVB7	1221	1257	0.05%	0.007%
61	10.529	2949	2951	2955	rVB3	1242	729	0.03%	0.004%
62	10.564	2955	2962	2967	rBV7	3220	4588	0.19%	0.026%
63	10.638	2978	2985	2994	rVB8	3640	5397	0.22%	0.030%
64	10.863	3052	3055	3058	rBV6	655	612	0.03%	0.003%
65	10.924	3070	3074	3078	rBV5	611	730	0.03%	0.004%
66	10.988	3086	3094	3100	rBV8	2463	3569	0.15%	0.020%
67	11.046	3108	3112	3116	rBV5	1155	1068	0.04%	0.006%
68	11.123	3126	3136	3143	rBV7	11645	18592	0.76%	0.104%
69	11.178	3143	3153	3184	rVV	1090879	1726725	70.84%	9.673%
70	11.503	3248	3254	3256	rVV6	4661	4776	0.20%	0.027%
71	11.554	3259	3270	3304	rVB	1091960	1762869	72.32%	9.875%
72	11.834	3350	3357	3360	rBV8	3675	4568	0.19%	0.026%
73	11.953	3384	3394	3405	rBV10	4411	8725	0.36%	0.049%
74	12.191	3462	3468	3470	rBV6	947	910	0.04%	0.005%
75	12.252	3480	3487	3489	rBV7	1697	1752	0.07%	0.010%
76	12.303	3500	3503	3506	rVB4	1277	918	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037698.D
 Acq On : 01 Oct 2024 13:20
 Operator : SY/MD
 Sample : P4203-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.545	3573	3578	3582	rBV6	1069	1050	0.04%	0.006%
78	12.583	3585	3590	3591	rBV4	1849	1485	0.06%	0.008%
79	12.680	3615	3620	3624	rVB8	1429	1142	0.05%	0.006%
80	12.709	3626	3629	3630	rBV4	774	504	0.02%	0.003%
81	12.879	3680	3682	3685	rVV3	748	583	0.02%	0.003%
82	12.947	3701	3703	3706	rBV2	904	618	0.03%	0.003%
83	13.033	3726	3730	3734	rVB4	906	648	0.03%	0.004%
84	13.146	3762	3765	3767	rBV3	759	512	0.02%	0.003%
85	13.307	3811	3815	3817	rBV4	970	550	0.02%	0.003%
86	13.455	3853	3861	3869	rBV4	4317	7391	0.30%	0.041%
87	13.580	3893	3900	3904	rVB5	1246	1631	0.07%	0.009%
88	13.606	3904	3908	3912	rVB5	1483	1225	0.05%	0.007%
89	13.683	3922	3932	3935	rBV8	4152	5456	0.22%	0.031%
90	13.715	3941	3942	3949	rVB7	969	813	0.03%	0.005%
91	13.946	4011	4014	4015	rBV3	931	547	0.02%	0.003%
92	14.085	4055	4057	4059	rVB3	1788	722	0.03%	0.004%
93	14.110	4059	4065	4068	rBV6	1103	1323	0.05%	0.007%
94	14.345	4127	4138	4147	rBV6	6020	10501	0.43%	0.059%
95	14.381	4147	4149	4155	rVB5	1894	995	0.04%	0.006%
96	14.455	4170	4172	4175	rBV2	916	527	0.02%	0.003%
97	14.474	4175	4178	4180	rBV3	948	585	0.02%	0.003%
98	14.532	4191	4196	4207	rVB9	2346	3550	0.15%	0.020%
99	14.586	4207	4213	4216	rBV8	2525	3041	0.12%	0.017%
100	15.053	4353	4358	4363	rVV6	3981	4740	0.19%	0.027%

Sum of corrected areas: 17851073




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037698.D
Acq On : 01 Oct 2024 13:20
Operator : SY/MD
Sample : P4203-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

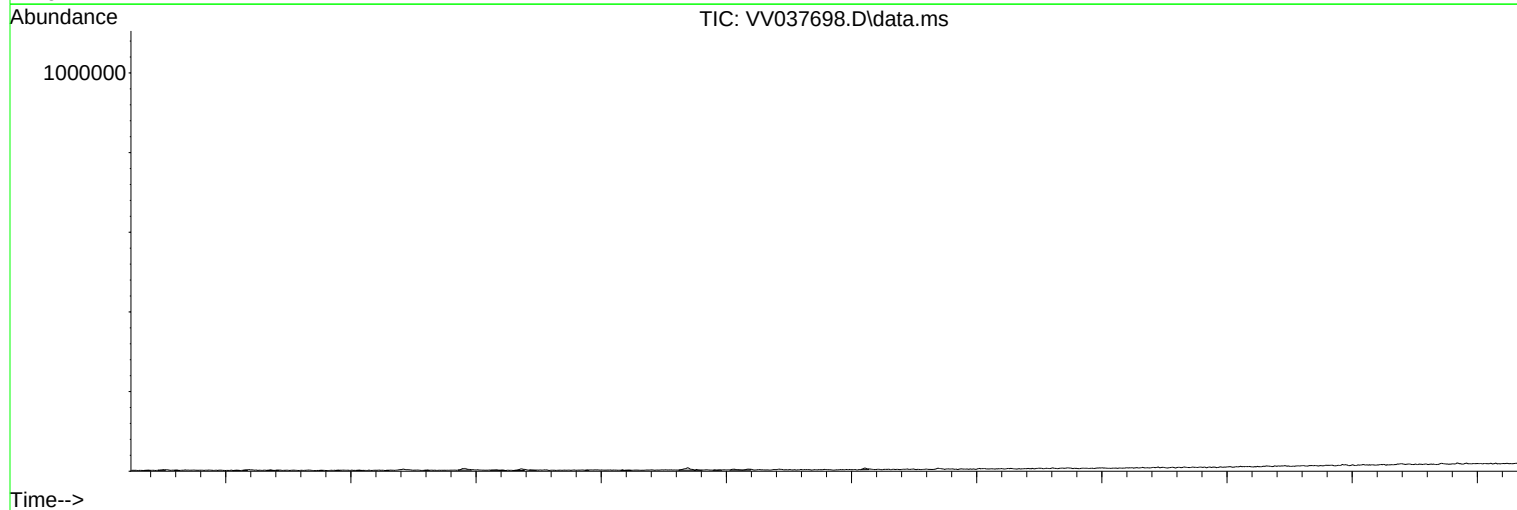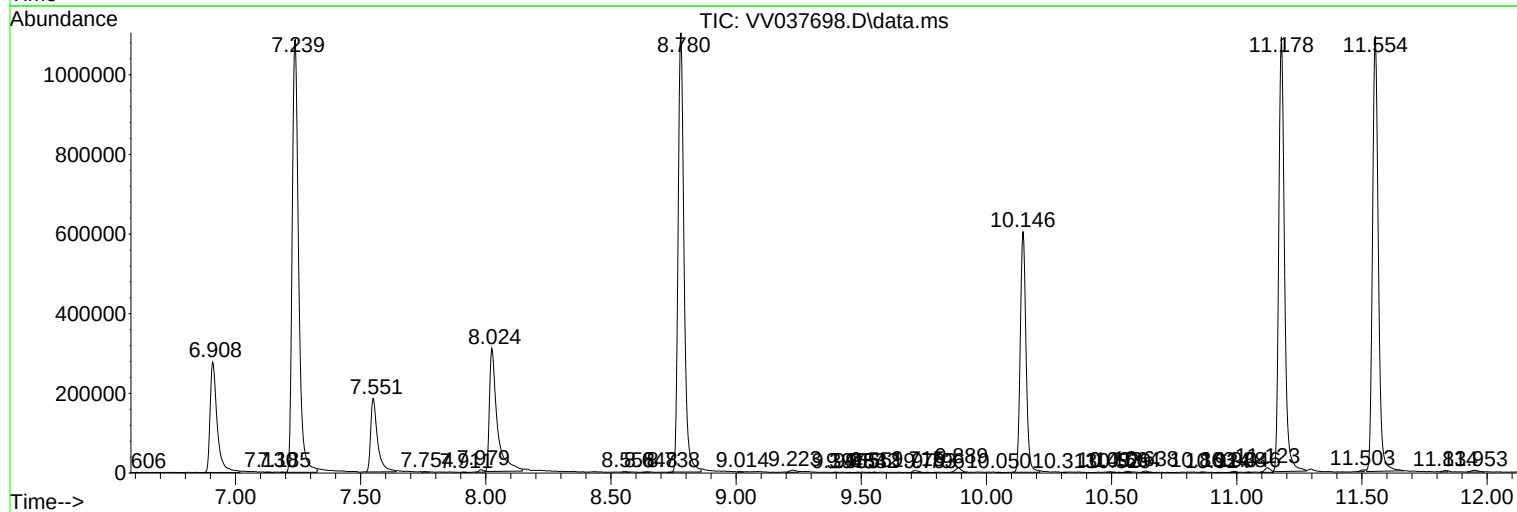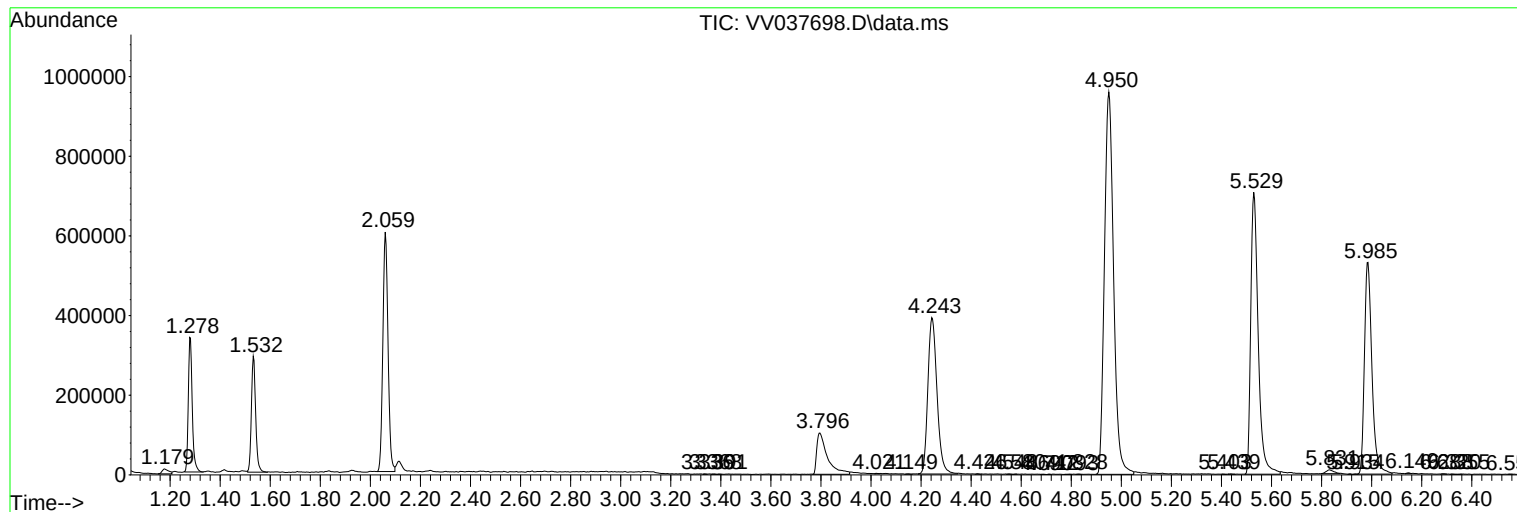

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037698.D
Acq On : 01 Oct 2024 13:20
Operator : SY/MD
Sample : P4203-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037698.D
Acq On : 01 Oct 2024 13:20
Operator : SY/MD
Sample : P4203-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FC4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
