

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037700.D
 Acq On : 01 Oct 2024 14:13
 Operator : SY/MD
 Sample : P4237-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037700.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.176	37	42	51	rBV	10961	17597	0.73%	0.103%
2	1.282	68	75	91	rVB	258056	282346	11.65%	1.659%
3	1.532	146	153	167	rVB	248267	292615	12.07%	1.719%
4	2.060	308	317	328	rBV	501010	714951	29.50%	4.200%
5	3.446	746	748	751	rBV3	606	320	0.01%	0.002%
6	3.561	781	784	787	rBV5	486	375	0.02%	0.002%
7	3.600	793	796	800	rVB5	596	412	0.02%	0.002%
8	3.664	814	816	819	rVB3	611	339	0.01%	0.002%
9	3.680	819	821	822	rBV	591	221	0.01%	0.001%
10	3.690	822	824	828	rVB3	488	294	0.01%	0.002%
11	3.754	841	844	846	rBV2	568	297	0.01%	0.002%
12	3.793	848	856	899	rBV	116529	376278	15.53%	2.210%
13	4.243	982	996	1023	rBV	402008	1008448	41.61%	5.924%
14	4.680	1130	1132	1133	rBV	320	172	0.01%	0.001%
15	4.780	1160	1163	1165	rBV4	383	168	0.01%	0.001%
16	4.806	1168	1171	1172	rBV4	440	245	0.01%	0.001%
17	4.825	1175	1177	1179	rBV2	365	191	0.01%	0.001%
18	4.838	1179	1181	1184	rVB2	523	254	0.01%	0.001%
19	4.857	1185	1187	1190	rBV3	524	339	0.01%	0.002%
20	4.950	1199	1216	1249	rBV2	944774	2423440	100.00%	14.236%
21	5.436	1364	1367	1369	rBV3	887	582	0.02%	0.003%
22	5.529	1385	1396	1422	rBV	604379	1252957	51.70%	7.360%
23	5.986	1525	1538	1565	rBV	544301	1131921	46.71%	6.649%
24	6.330	1643	1645	1648	rBV4	847	399	0.02%	0.002%
25	6.388	1659	1663	1667	rVB6	803	684	0.03%	0.004%
26	6.545	1709	1712	1713	rBV2	631	355	0.01%	0.002%
27	6.580	1721	1723	1728	rVB3	1154	689	0.03%	0.004%
28	6.606	1728	1731	1732	rBV2	547	226	0.01%	0.001%
29	6.616	1732	1734	1736	rVB	707	285	0.01%	0.002%
30	6.629	1736	1738	1741	rBV4	1108	749	0.03%	0.004%
31	6.699	1757	1760	1761	rBV2	447	226	0.01%	0.001%
32	6.770	1778	1782	1784	rBV4	911	778	0.03%	0.005%
33	6.802	1789	1792	1796	rVB6	714	591	0.02%	0.003%
34	6.841	1801	1804	1807	rBV4	400	271	0.01%	0.002%
35	6.863	1807	1811	1815	rBV3	605	495	0.02%	0.003%
36	6.908	1815	1825	1857	rBV	286087	559714	23.10%	3.288%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
 Data File : VV037700.D
 Acq On : 01 Oct 2024 14:13
 Operator : SY/MD
 Sample : P4237-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4EB9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.236	1917	1927	1956	rBV	1058882	1875485	77.39%	11.017%
38	7.548	2016	2024	2056	rBV	189596	358591	14.80%	2.107%
39	7.908	2133	2136	2140	rBV5	1843	1682	0.07%	0.010%
40	8.024	2163	2172	2212	rBV2	336696	733122	30.25%	4.307%
41	8.719	2385	2388	2389	rBV3	910	401	0.02%	0.002%
42	8.780	2395	2407	2432	rBV	950080	1575691	65.02%	9.256%
43	9.291	2564	2566	2569	rBV3	781	554	0.02%	0.003%
44	9.362	2585	2588	2590	rBV4	638	472	0.02%	0.003%
45	9.420	2604	2606	2607	rBV2	498	171	0.01%	0.001%
46	9.455	2614	2617	2618	rBV2	766	450	0.02%	0.003%
47	9.567	2650	2652	2653	rBV	870	351	0.01%	0.002%
48	9.593	2658	2660	2661	rBV2	748	214	0.01%	0.001%
49	9.625	2668	2670	2671	rBV2	624	271	0.01%	0.002%
50	9.667	2679	2683	2686	rBV5	1168	980	0.04%	0.006%
51	9.767	2710	2714	2717	rBV5	854	722	0.03%	0.004%
52	9.889	2745	2752	2762	rBV9	3762	6457	0.27%	0.038%
53	9.973	2773	2778	2781	rVB4	1029	1012	0.04%	0.006%
54	9.989	2781	2783	2785	rBV2	792	464	0.02%	0.003%
55	10.047	2799	2801	2804	rVB3	631	280	0.01%	0.002%
56	10.066	2804	2807	2809	rBV2	358	198	0.01%	0.001%
57	10.095	2813	2816	2818	rBV3	949	467	0.02%	0.003%
58	10.146	2818	2832	2854	rBV	673713	1062449	43.84%	6.241%
59	10.358	2894	2898	2899	rBV4	1052	658	0.03%	0.004%
60	10.612	2973	2977	2978	rBV3	905	589	0.02%	0.003%
61	10.870	3049	3057	3065	rVB9	1134	1880	0.08%	0.011%
62	10.902	3065	3067	3070	rBV2	586	314	0.01%	0.002%
63	10.940	3075	3079	3081	rBV2	432	317	0.01%	0.002%
64	11.082	3121	3123	3124	rBV	301	80	0.00%	0.000%
65	11.120	3129	3135	3136	rBV6	2355	2100	0.09%	0.012%
66	11.178	3143	3153	3181	rBV	913507	1473626	60.81%	8.657%
67	11.551	3259	3269	3301	rVB	1138158	1837063	75.80%	10.792%
68	12.300	3491	3502	3509	rBV	4585	9016	0.37%	0.053%
69	12.590	3585	3592	3595	rBV5	1983	2419	0.10%	0.014%
70	12.979	3711	3713	3715	rBV3	956	448	0.02%	0.003%
71	13.127	3755	3759	3763	rBV5	897	884	0.04%	0.005%
72	13.448	3854	3859	3860	rBV4	2293	1771	0.07%	0.010%
73	14.329	4129	4133	4134	rBV3	1549	1112	0.05%	0.007%

Sum of corrected areas: 17022985




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037700.D
Acq On : 01 Oct 2024 14:13
Operator : SY/MD
Sample : P4237-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

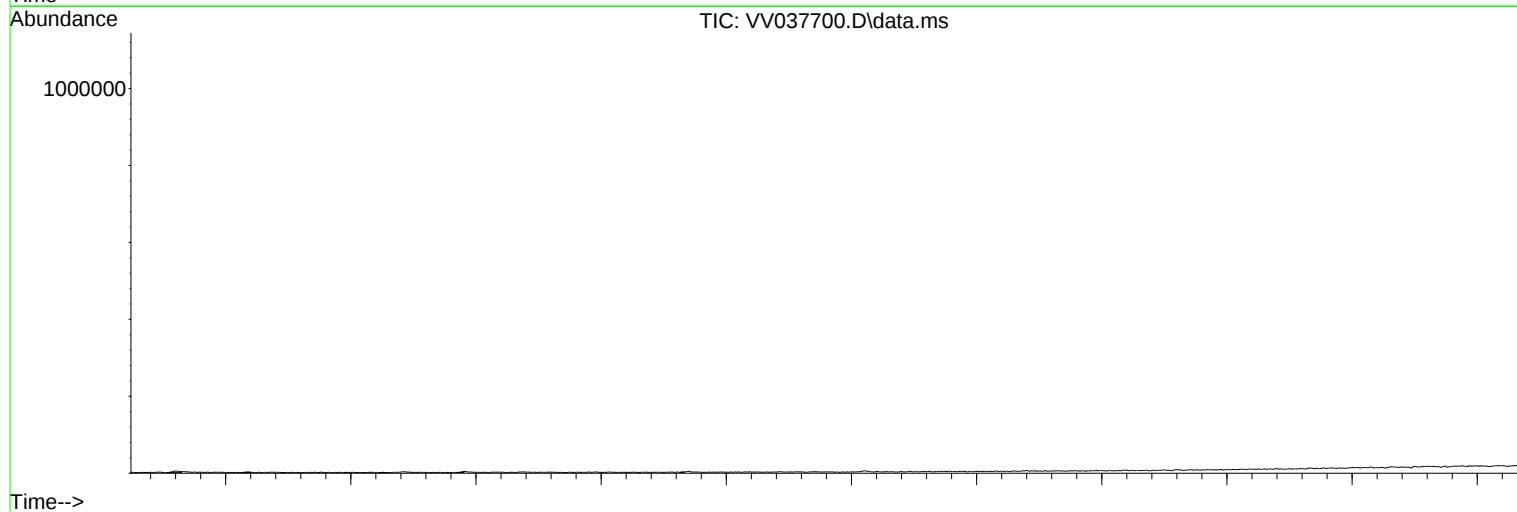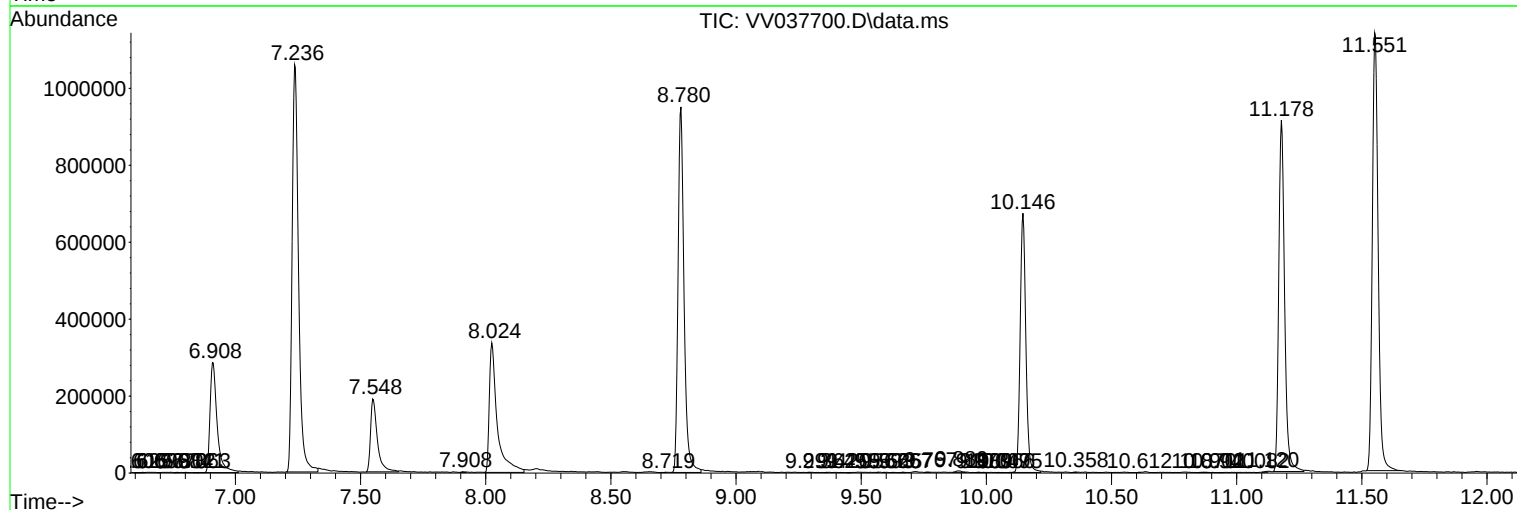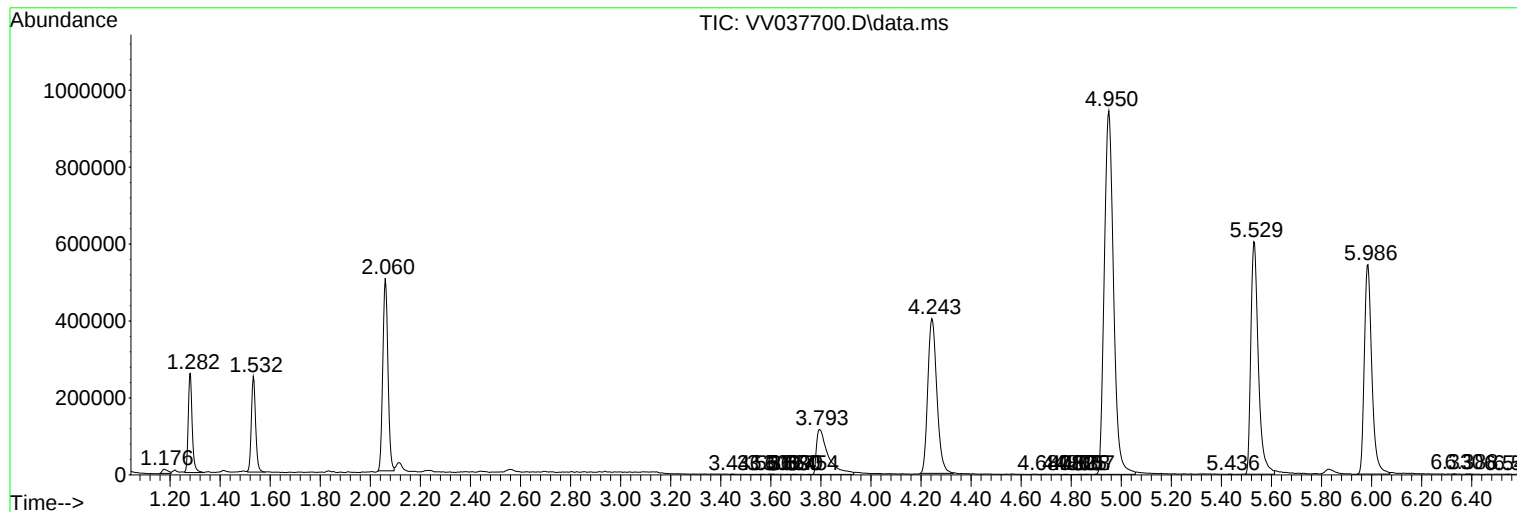

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037700.D
Acq On : 01 Oct 2024 14:13
Operator : SY/MD
Sample : P4237-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100124\
Data File : VV037700.D
Acq On : 01 Oct 2024 14:13
Operator : SY/MD
Sample : P4237-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4EB9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------